

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052096.D
 Acq On : 20 Jan 2022 16:53
 Operator : CG/JU
 Sample : PB142154BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK154

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.582	11	16	23	rVB2	6946	11560	1.37%	0.137%
2	4.005	83	88	100	rBV	91120	159071	18.89%	1.880%
3	4.363	146	149	151	rBV2	1886	1848	0.22%	0.022%
4	4.492	168	171	174	rBV	1060	1425	0.17%	0.017%
5	7.400	659	666	675	rBV2	128208	216179	25.67%	2.555%
6	7.565	688	694	705	rVB	84325	143400	17.03%	1.695%
7	7.788	724	732	741	rBV	114966	197419	23.44%	2.333%
8	8.258	804	812	820	rBB	91773	157124	18.66%	1.857%
9	8.963	923	932	940	rBV	150673	264510	31.41%	3.126%
10	9.433	1003	1012	1020	rBV	120828	212230	25.20%	2.508%
11	10.161	1127	1136	1143	rBV	102383	182111	21.63%	2.152%
12	10.708	1222	1229	1238	rBV	149916	273035	32.42%	3.227%
13	11.095	1288	1295	1306	rVB	131556	234832	27.89%	2.776%
14	11.219	1308	1316	1329	rVV	148291	268235	31.85%	3.170%
15	12.670	1558	1563	1566	rBV2	2037	3471	0.41%	0.041%
16	14.285	1831	1838	1845	rVB	294972	422630	50.19%	4.995%
17	14.590	1883	1890	1899	rBV	328556	516157	61.29%	6.101%
18	14.896	1936	1942	1949	rVB	235457	352467	41.86%	4.166%
19	15.072	1966	1972	1987	rBV	114800	205612	24.42%	2.430%
20	15.883	2102	2110	2118	rBV	417522	634013	75.29%	7.494%
21	15.989	2123	2128	2137	rBV	106735	164656	19.55%	1.946%
22	16.130	2148	2152	2157	rBV2	1731	2926	0.35%	0.035%
23	17.428	2368	2373	2377	rBV2	1485	2398	0.28%	0.028%
24	17.645	2403	2410	2416	rBV	296838	448966	53.32%	5.307%
25	17.745	2419	2427	2434	rBV	481390	718973	85.38%	8.498%
26	19.584	2735	2740	2744	rBV3	6469	9341	1.11%	0.110%
27	19.660	2748	2753	2759	rVV2	6496	9514	1.13%	0.112%
28	19.960	2800	2804	2807	rBV5	1063	1887	0.22%	0.022%
29	20.018	2807	2814	2822	rBV	597136	842089	100.00%	9.953%
30	20.130	2831	2833	2836	rBV3	1700	1299	0.15%	0.015%
31	20.336	2867	2868	2871	rBV4	1807	1624	0.19%	0.019%
32	20.947	2971	2972	2973	rBV	2499	1640	0.19%	0.019%
33	21.105	2997	2999	3000	rBV2	2122	1378	0.16%	0.016%
34	21.963	3138	3145	3153	rVB	273896	485212	57.62%	5.735%
35	22.791	3284	3286	3287	rBV2	2933	2544	0.30%	0.030%
36	25.211	3687	3698	3711	rVB	281505	800241	95.03%	9.459%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052096.D
Acq On : 20 Jan 2022 16:53
Operator : CG/JU
Sample : PB142154BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK154

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

37	25.452	3728	3739	3754	rVB2	161767	495603	58.85%	5.858%
38	26.010	3832	3834	3835	rBV2	3146	1403	0.17%	0.017%
39	28.061	4181	4183	4186	rBV3	2589	1250	0.15%	0.015%
40	28.102	4188	4190	4191	rBV2	2472	1384	0.16%	0.016%
41	28.495	4255	4257	4260	rVB3	2976	2976	0.35%	0.035%
42	31.103	4699	4701	4702	rVB2	2574	1153	0.14%	0.014%
43	31.979	4848	4850	4851	rBV2	2786	2378	0.28%	0.028%
44	32.014	4854	4856	4859	rVV3	2455	2328	0.28%	0.028%




Sum of corrected areas: 8460492

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052096.D
Acq On : 20 Jan 2022 16:53
Operator : CG/JU
Sample : PB142154BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

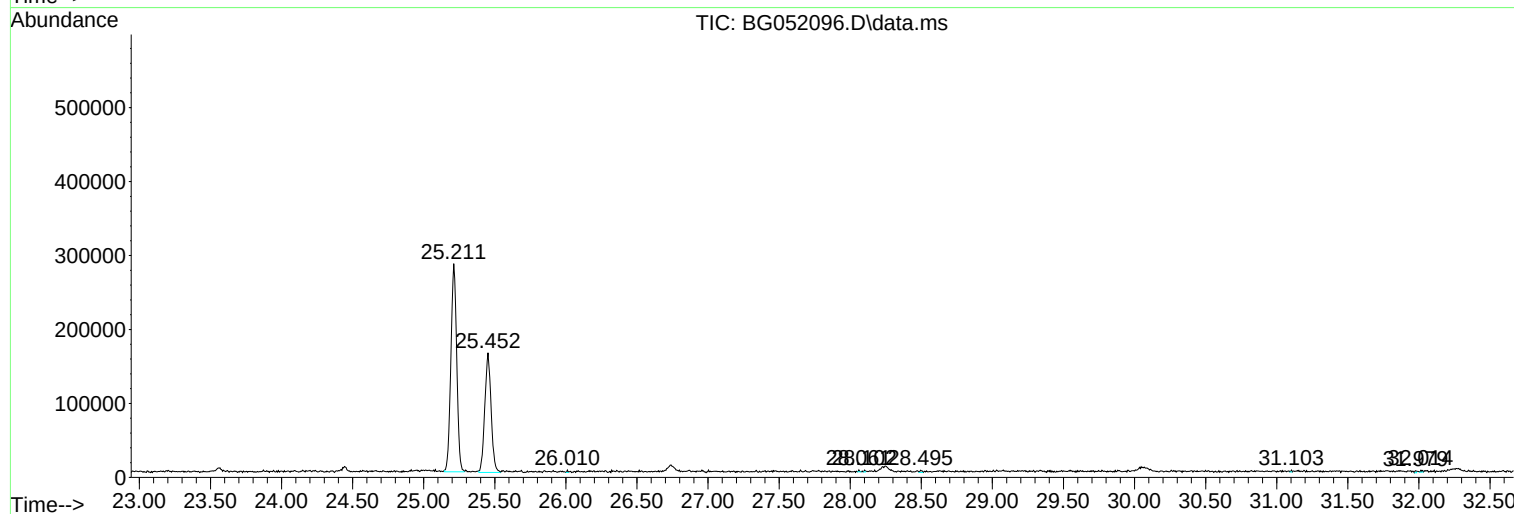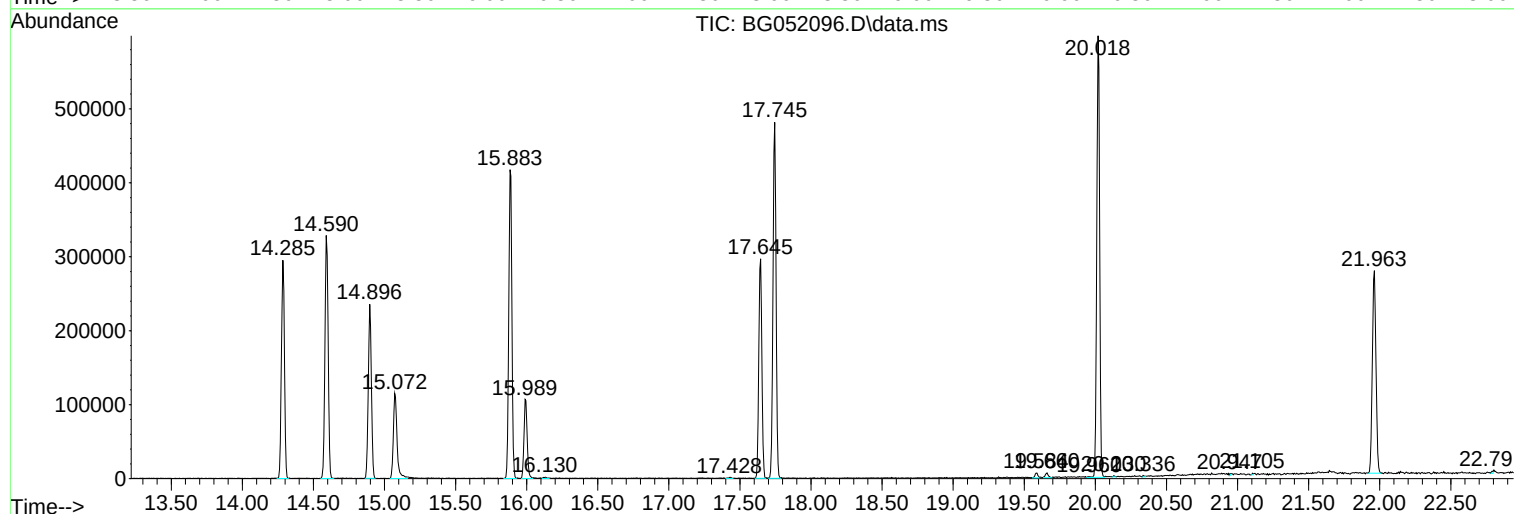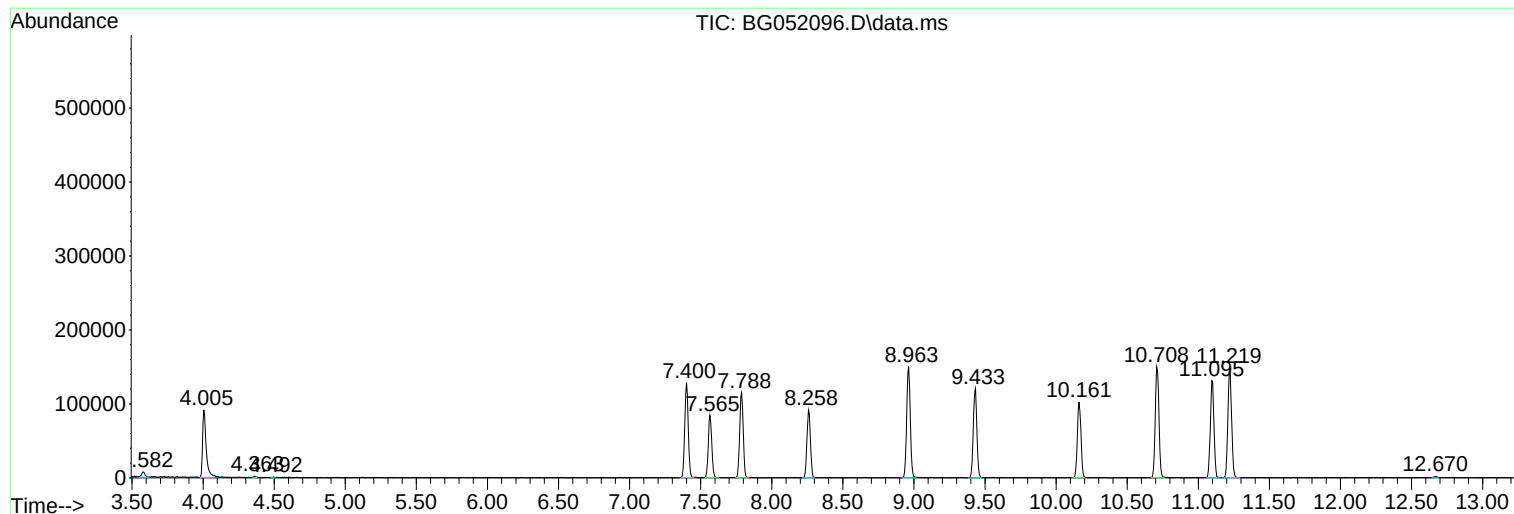

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052096.D
Acq On : 20 Jan 2022 16:53
Operator : CG/JU
Sample : PB142154BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052096.D
Acq On : 20 Jan 2022 16:53
Operator : CG/JU
Sample : PB142154BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc