

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052104.D
 Acq On : 20 Jan 2022 22:32
 Operator : CG/JU
 Sample : PB142157BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK157

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.573	8	14	20	rBV	7631	12323	1.34%	0.130%
2	3.655	26	28	32	rVB	1213	1284	0.14%	0.013%
3	3.996	81	86	98	rBV	96528	167276	18.25%	1.758%
4	4.354	141	147	153	rBV4	2518	4658	0.51%	0.049%
5	7.380	656	662	670	rBV	136226	237593	25.93%	2.497%
6	7.550	684	691	700	rVB	92488	157765	17.22%	1.658%
7	7.767	720	728	736	rBB	125164	219736	23.98%	2.309%
8	8.243	802	809	816	rVB	108337	182233	19.89%	1.915%
9	8.942	921	928	939	rVB	168538	292390	31.91%	3.073%
10	9.412	1000	1008	1018	rBV	135313	238569	26.03%	2.507%
11	10.146	1124	1133	1140	rBV2	119696	213431	23.29%	2.243%
12	10.693	1218	1226	1239	rBV	176793	317511	34.65%	3.337%
13	11.080	1285	1292	1301	rVB	160945	279116	30.46%	2.934%
14	11.204	1306	1313	1321	rBV	165652	304156	33.19%	3.197%
15	12.655	1553	1560	1563	rBV3	2528	4618	0.50%	0.049%
16	14.276	1829	1836	1843	rBV	344188	499794	54.54%	5.253%
17	14.582	1880	1888	1895	rBV	370879	583190	63.64%	6.129%
18	14.887	1933	1940	1946	rBV	276756	421826	46.03%	4.433%
19	15.063	1964	1970	1985	rBV3	129618	233359	25.46%	2.453%
20	15.874	2102	2108	2117	rVB	462995	714418	77.96%	7.509%
21	15.980	2120	2126	2136	rBV	119790	186602	20.36%	1.961%
22	16.115	2146	2149	2153	rVB2	2666	3017	0.33%	0.032%
23	17.354	2355	2360	2364	rBV	1014	1377	0.15%	0.014%
24	17.419	2368	2371	2375	rVB2	1078	1552	0.17%	0.016%
25	17.636	2400	2408	2417	rBV	345520	519414	56.68%	5.459%
26	17.736	2418	2425	2433	rVB	527933	785626	85.73%	8.257%
27	19.440	2711	2715	2717	rVB3	876	1275	0.14%	0.013%
28	19.534	2728	2731	2732	rBV2	1451	1309	0.14%	0.014%
29	19.581	2735	2739	2743	rVV3	7011	9388	1.02%	0.099%
30	19.651	2747	2751	2754	rBV	5899	8391	0.92%	0.088%
31	19.851	2782	2785	2787	rBV3	1331	1506	0.16%	0.016%
32	20.010	2806	2812	2819	rBV	629925	916406	100.00%	9.631%
33	20.151	2834	2836	2839	rVB4	1256	1392	0.15%	0.015%
34	20.662	2921	2923	2926	rBV4	1853	2093	0.23%	0.022%
35	20.744	2935	2937	2938	rBV2	1758	1270	0.14%	0.013%
36	21.008	2980	2982	2984	rBV3	2587	2157	0.24%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052104.D
Acq On : 20 Jan 2022 22:32
Operator : CG/JU
Sample : PB142157BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK157

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

37	21.954	3136	3143	3150	rVB2	317918	542263	59.17%	5.699%
38	23.311	3372	3374	3377	rBV3	2899	3266	0.36%	0.034%
39	23.428	3392	3394	3395	rBV2	2878	2345	0.26%	0.025%
40	23.887	3471	3472	3473	rBV	3526	1292	0.14%	0.014%
41	24.081	3503	3505	3506	rBV2	2741	1390	0.15%	0.015%
42	24.415	3560	3562	3570	rVB6	8794	16862	1.84%	0.177%
43	25.197	3683	3695	3708	rBV2	290628	877115	95.71%	9.219%
44	25.438	3725	3736	3748	rVB2	172348	537738	58.68%	5.652%
45	31.335	4738	4740	4744	rBV5	3016	4384	0.48%	0.046%



Sum of corrected areas: 9514676

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052104.D
Acq On : 20 Jan 2022 22:32
Operator : CG/JU
Sample : PB142157BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

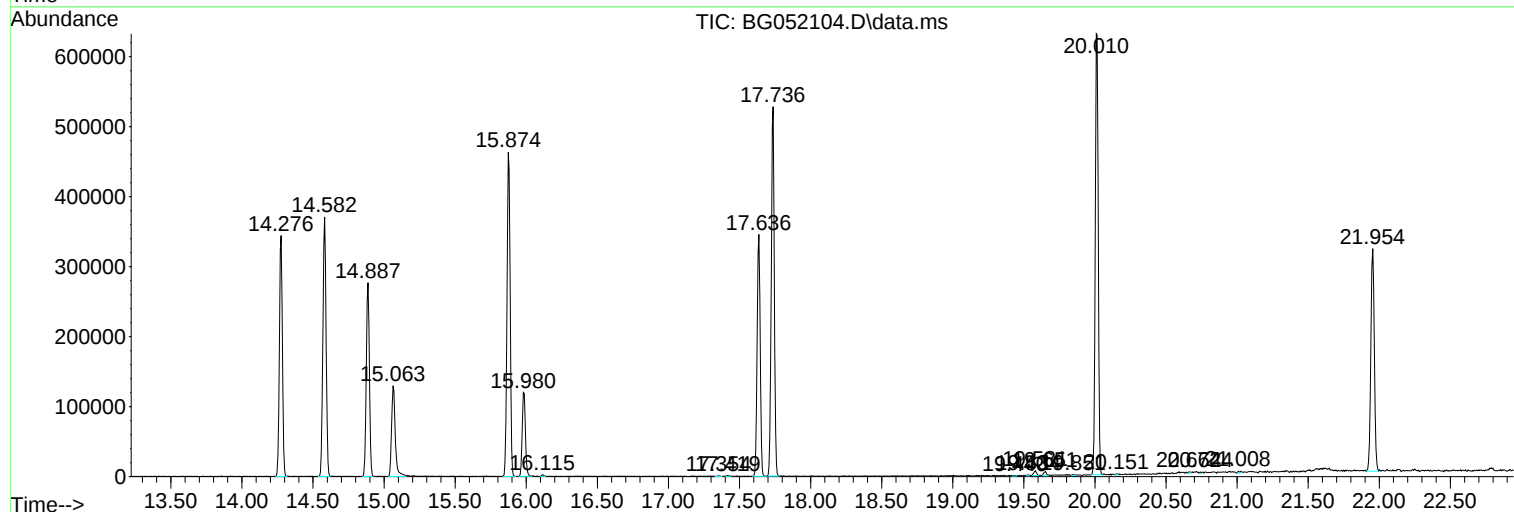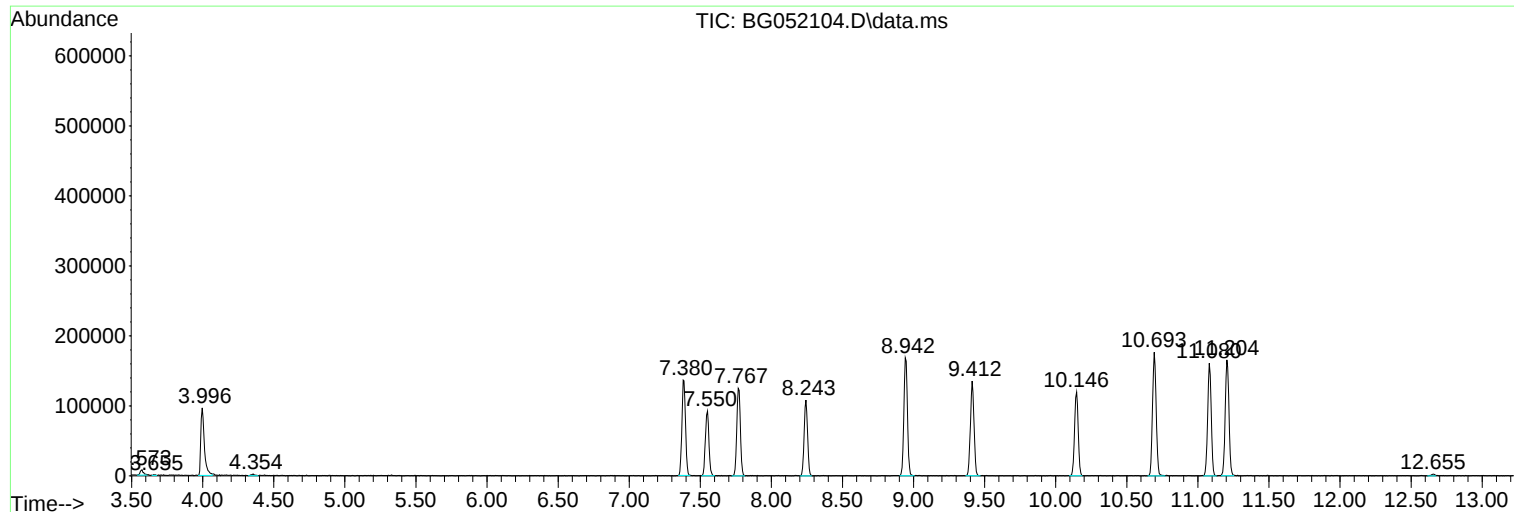

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052104.D
Acq On : 20 Jan 2022 22:32
Operator : CG/JU
Sample : PB142157BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052104.D
Acq On : 20 Jan 2022 22:32
Operator : CG/JU
Sample : PB142157BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc