

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052105.D
 Acq On : 20 Jan 2022 23:09
 Operator : CG/JU
 Sample : N1199-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.570	10	14	20	rVB	8694	11619	1.04%	0.118%
2	3.999	84	87	101	rBV	25352	46518	4.18%	0.471%
3	4.352	143	147	154	rBV3	2190	4013	0.36%	0.041%
4	7.389	657	664	676	rVB2	31355	57599	5.18%	0.584%
5	7.547	685	691	700	rVB	104290	174990	15.73%	1.774%
6	7.770	722	729	737	rBV	110579	188880	16.98%	1.914%
7	8.240	802	809	815	rBV	104154	173830	15.63%	1.762%
8	8.287	815	817	823	rVB2	5487	8225	0.74%	0.083%
9	8.945	922	929	940	rVB2	89373	160927	14.47%	1.631%
10	9.415	1001	1009	1015	rBV	144694	261020	23.47%	2.645%
11	9.826	1077	1079	1083	rVB2	1812	2448	0.22%	0.025%
12	10.144	1125	1133	1140	rBV2	127912	225650	20.29%	2.287%
13	10.690	1220	1226	1235	rBV	176701	318618	28.65%	3.229%
14	10.825	1245	1249	1252	rBV3	2289	3403	0.31%	0.034%
15	11.084	1284	1293	1300	rBB	147156	267031	24.01%	2.706%
16	11.201	1304	1313	1325	rVV	143995	271164	24.38%	2.748%
17	12.476	1526	1530	1531	rBV	1742	1825	0.16%	0.018%
18	12.652	1554	1560	1566	rBV4	2698	5182	0.47%	0.053%
19	13.692	1734	1737	1741	rBV3	3279	3763	0.34%	0.038%
20	14.273	1829	1836	1842	rBV	405747	556591	50.04%	5.641%
21	14.520	1871	1878	1881	rBV3	1355	2641	0.24%	0.027%
22	14.579	1881	1888	1896	rVB	417718	652063	58.62%	6.609%
23	14.761	1916	1919	1921	rVB3	1633	1631	0.15%	0.017%
24	14.884	1930	1940	1947	rBV2	261301	402519	36.19%	4.080%
25	15.066	1963	1971	1981	rBV2	29182	53110	4.77%	0.538%
26	15.601	2058	2062	2067	rVB2	1315	2179	0.20%	0.022%
27	15.677	2067	2075	2083	rBV	60429	89031	8.00%	0.902%
28	15.877	2102	2109	2116	rVB	549381	850636	76.48%	8.621%
29	15.983	2121	2127	2136	rVB	170041	252074	22.66%	2.555%
30	16.112	2146	2149	2154	rVB2	2400	3099	0.28%	0.031%
31	16.230	2165	2169	2173	rBV2	1142	1525	0.14%	0.015%
32	16.453	2202	2207	2210	rBV2	1205	1871	0.17%	0.019%
33	17.363	2359	2362	2367	rBV	1761	2490	0.22%	0.025%
34	17.410	2367	2370	2375	rBV2	1626	2677	0.24%	0.027%
35	17.634	2401	2408	2415	rBV	329171	503227	45.24%	5.100%
36	17.733	2417	2425	2437	rVB	647467	975106	87.67%	9.883%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052105.D
 Acq On : 20 Jan 2022 23:09
 Operator : CG/JU
 Sample : N1199-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	17.898	2449	2453	2456	rBV	1565	1661	0.15%	0.017%
38	18.004	2467	2471	2475	rBV3	1263	2214	0.20%	0.022%
39	18.103	2485	2488	2493	rBV3	1372	1898	0.17%	0.019%
40	18.286	2511	2519	2521	rBV4	2509	4071	0.37%	0.041%
41	18.503	2551	2556	2558	rBV3	1507	2520	0.23%	0.026%
42	18.573	2565	2568	2572	rBV2	1526	2003	0.18%	0.020%
43	19.261	2681	2685	2687	rBV3	1276	1745	0.16%	0.018%
44	19.413	2710	2711	2718	rVB3	1811	2311	0.21%	0.023%
45	19.578	2735	2739	2745	rVB4	8406	13269	1.19%	0.134%
46	19.643	2747	2750	2755	rVB	6796	10141	0.91%	0.103%
47	20.013	2806	2813	2821	rVB	762444	1112298	100.00%	11.273%
48	20.312	2862	2864	2866	rBV3	1973	1905	0.17%	0.019%
49	20.347	2866	2870	2871	rVB3	1960	2545	0.23%	0.026%
50	20.970	2973	2976	2983	rVB5	9941	14115	1.27%	0.143%
51	21.023	2983	2985	2987	rBV2	2751	1978	0.18%	0.020%
52	21.552	3072	3075	3076	rBV3	5503	4976	0.45%	0.050%
53	21.951	3137	3143	3155	rVB	297607	521468	46.88%	5.285%
54	22.227	3188	3190	3191	rVB2	3314	1636	0.15%	0.017%
55	25.194	3684	3695	3709	rVB	353685	1065117	95.76%	10.795%
56	25.435	3726	3736	3752	rVB2	164920	548887	49.35%	5.563%
57	25.999	3831	3832	3835	rBV2	3122	2447	0.22%	0.025%
58	27.784	4134	4136	4140	rBV5	2914	2285	0.21%	0.023%
59	27.984	4169	4170	4172	rVB2	3285	1678	0.15%	0.017%
60	29.623	4447	4449	4451	rBV3	2958	2805	0.25%	0.028%
61	32.601	4954	4956	4957	rBV2	2590	1613	0.15%	0.016%




Sum of corrected areas: 9866761

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052105.D
Acq On : 20 Jan 2022 23:09
Operator : CG/JU
Sample : N1199-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

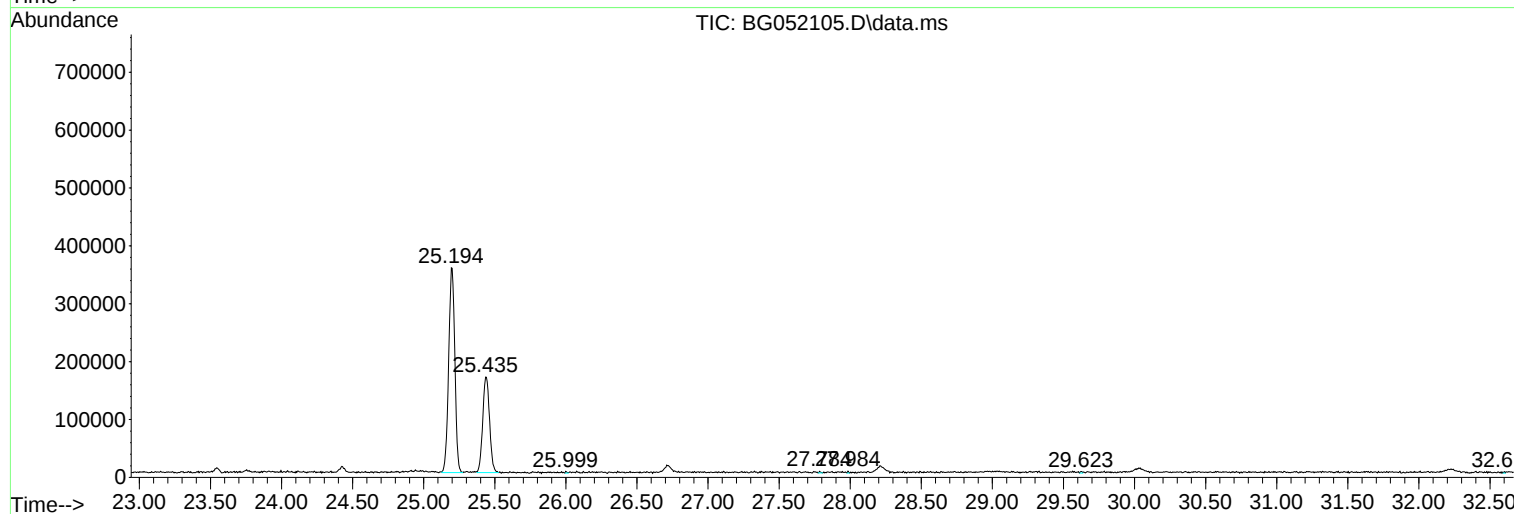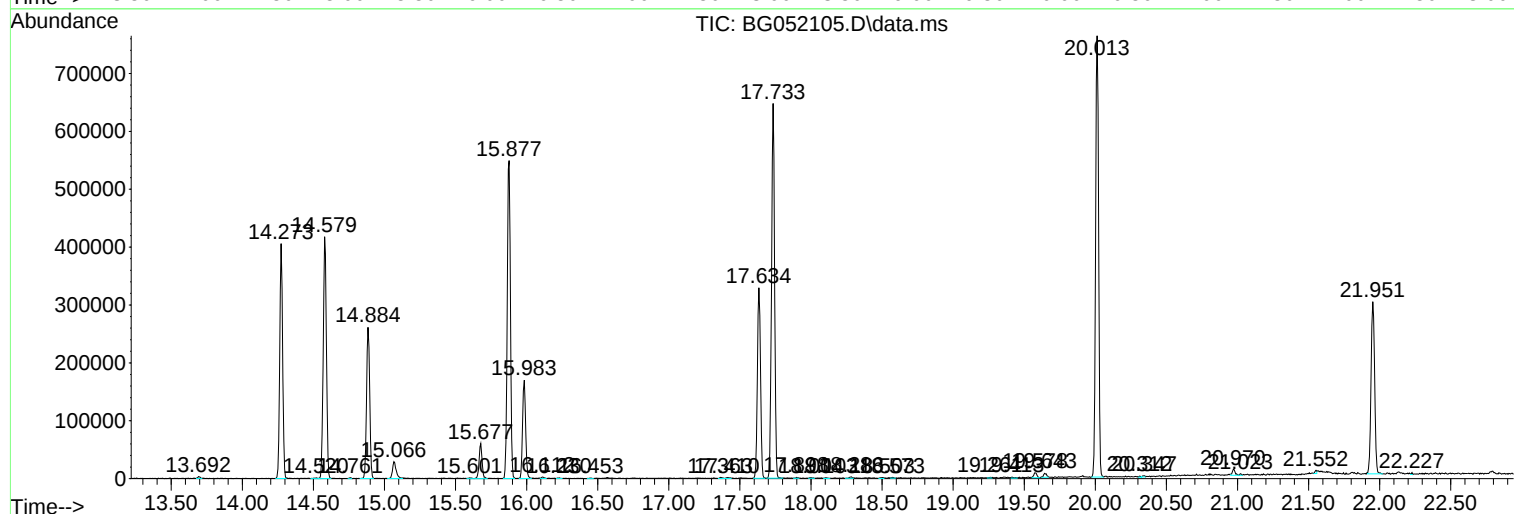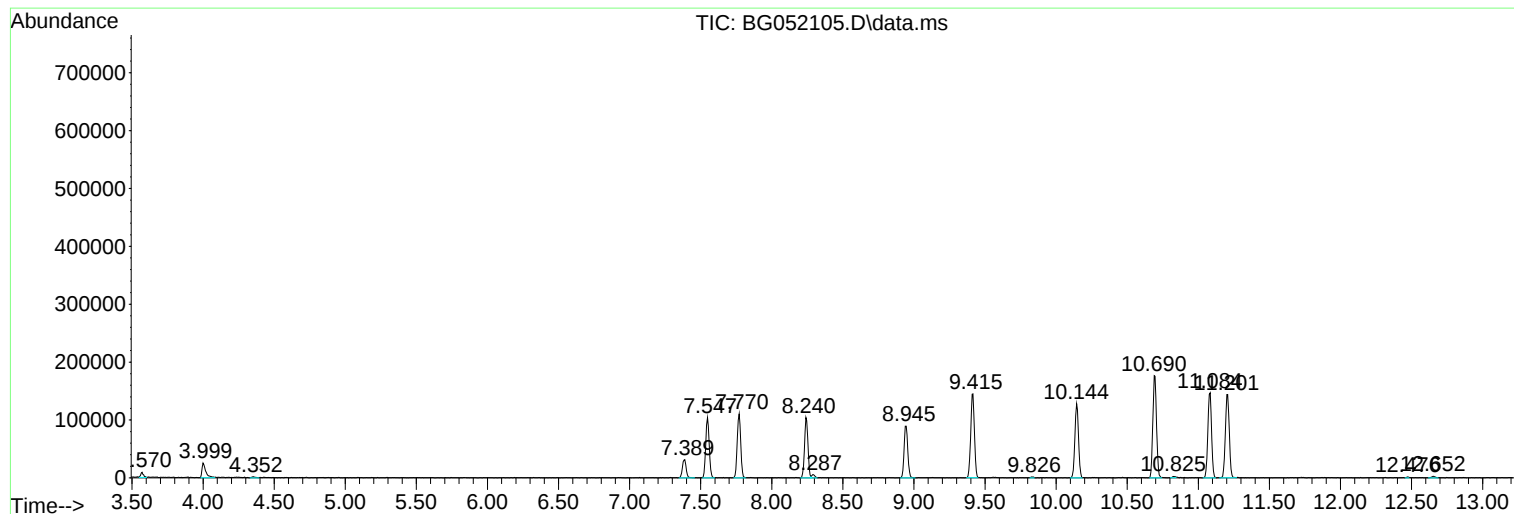

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052105.D
Acq On : 20 Jan 2022 23:09
Operator : CG/JU
Sample : N1199-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052105.D
Acq On : 20 Jan 2022 23:09
Operator : CG/JU
Sample : N1199-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc