

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052107.D
 Acq On : 21 Jan 2022 00:24
 Operator : CG/JU
 Sample : N1199-08
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.566	10	13	21	rVB2	6169	9280	0.87%	0.098%
2	4.007	84	88	94	rBV	12175	20088	1.89%	0.213%
3	4.353	142	147	151	rVB4	1940	2707	0.25%	0.029%
4	5.293	303	307	311	rVB2	1305	1940	0.18%	0.021%
5	7.385	657	663	672	rBV2	37907	67060	6.30%	0.710%
6	7.549	683	691	699	rBV	104037	176472	16.58%	1.868%
7	7.772	721	729	736	rVB	113274	199245	18.72%	2.109%
8	8.242	802	809	815	rBV	94309	155925	14.65%	1.650%
9	8.289	815	817	822	rVB3	4030	5497	0.52%	0.058%
10	8.941	919	928	937	rBV	101267	182739	17.16%	1.934%
11	9.411	1000	1008	1018	rVB	149177	266639	25.05%	2.822%
12	9.828	1075	1079	1083	rBB2	2189	3059	0.29%	0.032%
13	10.146	1125	1133	1140	rVB	136127	230455	21.65%	2.439%
14	10.692	1216	1226	1237	rBV	186040	330330	31.03%	3.496%
15	10.833	1245	1250	1253	rBV3	1719	2655	0.25%	0.028%
16	11.080	1285	1292	1299	rBV	132545	238585	22.41%	2.525%
17	11.203	1306	1313	1326	rBV	113857	216240	20.31%	2.288%
18	12.466	1526	1528	1532	rBB2	1578	1652	0.16%	0.017%
19	12.654	1554	1560	1566	rBV	2896	4928	0.46%	0.052%
20	12.942	1606	1609	1613	rBV2	1109	1684	0.16%	0.018%
21	13.700	1734	1738	1741	rBV	1795	2475	0.23%	0.026%
22	13.758	1746	1748	1756	rBV3	1063	1781	0.17%	0.019%
23	14.199	1818	1823	1824	rBV	1453	1531	0.14%	0.016%
24	14.275	1829	1836	1842	rVV	395827	554710	52.10%	5.870%
25	14.581	1881	1888	1895	rBV	415797	653083	61.34%	6.912%
26	14.886	1933	1940	1947	rBV	240146	367953	34.56%	3.894%
27	15.068	1965	1971	1983	rBV2	33690	62194	5.84%	0.658%
28	15.679	2068	2075	2080	rBV2	36259	54757	5.14%	0.579%
29	15.808	2093	2097	2100	rBV2	2545	3490	0.33%	0.037%
30	15.873	2102	2108	2117	rVV	539672	833368	78.28%	8.819%
31	15.985	2121	2127	2137	rVB	161475	251204	23.60%	2.658%
32	16.120	2144	2150	2154	rVB	2895	4840	0.45%	0.051%
33	16.596	2228	2231	2235	rVB2	1792	2158	0.20%	0.023%
34	17.095	2312	2316	2319	rVB	1329	2045	0.19%	0.022%
35	17.418	2368	2371	2376	rBV3	2994	3128	0.29%	0.033%
36	17.635	2402	2408	2417	rVB	303725	453840	42.63%	4.803%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052107.D
 Acq On : 21 Jan 2022 00:24
 Operator : CG/JU
 Sample : N1199-08
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	17.735	2419	2425	2432	rVV2	617320	935703	87.89%	9.903%
38	17.888	2447	2451	2454	rBV2	1460	2444	0.23%	0.026%
39	18.282	2514	2518	2525	rVB3	10299	12406	1.17%	0.131%
40	18.505	2553	2556	2561	rBV3	1577	2807	0.26%	0.030%
41	18.569	2561	2567	2572	rVB4	2383	4491	0.42%	0.048%
42	19.409	2707	2710	2711	rBV	1666	1531	0.14%	0.016%
43	19.439	2711	2715	2719	rVB2	15405	17446	1.64%	0.185%
44	19.574	2735	2738	2743	rVB5	8856	12264	1.15%	0.130%
45	19.644	2746	2750	2756	rVV2	7068	10068	0.95%	0.107%
46	19.903	2791	2794	2798	rVB3	3367	4101	0.39%	0.043%
47	20.015	2806	2813	2821	rBV	738528	1064625	100.00%	11.267%
48	20.338	2866	2868	2871	rBV2	3319	3093	0.29%	0.033%
49	20.578	2907	2909	2913	rBV4	2869	3590	0.34%	0.038%
50	21.953	3137	3143	3150	rVB	270323	462354	43.43%	4.893%
51	22.135	3172	3174	3178	rVB4	3928	4223	0.40%	0.045%
52	23.909	3474	3476	3477	rBV2	3112	2385	0.22%	0.025%
53	24.426	3560	3564	3572	rVB5	9765	20701	1.94%	0.219%
54	25.202	3683	3696	3709	rBV2	352842	1015407	95.38%	10.746%
55	25.437	3726	3736	3750	rVB2	155704	496244	46.61%	5.252%
56	26.670	3944	3946	3947	rBV3	3140	2085	0.20%	0.022%
57	31.329	4737	4739	4740	rBV2	2776	1449	0.14%	0.015%




Sum of corrected areas: 9449154

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052107.D
Acq On : 21 Jan 2022 00:24
Operator : CG/JU
Sample : N1199-08
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

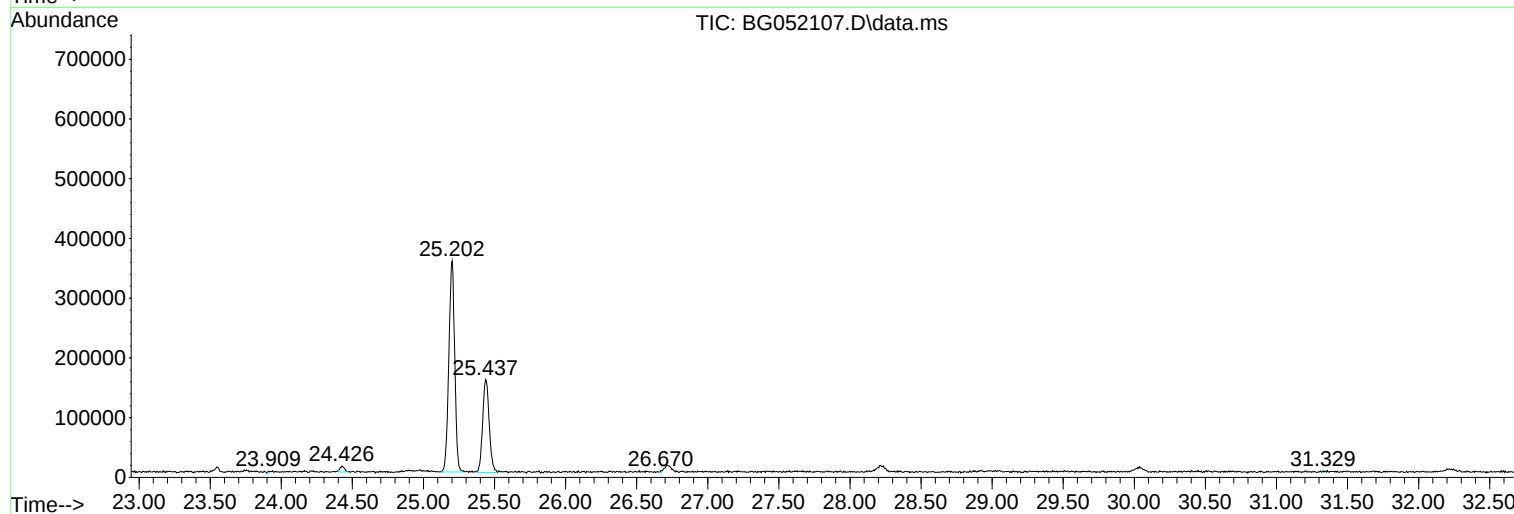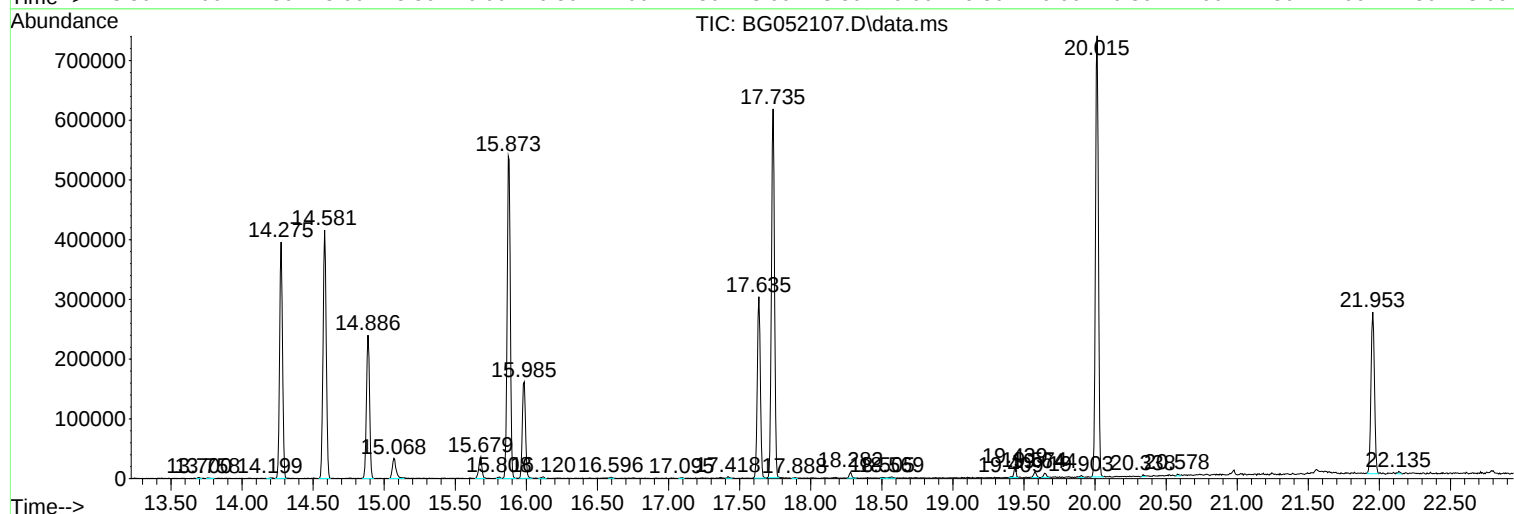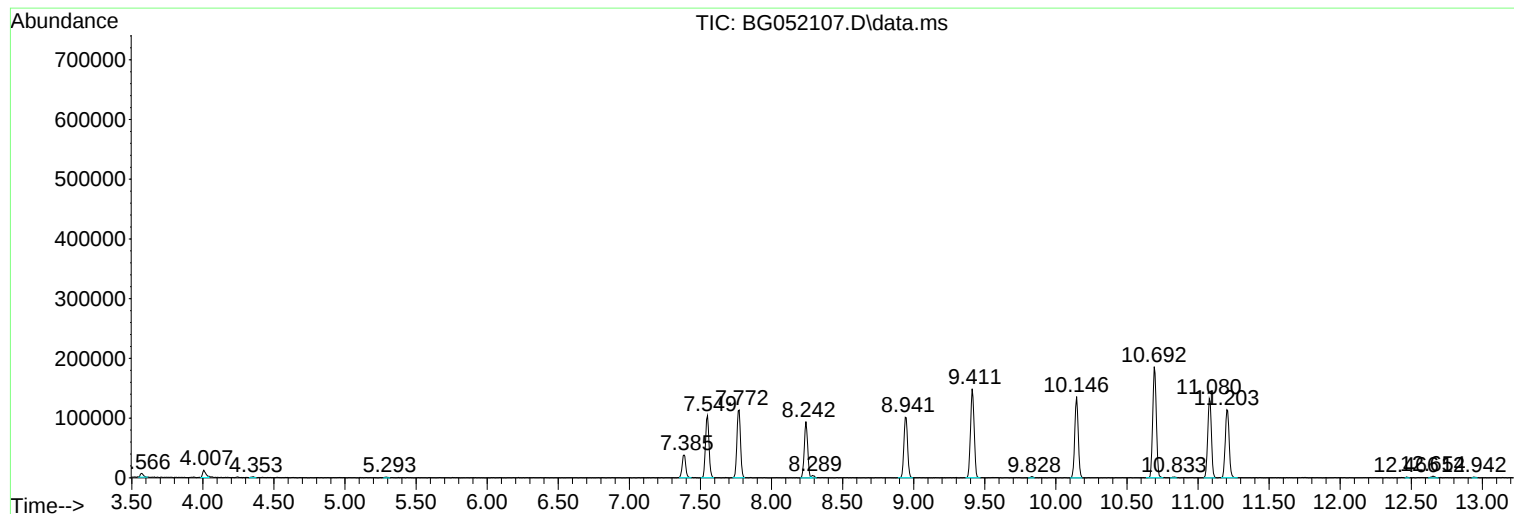

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052107.D
Acq On : 21 Jan 2022 00:24
Operator : CG/JU
Sample : N1199-08
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052107.D
Acq On : 21 Jan 2022 00:24
Operator : CG/JU
Sample : N1199-08
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
