

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052112.D
 Acq On : 21 Jan 2022 9:22
 Operator : CG/JU
 Sample : PB142157BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK157

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.576	10	15	21	rVB2	7960	12335	1.23%	0.122%
2	4.005	83	88	103	rBV	110416	185414	18.56%	1.838%
3	4.357	145	148	155	rVB2	1890	2931	0.29%	0.029%
4	7.400	659	666	675	rVB	159356	269084	26.93%	2.668%
5	7.564	686	694	704	rVB	105481	177804	17.80%	1.763%
6	7.788	724	732	742	rBV	140676	241684	24.19%	2.396%
7	8.263	804	813	820	rBB	91355	161278	16.14%	1.599%
8	8.963	924	932	942	rVB	188558	324292	32.46%	3.215%
9	9.432	1004	1012	1020	rBV	144364	260323	26.06%	2.581%
10	10.161	1130	1136	1145	rVB	128122	228653	22.89%	2.267%
11	10.713	1222	1230	1241	rBV	186559	343290	34.36%	3.404%
12	11.095	1287	1295	1304	rBV	137022	248384	24.86%	2.463%
13	11.218	1308	1316	1325	rBV	178424	331377	33.17%	3.286%
14	12.669	1558	1563	1567	rVV2	2759	4426	0.44%	0.044%
15	14.285	1832	1838	1845	rVB	373347	527901	52.84%	5.234%
16	14.590	1883	1890	1897	rBV	406708	631467	63.20%	6.261%
17	14.896	1935	1942	1949	rBV	242135	372677	37.30%	3.695%
18	15.078	1966	1973	1984	rBV	139541	242473	24.27%	2.404%
19	15.888	2104	2111	2118	rBV	509838	770164	77.09%	7.636%
20	15.994	2123	2129	2139	rBV	127519	202513	20.27%	2.008%
21	16.123	2147	2151	2152	rBV2	1912	2044	0.20%	0.020%
22	17.645	2403	2410	2419	rVB	314684	464731	46.52%	4.608%
23	17.745	2420	2427	2434	rVV	538767	855628	85.64%	8.484%
24	19.583	2735	2740	2747	rBV3	8065	12445	1.25%	0.123%
25	19.654	2747	2752	2756	rBV	7330	9589	0.96%	0.095%
26	20.018	2807	2814	2822	rVV	687199	999094	100.00%	9.906%
27	20.142	2829	2835	2836	rVV4	973	1568	0.16%	0.016%
28	20.177	2838	2841	2844	rBV4	1578	1885	0.19%	0.019%
29	20.547	2901	2904	2907	rBV3	1934	3018	0.30%	0.030%
30	20.764	2938	2941	2944	rBV5	2172	3030	0.30%	0.030%
31	20.946	2970	2972	2974	rVB4	2764	1711	0.17%	0.017%
32	20.970	2974	2976	2978	rBV2	2177	1773	0.18%	0.018%
33	21.510	3065	3068	3069	rBV3	2398	2404	0.24%	0.024%
34	21.822	3117	3121	3122	rBV2	2913	3403	0.34%	0.034%
35	21.916	3134	3137	3138	rBV2	2253	2580	0.26%	0.026%
36	21.957	3138	3144	3157	rVB2	292900	497507	49.80%	4.933%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052112.D
 Acq On : 21 Jan 2022 9:22
 Operator : CG/JU
 Sample : PB142157BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK157

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	22.391	3216	3218	3221	rBV4	1873	2341	0.23%	0.023%
38	22.944	3310	3312	3315	rVB4	1848	1598	0.16%	0.016%
39	23.484	3402	3404	3407	rBV4	1973	2533	0.25%	0.025%
40	23.549	3410	3415	3421	rVB6	8205	18117	1.81%	0.180%
41	23.596	3421	3423	3427	rBV4	2905	3274	0.33%	0.032%
42	23.725	3444	3445	3447	rBV2	1922	1695	0.17%	0.017%
43	23.795	3454	3457	3459	rBV2	2303	2156	0.22%	0.021%
44	23.919	3477	3478	3481	rBV2	1622	1622	0.16%	0.016%
45	23.972	3484	3487	3489	rVV4	2147	2121	0.21%	0.021%
46	24.024	3493	3496	3497	rBV2	1571	1981	0.20%	0.020%
47	24.060	3500	3502	3505	rVV4	2055	2372	0.24%	0.024%
48	24.101	3505	3509	3512	rVB5	2082	2644	0.26%	0.026%
49	24.201	3525	3526	3528	rBV2	2374	2002	0.20%	0.020%
50	24.442	3560	3567	3574	rVB5	9449	19253	1.93%	0.191%
51	24.700	3609	3611	3614	rBV4	2212	1994	0.20%	0.020%
52	24.853	3634	3637	3638	rVB2	2274	1708	0.17%	0.017%
53	24.865	3638	3639	3642	rBV3	3221	3279	0.33%	0.033%
54	24.994	3659	3661	3666	rVV5	1940	3003	0.30%	0.030%
55	25.041	3666	3669	3672	rVB5	2951	3489	0.35%	0.035%
56	25.111	3679	3681	3684	rVB4	2139	1904	0.19%	0.019%
57	25.211	3684	3698	3710	rBV3	315546	964433	96.53%	9.563%
58	25.452	3726	3739	3754	rVV2	161094	514123	51.46%	5.098%
59	25.669	3773	3776	3778	rBV4	2054	2577	0.26%	0.026%
60	25.810	3797	3800	3801	rBV3	2363	2199	0.22%	0.022%
61	25.869	3809	3810	3812	rBV2	2384	2009	0.20%	0.020%
62	26.110	3849	3851	3853	rBV3	1761	1702	0.17%	0.017%
63	26.492	3913	3916	3919	rBV4	1621	2667	0.27%	0.026%
64	26.521	3919	3921	3923	rVB3	1980	1644	0.16%	0.016%
65	26.721	3949	3955	3956	rBV5	9282	13406	1.34%	0.133%
66	26.827	3970	3973	3978	rBV7	1586	2202	0.22%	0.022%
67	27.020	4004	4006	4010	rVB3	1954	1677	0.17%	0.017%
68	27.079	4013	4016	4018	rVB4	1854	2161	0.22%	0.021%
69	27.391	4067	4069	4072	rVB4	2353	1830	0.18%	0.018%
70	27.485	4082	4085	4086	rBV2	1435	1567	0.16%	0.016%
71	27.543	4093	4095	4099	rBV4	1597	1741	0.17%	0.017%
72	28.019	4173	4176	4178	rVB3	2264	2230	0.22%	0.022%
73	28.043	4178	4180	4184	rBV5	2666	4046	0.40%	0.040%
74	28.219	4203	4210	4211	rBV5	10183	15952	1.60%	0.158%
75	28.366	4232	4235	4236	rBV3	1919	1683	0.17%	0.017%
76	28.383	4236	4238	4240	rVV3	1663	1775	0.18%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
 Data File : BG052112.D
 Acq On : 21 Jan 2022 9:22
 Operator : CG/JU
 Sample : PB142157BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK157

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	28.524	4261	4262	4263	rBV	3261	1753	0.18%	0.017%
78	28.642	4281	4282	4285	rBV3	1845	1703	0.17%	0.017%
79	28.859	4316	4319	4321	rBV3	2314	2472	0.25%	0.025%
80	28.977	4337	4339	4340	rBV2	2248	1882	0.19%	0.019%
81	29.259	4385	4387	4390	rVB4	2036	2033	0.20%	0.020%
82	29.282	4390	4391	4395	rBV3	1759	1967	0.20%	0.020%
83	29.341	4399	4401	4403	rVV3	2109	1626	0.16%	0.016%
84	29.364	4403	4405	4408	rVV4	1832	2034	0.20%	0.020%
85	29.494	4424	4427	4428	rBV2	2189	1800	0.18%	0.018%
86	29.564	4435	4439	4440	rVV3	2403	2390	0.24%	0.024%
87	29.664	4455	4456	4458	rBV2	2036	1699	0.17%	0.017%
88	29.776	4472	4475	4478	rBV4	1983	2491	0.25%	0.025%
89	29.858	4487	4489	4493	rBV5	1327	2136	0.21%	0.021%
90	30.022	4514	4517	4518	rBV2	3541	3446	0.34%	0.034%
91	30.040	4518	4520	4521	rBV2	2903	2948	0.30%	0.029%
92	30.240	4552	4554	4556	rBV3	1811	2144	0.21%	0.021%
93	30.516	4599	4601	4602	rBV2	1900	1735	0.17%	0.017%
94	30.792	4646	4648	4650	rBV3	2458	2109	0.21%	0.021%
95	31.062	4690	4694	4695	rBV4	1826	1911	0.19%	0.019%
96	31.097	4698	4700	4702	rBV2	2344	2374	0.24%	0.024%
97	31.215	4718	4720	4722	rBV3	1871	1842	0.18%	0.018%
98	31.790	4815	4818	4823	rVB5	2594	3153	0.32%	0.031%
99	32.231	4884	4893	4894	rBV8	5341	12001	1.20%	0.119%
100	32.613	4955	4958	4961	rBV4	2576	4111	0.41%	0.041%




Sum of corrected areas: 10085350

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052112.D
Acq On : 21 Jan 2022 9:22
Operator : CG/JU
Sample : PB142157BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

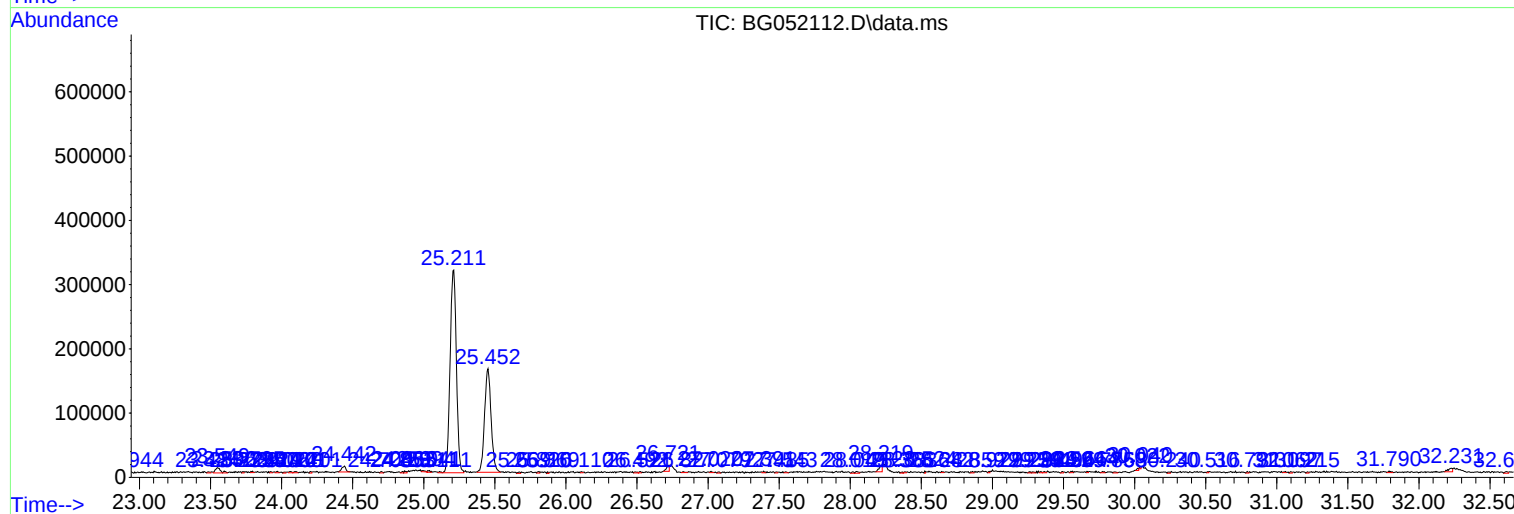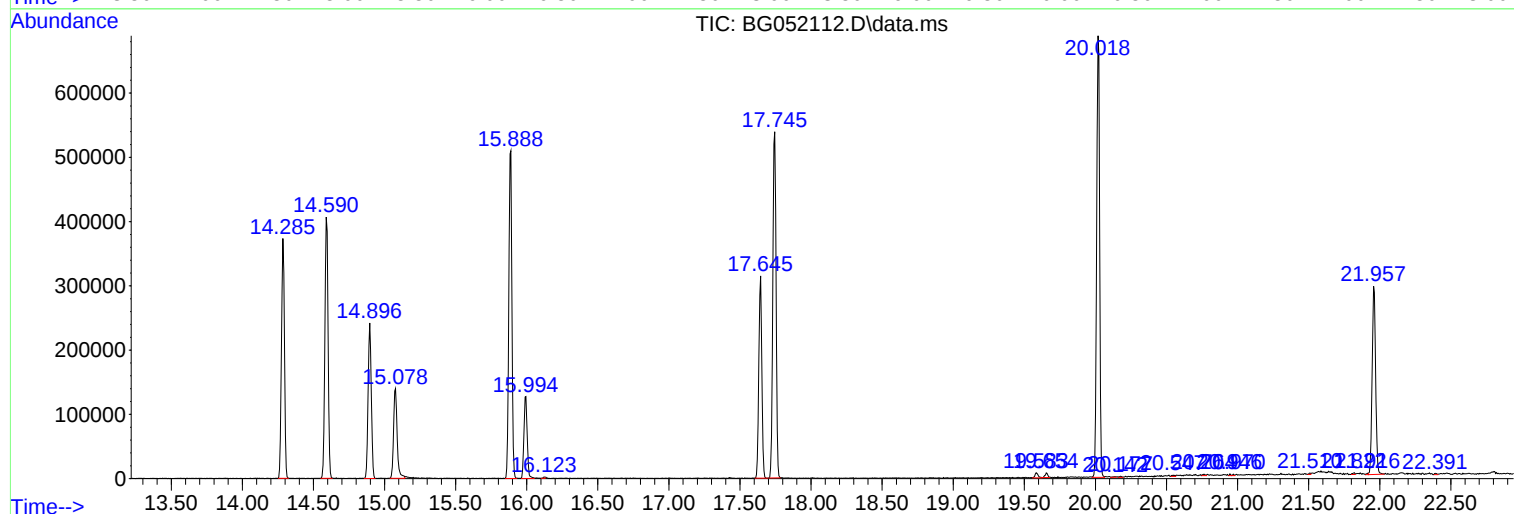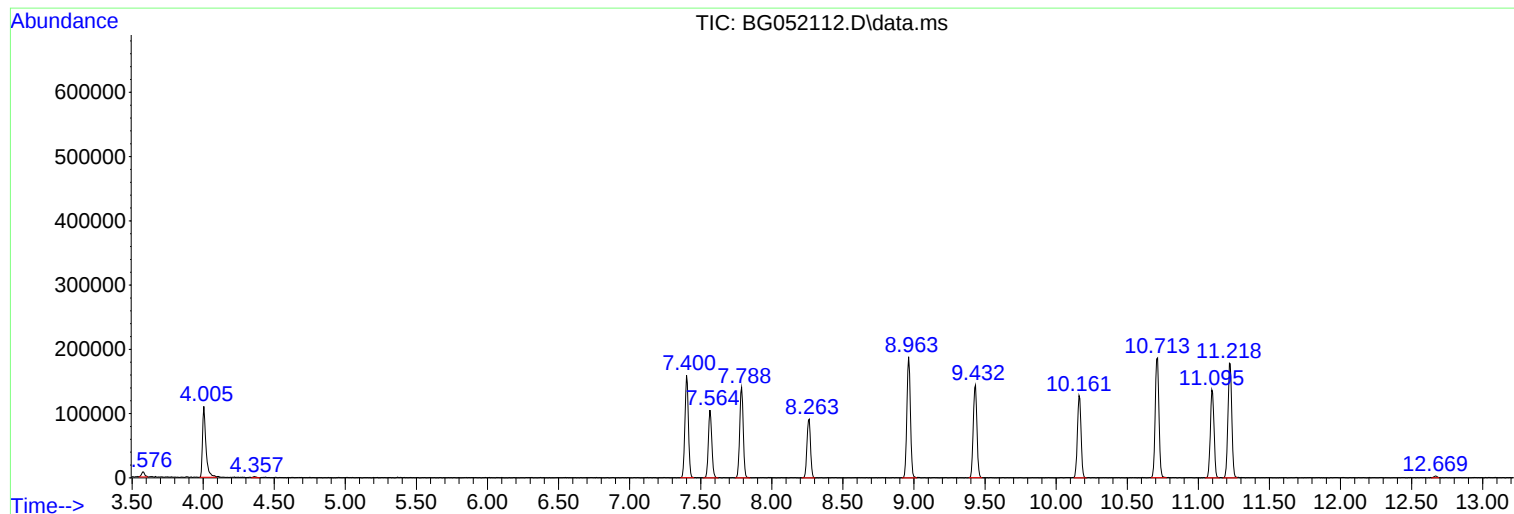

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052112.D
Acq On : 21 Jan 2022 9:22
Operator : CG/JU
Sample : PB142157BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011922\
Data File : BG052112.D
Acq On : 21 Jan 2022 9:22
Operator : CG/JU
Sample : PB142157BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc