


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011923\
Data File : BG056346.D
Acq On : 19 Jan 2023 13:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 19 00:31:30 2023

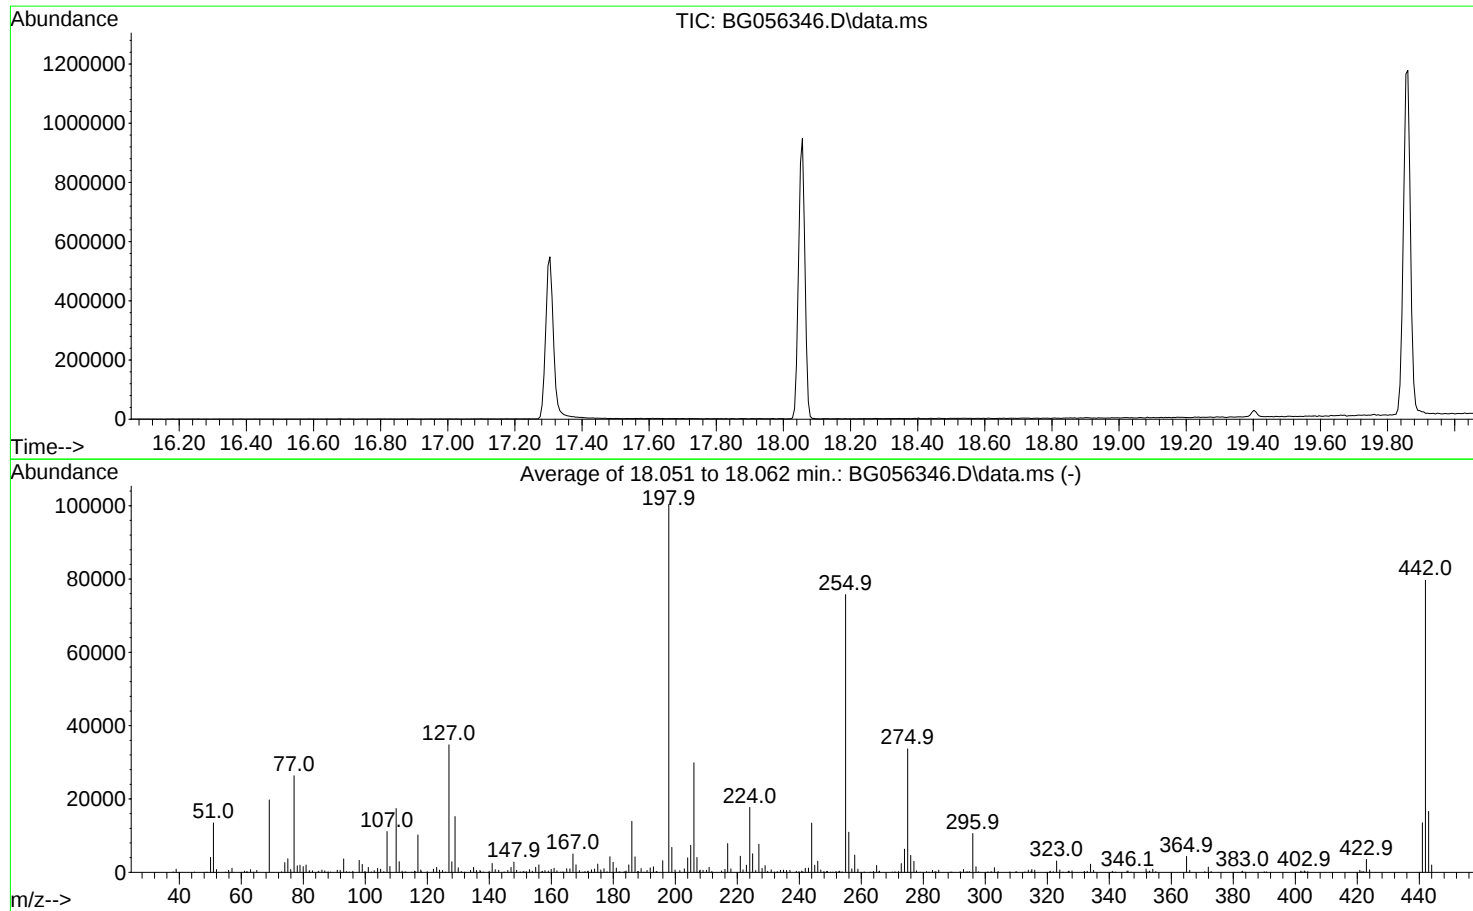




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	13.4	13467	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	19.7	19758	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.7	34781	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	100355	PASS
199	198	5	9	6.8	6788	PASS
275	198	10	60	33.6	33680	PASS
365	198	1	100	4.3	4356	PASS
441	198	0.01	100	13.5	13531	PASS
442	442	50	100	100.0	79669	PASS
443	442	15	24	20.8	16592	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011923\  
Data File : BG056346.D  
Acq On    : 19 Jan 2023   13:32  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 20 05:20:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

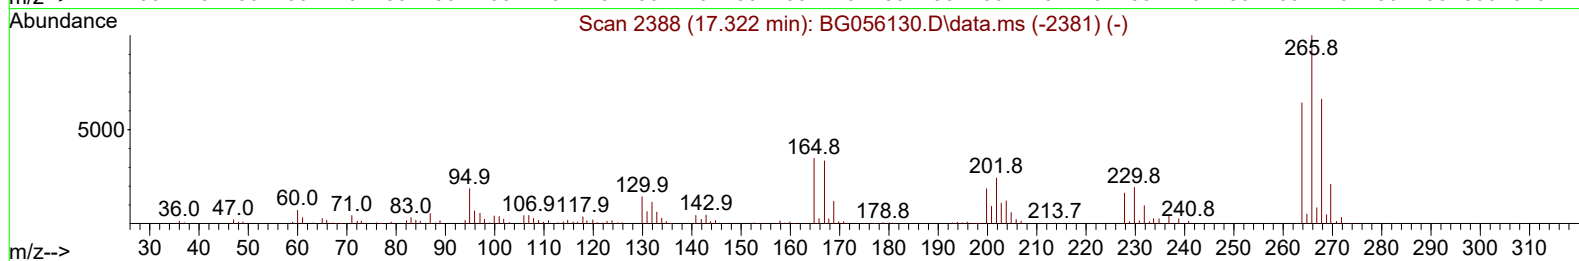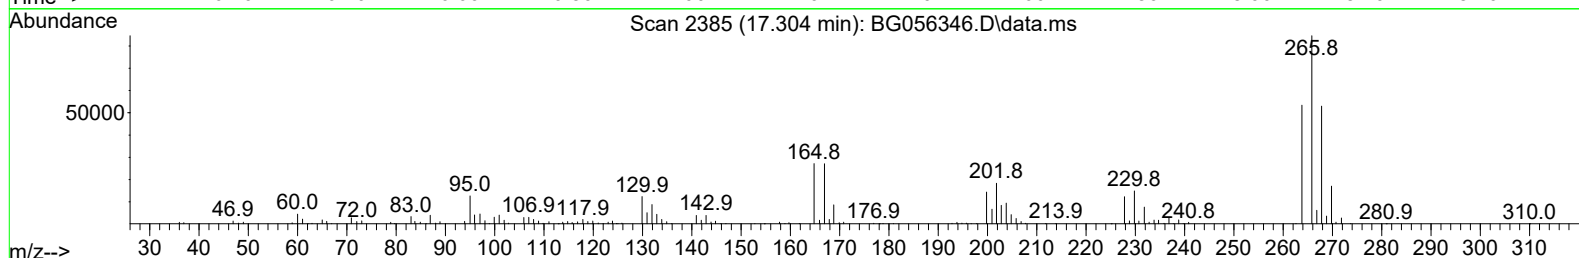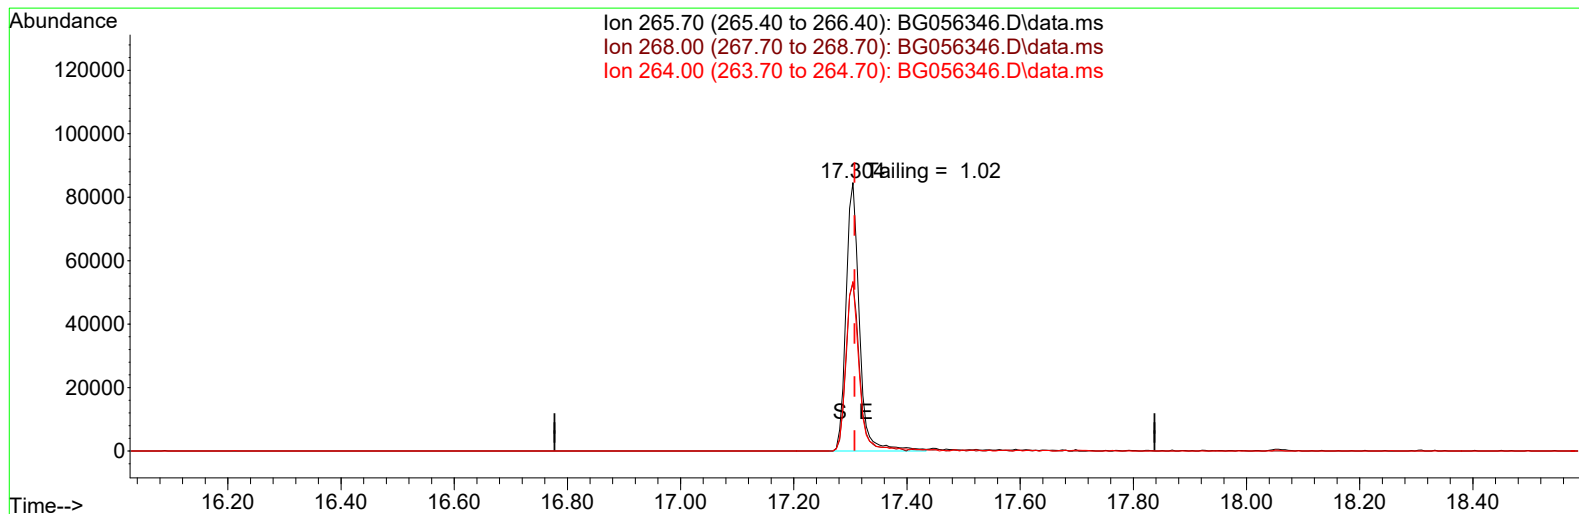

TIC: BG056346.D\data.ms

(70) Pentachlorophenol (C)

17.304min (-0.003) 23432.74 ng




response **138363**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	62.61
264.00	64.30	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011923\
Data File : BG056346.D
Acq On : 19 Jan 2023 13:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 20 05:20:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

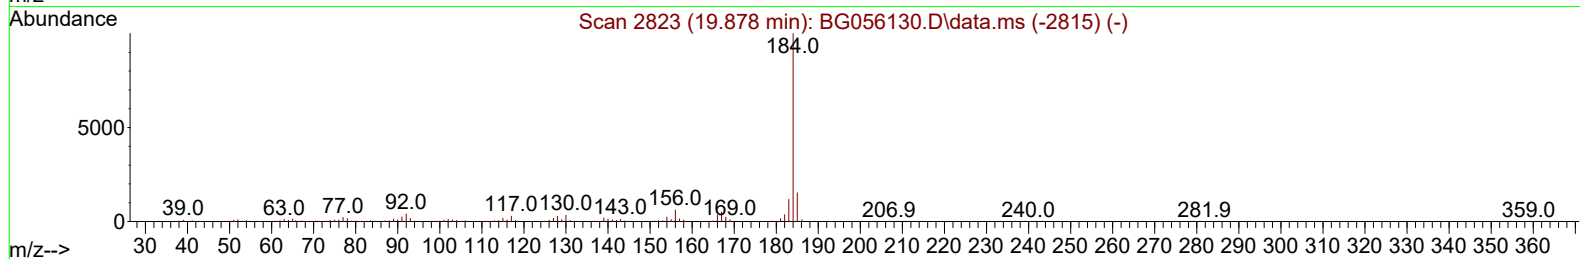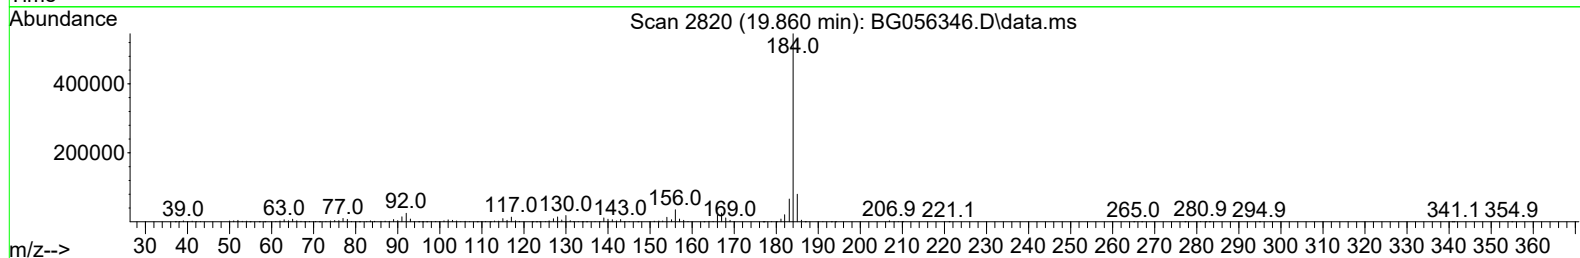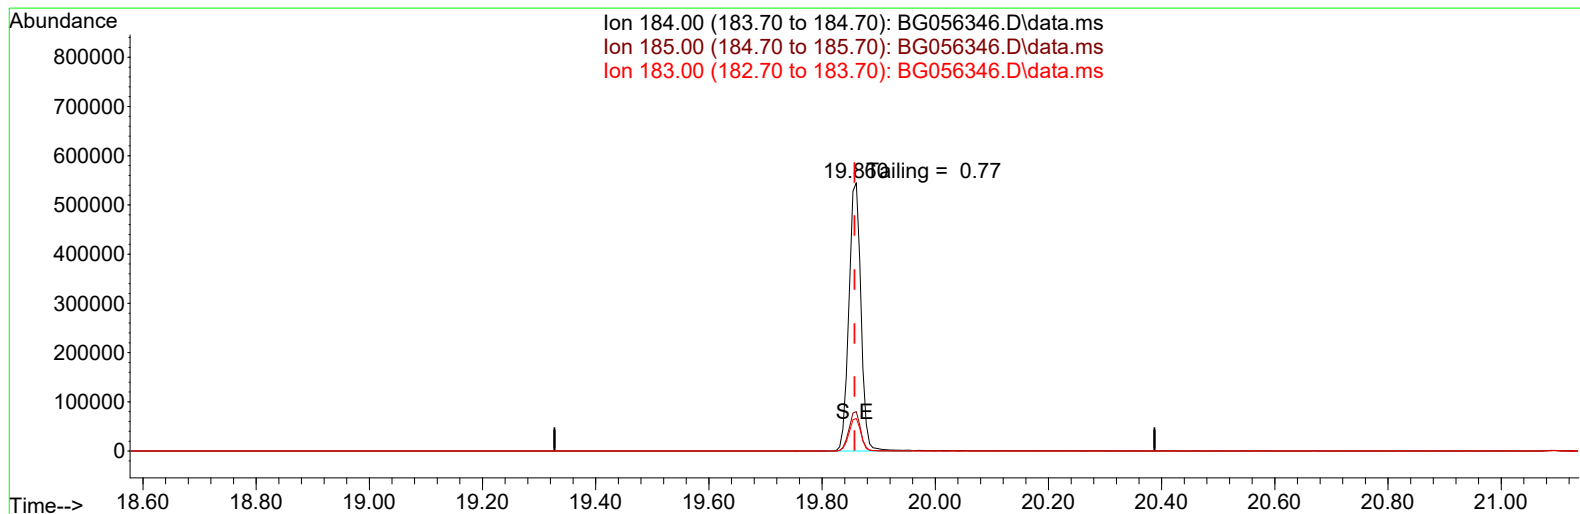

TIC: BG056346.D\data.ms

(77) Benzidine

19.860min (+ 0.003) 251426.76 ng

response 801808

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.68
183.00	11.70	12.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/19/2023	BNA_G	<u>BG056346.D</u>
Compound Name	Response	Retention Time
DDT	374943	21.088
DDD	12774	20.636
DDE	2757	20.136
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15531	390474	3.98

Instrument :
BNA_G
ClientSampleId :
DFTPP