
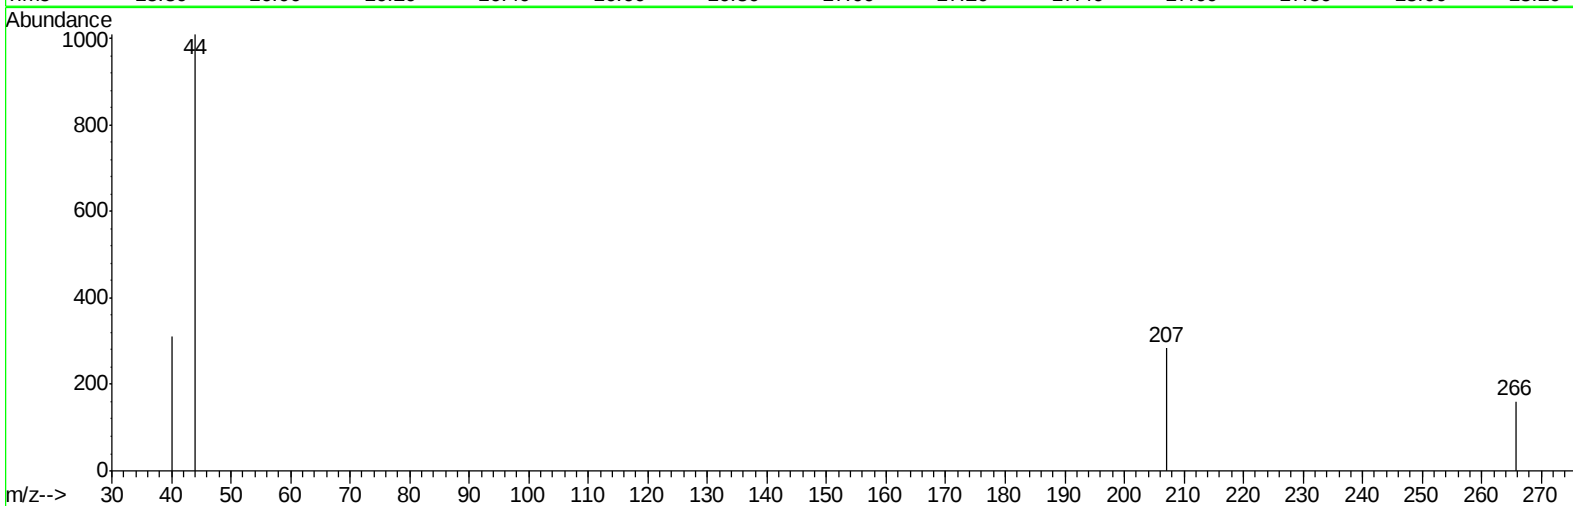


Data File : BG044154.D
Acq On : 22 Jan 2020 11:48
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 08:28:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

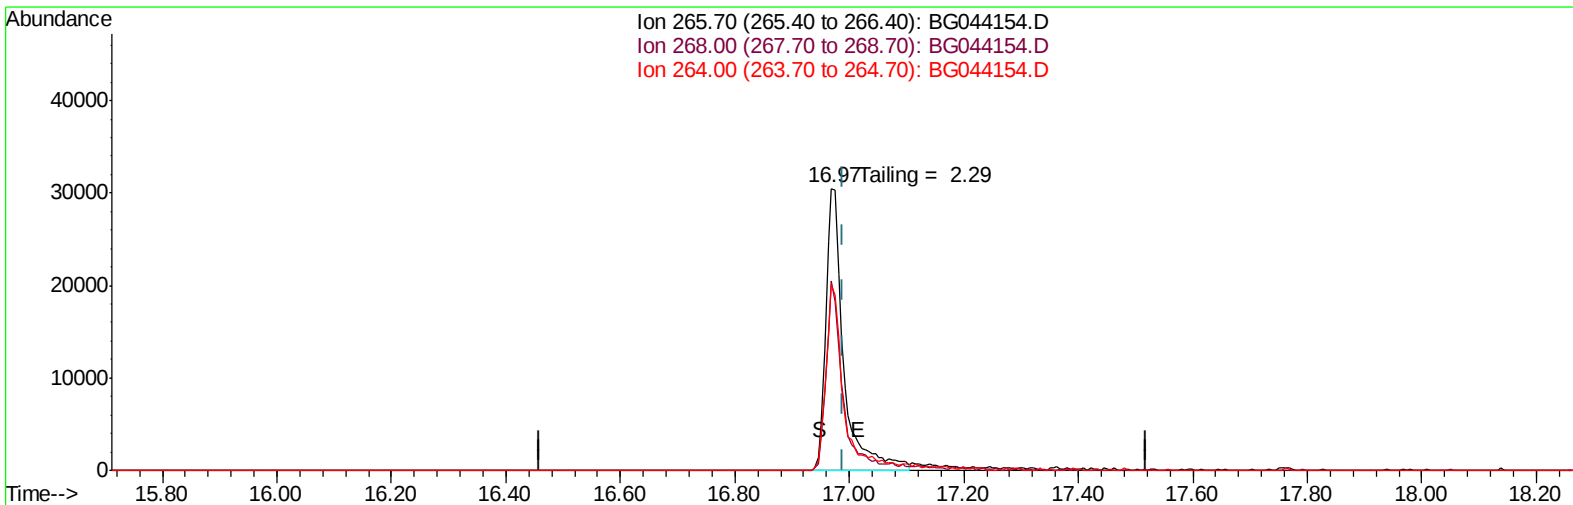

TIC: BG044154.D

(70) Pentachlorophenol (C)



16.969min (-0.020) 23372.14ng m

response 66203

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	67.38
264.00	63.50	65.73
0.00	0.00	0.00

Data File : BG044154.D
Acq On : 22 Jan 2020 11:48
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 08:28:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

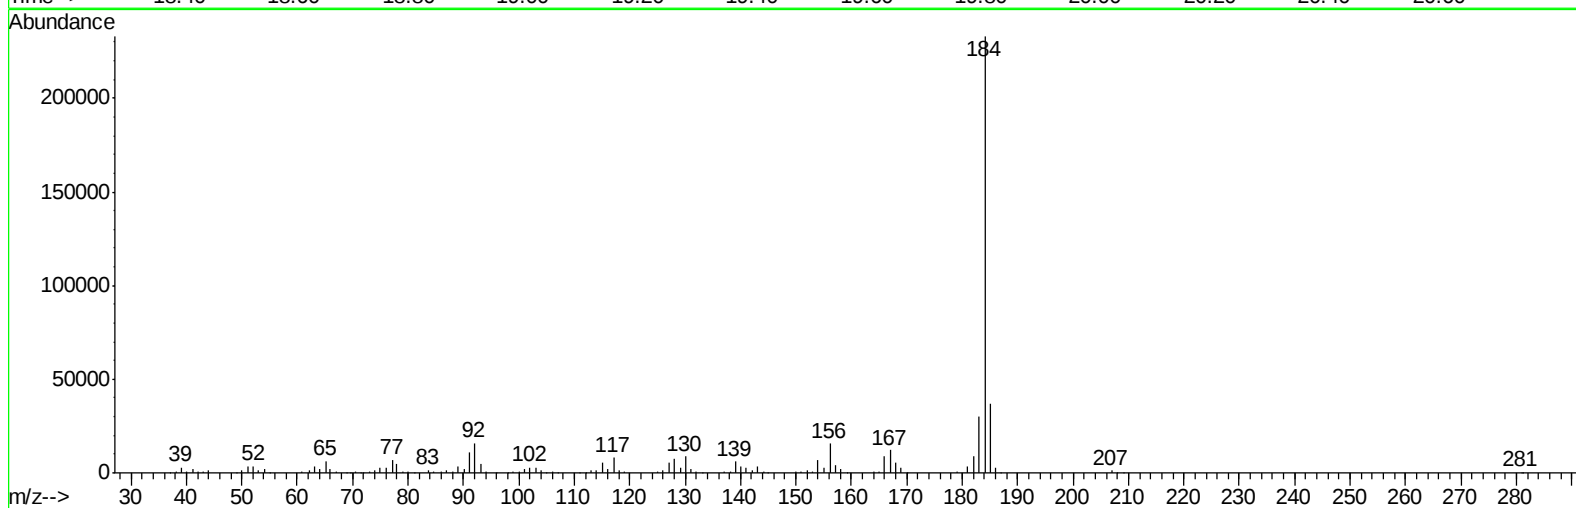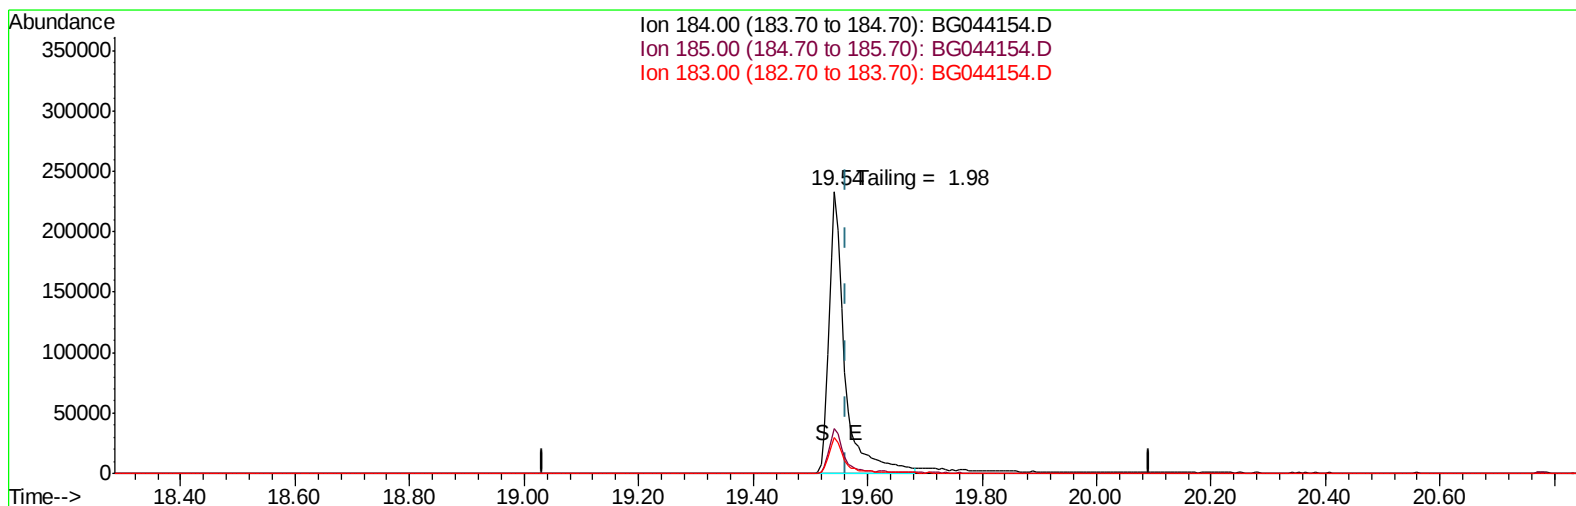

TIC: BG044154.D

(77) Benzidine

19.542min (-0.020) 0.00ng

response 450036

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.74
183.00	13.20	12.96
0.00	0.00	0.00