
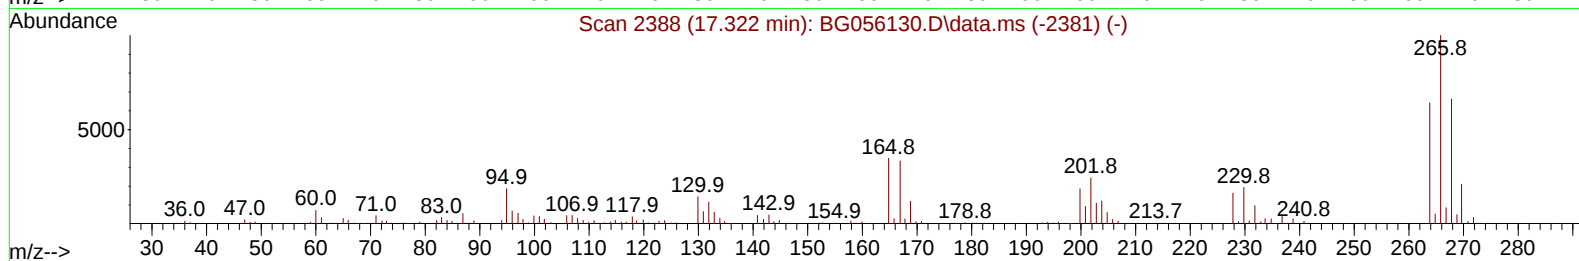
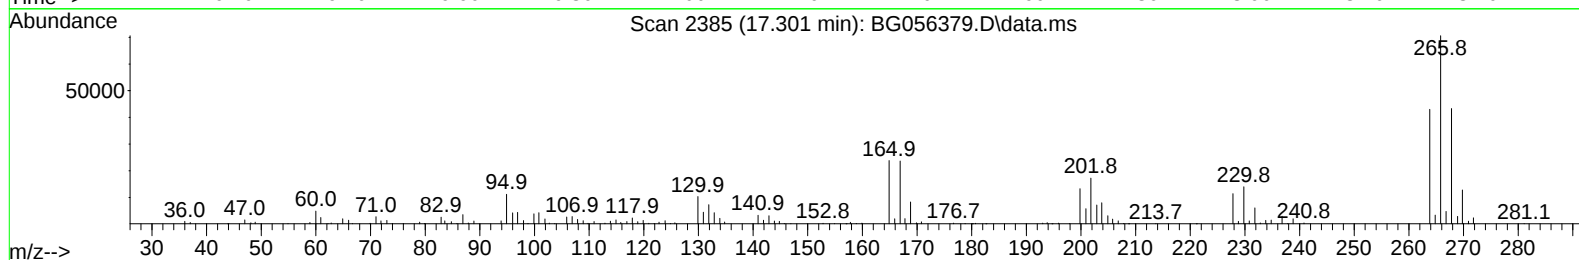


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012323\
Data File : BG056379.D
Acq On : 23 Jan 2023 10:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 04:48:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

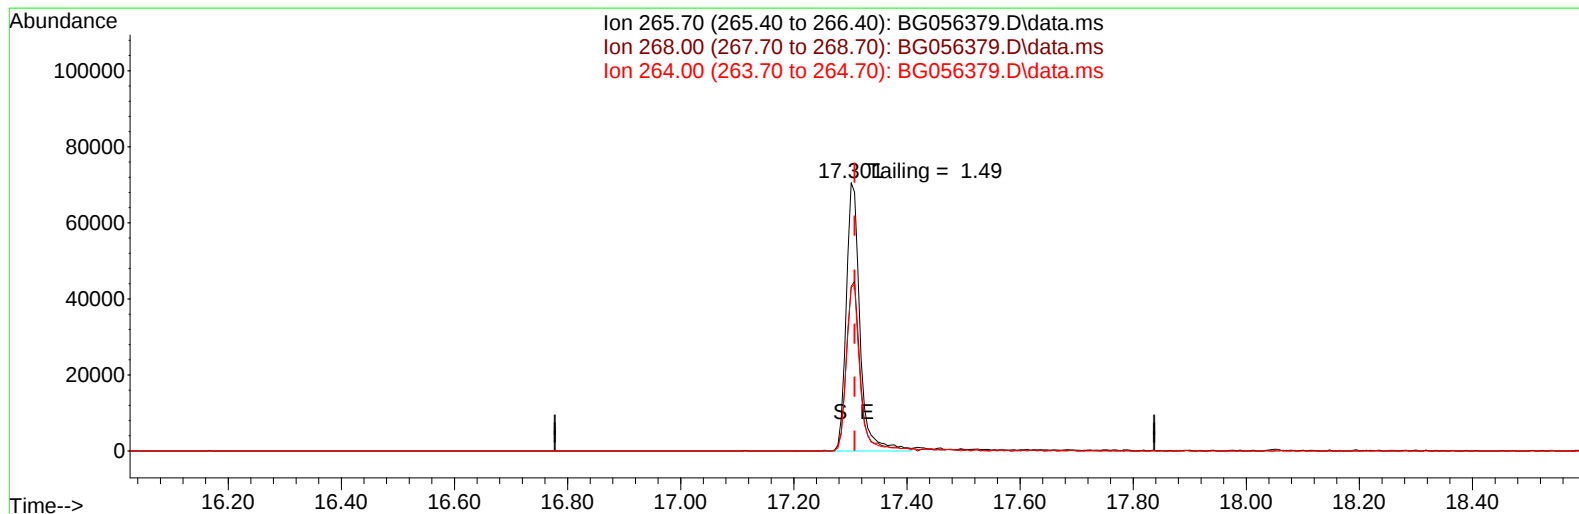

TIC: BG056379.D\data.ms

(70) Pentachlorophenol (C)




17.301min (-0.006) 207454.78 ng

response 119277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	61.37
264.00	64.30	60.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012323\
Data File : BG056379.D
Acq On : 23 Jan 2023 10:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 04:48:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

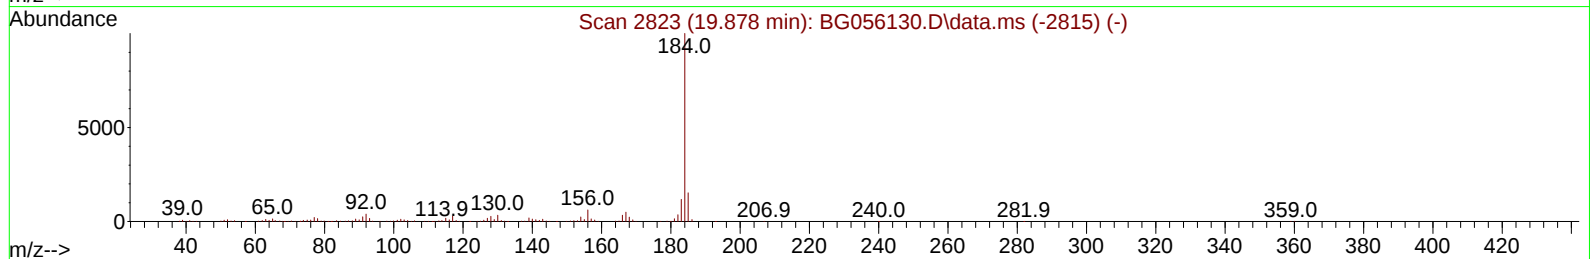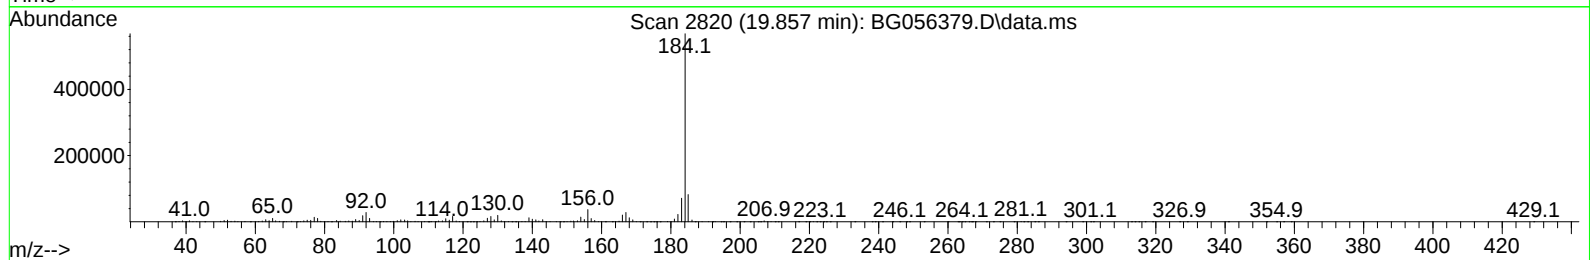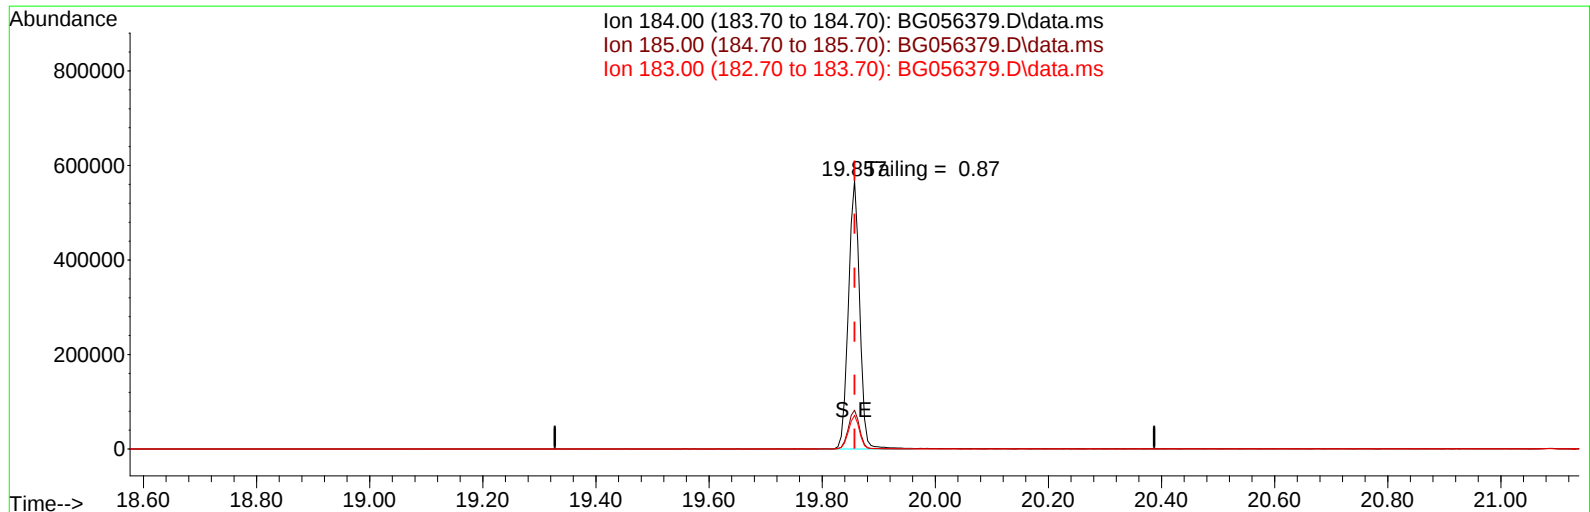

TIC: BG056379.D\data.ms

(77) Benzidine**19.857min (+ 0.000) 38441.69 ng****response 788090**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.48
183.00	11.70	12.54
0.00	0.00	0.00