

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012422\
 Data File : BG052128.D
 Acq On : 24 Jan 2022 16:13
 Operator : CG/JU
 Sample : N1199-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q09

Quant Time: Jan 24 23:59:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.245	152	28159	20.000	ng/u1	0.00
20) Naphthalene-d8	11.082	136	125064	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.889	164	84257	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.638	188	195002	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.962	240	178039	20.000	ng/u1	# 0.00
88) Perylene-d12	25.451	264	184324	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.569	96	4520	5.736	ng/uL	0.00
4) Pyridine-d5	4.004	84	17169	7.009	ng/u1	0.00
7) Phenol-d5	7.387	99	21866	7.934	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.546	67	54155	30.954	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.775	132	53521	29.331	ng/u1	0.00
15) 4-Methylphenol-d8	8.950	113	41349	19.300	ng/u1	0.00
21) Nitrobenzene-d5	9.414	128	35241	35.661	ng/u1	0.00
24) 2-Nitrophenol-d4	10.148	143	38620	35.336	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.701	165	76935	36.013	ng/u1	0.00
31) 4-Chloroaniline-d4	11.206	131	65266	21.937	ng/u1	0.00
46) Dimethylphthalate-d6	14.278	166	255992	36.757	ng/u1	0.00
49) Acenaphthylene-d8	14.584	160	326445	38.804	ng/u1	0.00
54) 4-Nitrophenol-d4	15.071	143	7927	6.808	ng/u1	0.00
60) Fluorene-d10	15.876	176	226100	37.235	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.988	200	40256	32.724	ng/u1	0.00
73) Anthracene-d10	17.738	188	352340	38.089	ng/u1	0.00
81) Pyrene-d10	20.017	212	392820	38.337	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.210	264	378042	38.959	ng/u1	0.02
Target Compounds						
					Qvalue	
41) 2,4,6-Trichlorophenol	13.326	196	2922	1.587	ng/u1	94
71) Pentachlorophenol	17.286	266	4185	2.960	ng/u1	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012422\
Data File : BG052128.D
Acq On : 24 Jan 2022 16:13
Operator : CG/JU
Sample : N1199-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q09


Quant Time: Jan 24 23:59:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

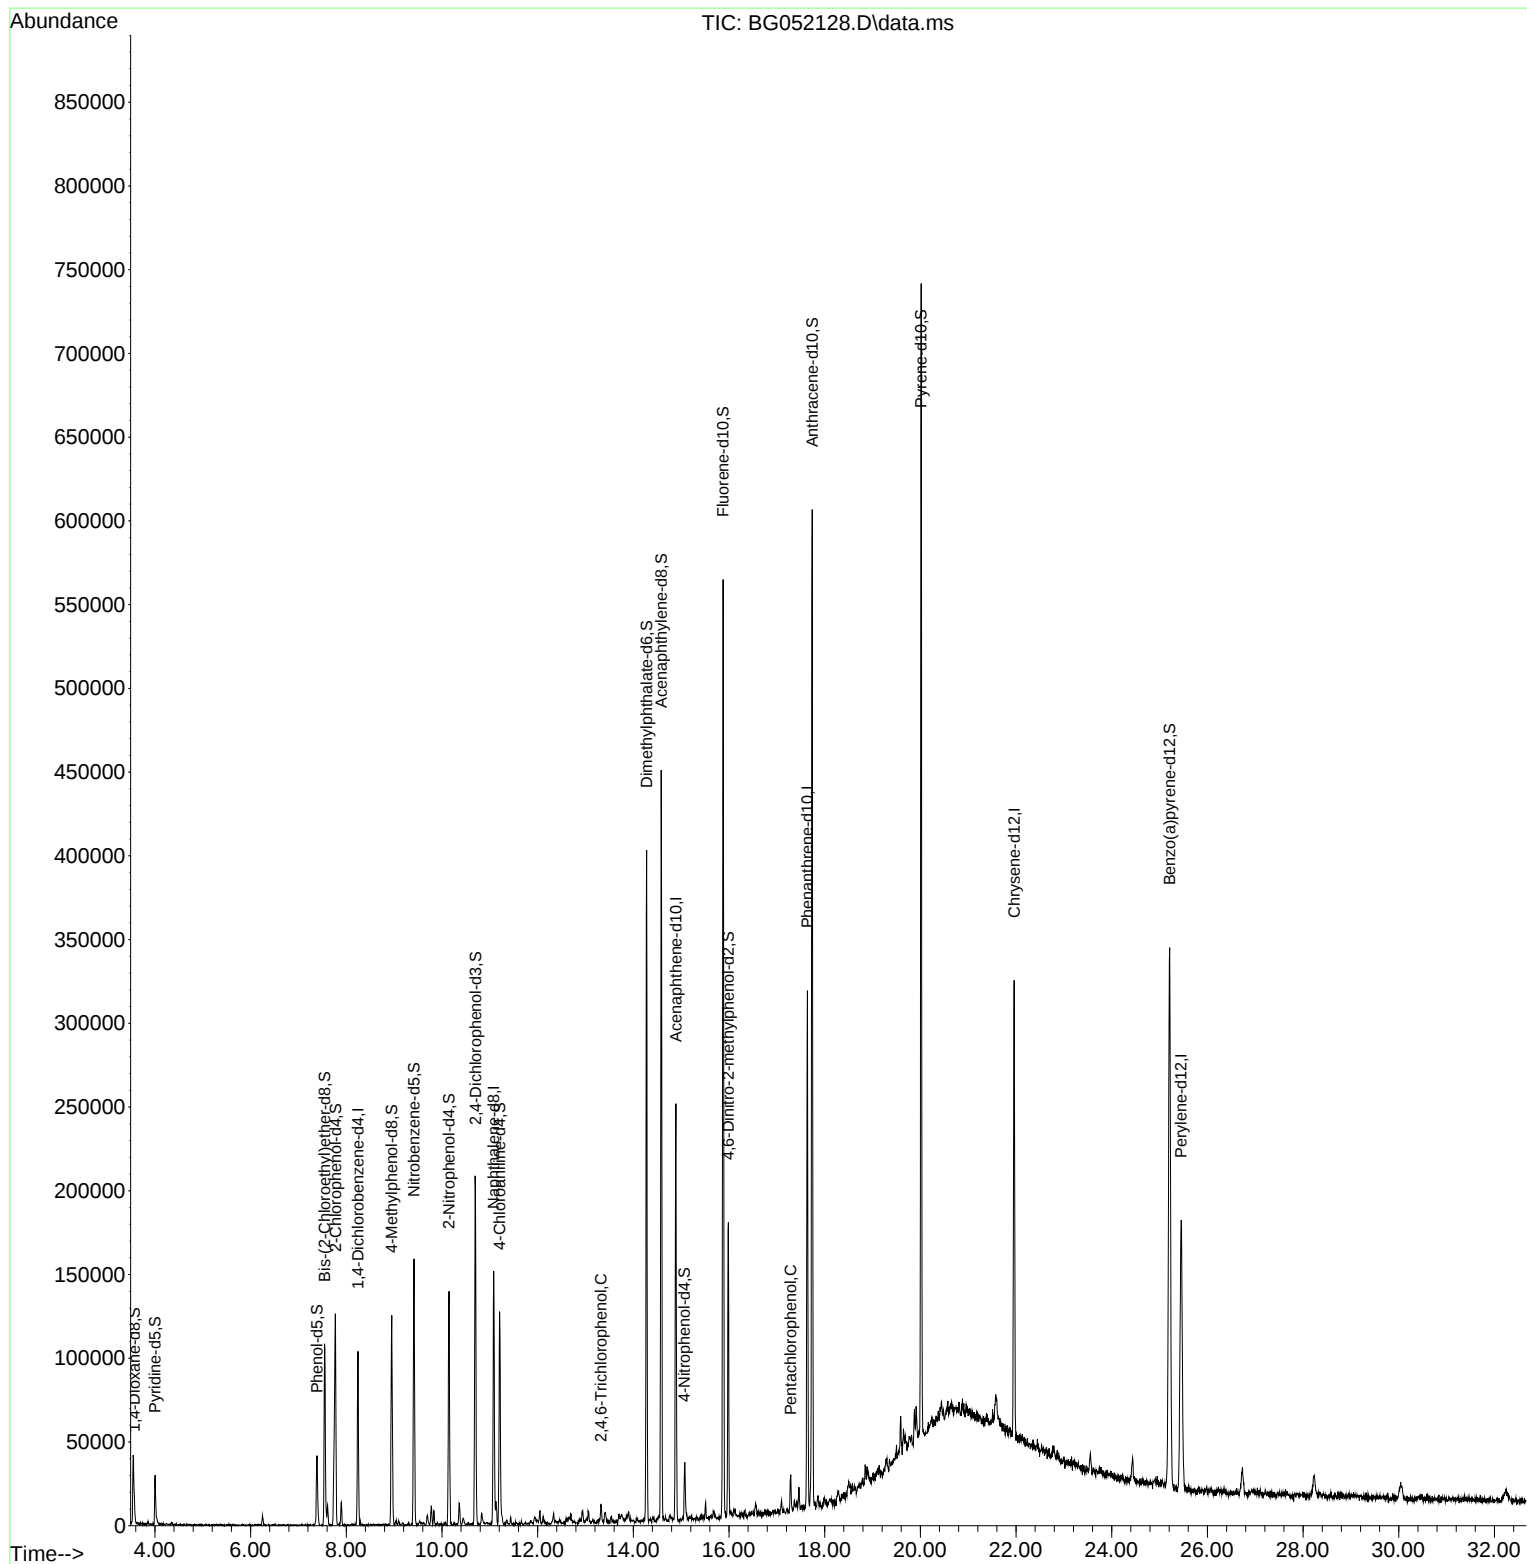



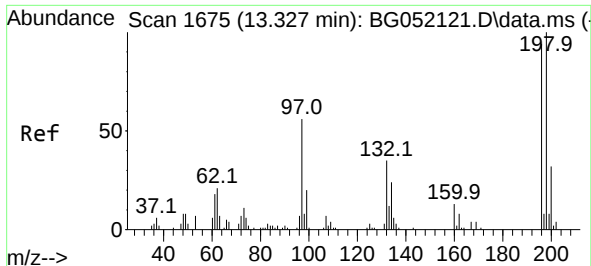


#41
2,4,6-Trichlorophenol
Concen: 1.587 ng/ul
RT: 13.326 min Scan# 1
Delta R.T. -0.002 min
Lab File: BG052128.D
Acq: 24 Jan 2022 16:13


Instrument :
BNA_G
ClientSampleId :
C0Q09

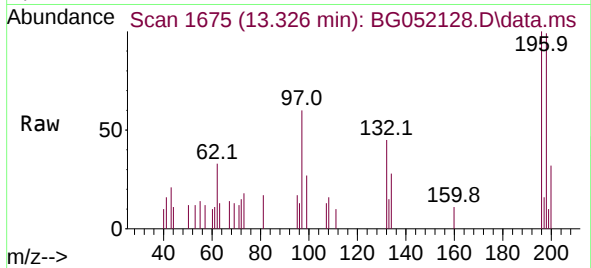

Tgt Ion:196 Resp: 2922
Ion Ratio Lower Upper
196 100
198 99.1 74.3 111.5
200 31.6 23.8 35.6

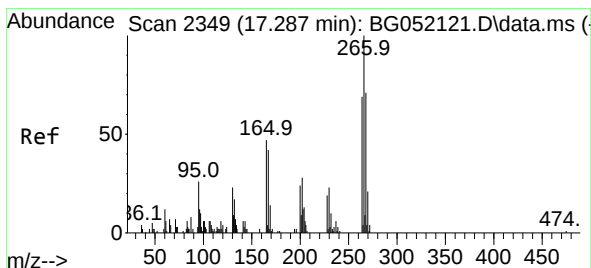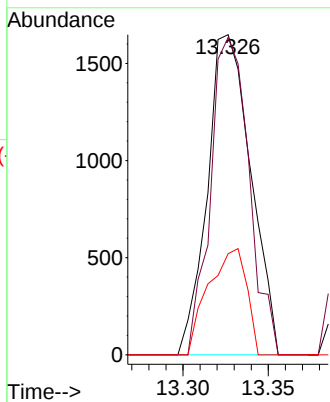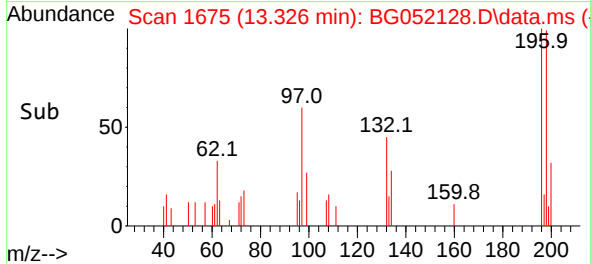

#71
Pentachlorophenol
Concen: 2.960 ng/ul
RT: 17.286 min Scan# 2349
Delta R.T. -0.002 min
Lab File: BG052128.D
Acq: 24 Jan 2022 16:13

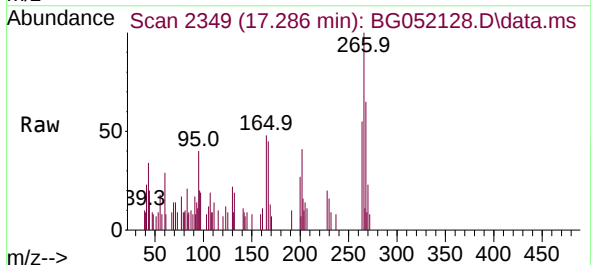

Tgt Ion:266 Resp: 4185
Ion Ratio Lower Upper
266 100
264 54.9 54.3 81.5
268 65.0 51.0 76.6

