

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012422\
 Data File : BG052122.D
 Acq On : 24 Jan 2022 12:27
 Operator : CG/JU
 Sample : PB142203BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK203

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.575	11	15	24	rVB2	9122	14581	1.43%	0.144%
2	4.004	84	88	105	rBV	112773	195055	19.15%	1.932%
3	4.356	144	148	149	rBV2	1611	1729	0.17%	0.017%
4	7.399	658	666	675	rBV	157873	267507	26.26%	2.649%
5	7.564	687	694	701	rBV	104862	175623	17.24%	1.739%
6	7.781	724	731	739	rBV	136999	237975	23.36%	2.357%
7	8.257	805	812	821	rVB	107957	174045	17.08%	1.724%
8	8.956	924	931	939	rBV	184603	318181	31.23%	3.151%
9	9.426	1003	1011	1019	rBV	149281	260410	25.56%	2.579%
10	10.155	1129	1135	1143	rBV	123968	224808	22.07%	2.226%
11	10.707	1221	1229	1239	rBV	188885	336099	32.99%	3.328%
12	11.094	1288	1295	1302	rVB	145248	258863	25.41%	2.564%
13	11.218	1308	1316	1326	rBV2	176260	332480	32.64%	3.293%
14	12.663	1557	1562	1568	rVB2	2897	5198	0.51%	0.051%
15	14.284	1831	1838	1845	rBV	372755	535306	52.54%	5.301%
16	14.590	1882	1890	1897	rBV	420359	636105	62.44%	6.299%
17	14.895	1933	1942	1950	rBV	265080	398349	39.10%	3.945%
18	15.071	1966	1972	1990	rBV	141326	253461	24.88%	2.510%
19	15.882	2102	2110	2122	rBV	532103	794703	78.01%	7.870%
20	15.988	2122	2128	2136	rBV	126123	194602	19.10%	1.927%
21	16.123	2146	2151	2157	rBV4	2050	3298	0.32%	0.033%
22	17.427	2369	2373	2376	rBV	1228	1467	0.14%	0.015%
23	17.644	2402	2410	2416	rBV	343910	515290	50.58%	5.103%
24	17.744	2419	2427	2436	rBV	572721	882275	86.60%	8.737%
25	18.749	2593	2598	2600	rBV2	952	1553	0.15%	0.015%
26	19.330	2696	2697	2701	rBV2	1321	1455	0.14%	0.014%
27	19.418	2708	2712	2714	rVB3	1014	1442	0.14%	0.014%
28	19.583	2736	2740	2745	rBV3	7081	10792	1.06%	0.107%
29	19.659	2749	2753	2757	rVB	6141	8902	0.87%	0.088%
30	20.018	2808	2814	2825	rVB	685482	1018775	100.00%	10.089%
31	21.962	3139	3145	3154	rVB	315834	530767	52.10%	5.256%
32	22.238	3190	3192	3193	rBV2	2941	1831	0.18%	0.018%
33	23.078	3333	3335	3337	rBV2	2734	1736	0.17%	0.017%
34	23.560	3413	3417	3421	rBV4	7217	10201	1.00%	0.101%
35	24.441	3562	3567	3570	rBV6	6094	11842	1.16%	0.117%
36	25.216	3688	3699	3713	rVB	315910	957894	94.02%	9.486%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012422\
Data File : BG052122.D
Acq On : 24 Jan 2022 12:27
Operator : CG/JU
Sample : PB142203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK203

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

37	25.457	3729	3740	3751	rBV	165853	518189	50.86%	5.132%
38	29.411	4411	4413	4415	rBV3	2277	1633	0.16%	0.016%
39	30.310	4562	4566	4567	rBV3	2927	3391	0.33%	0.034%




Sum of corrected areas: 10097813

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012422\
Data File : BG052122.D
Acq On : 24 Jan 2022 12:27
Operator : CG/JU
Sample : PB142203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK203

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

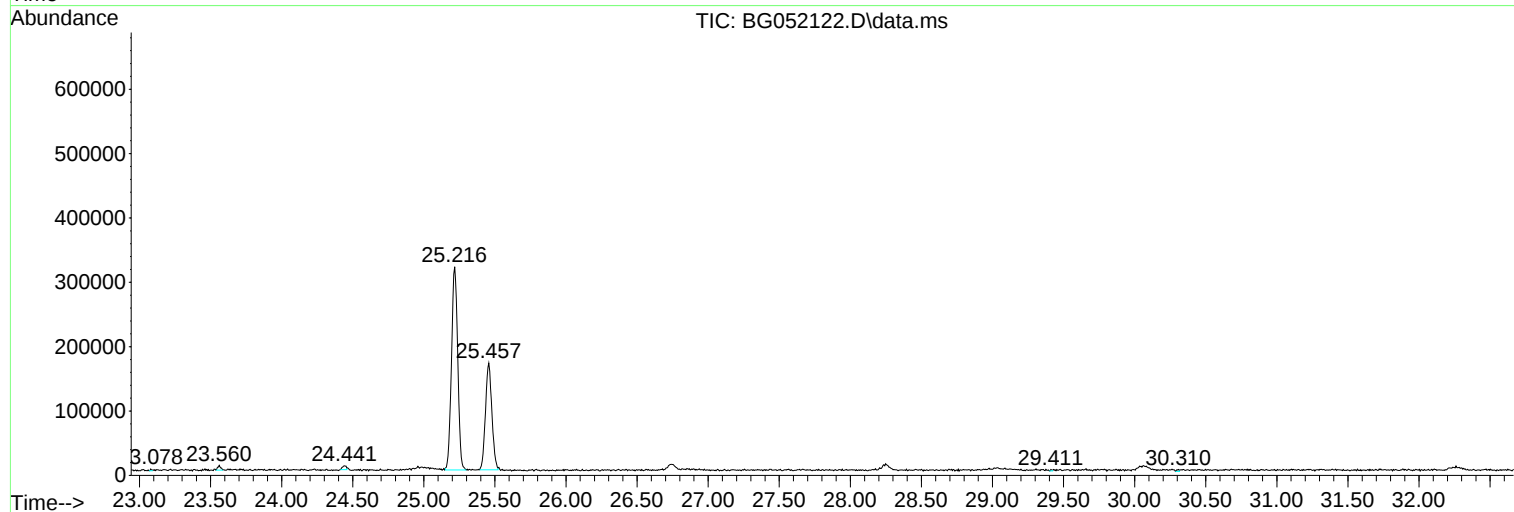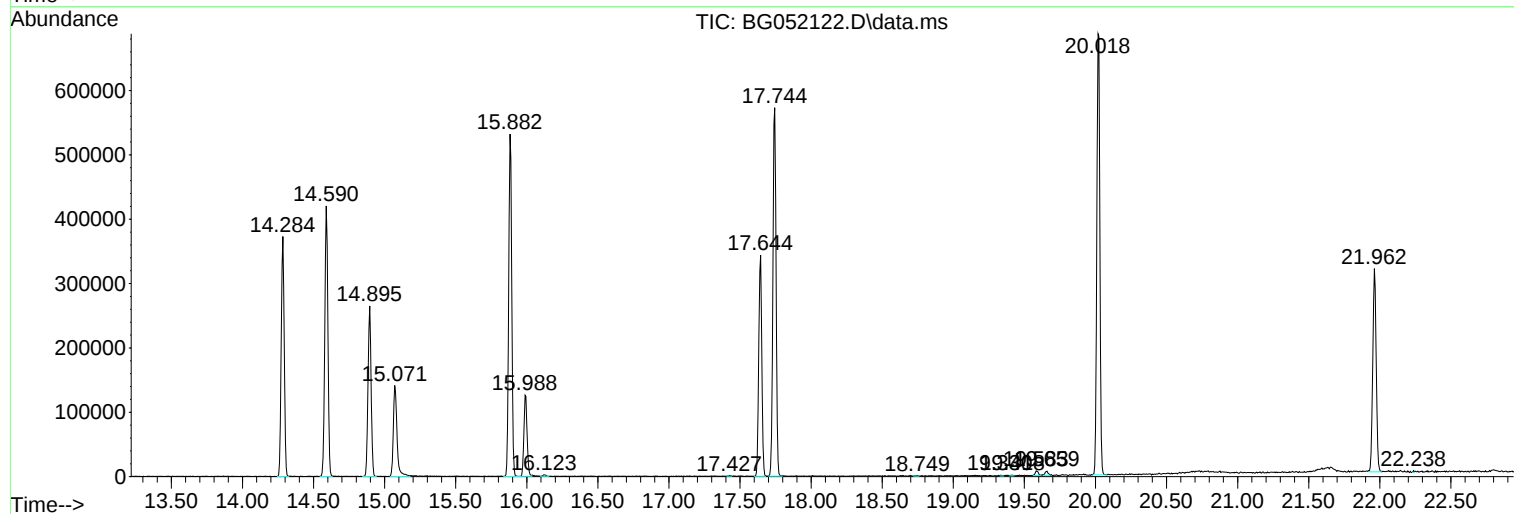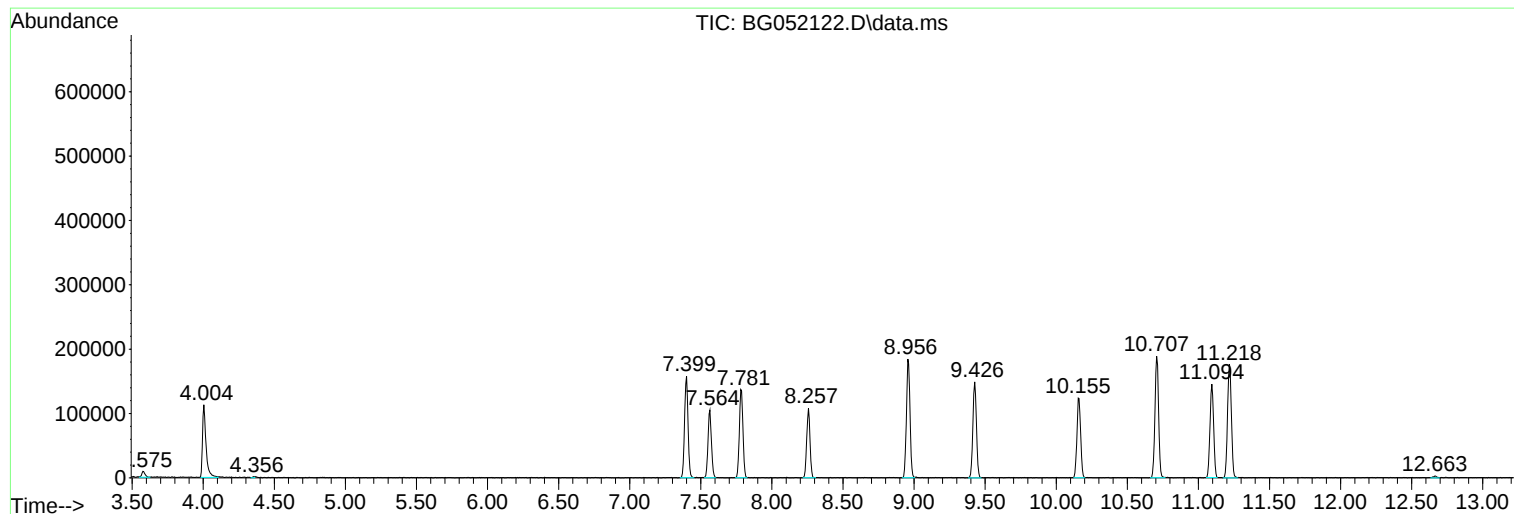

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012422\
Data File : BG052122.D
Acq On : 24 Jan 2022 12:27
Operator : CG/JU
Sample : PB142203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK203

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012422\
Data File : BG052122.D
Acq On : 24 Jan 2022 12:27
Operator : CG/JU
Sample : PB142203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK203

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc