

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012519\
 Data File : BG039281.D
 Acq On : 25 Jan 2019 16:42
 Operator : JU/SJ
 Sample : PB116613BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB116613BL

Quant Time: Jan 28 03:13:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	12133	20.00	ng	0.00
21) Naphthalene-d8	10.82	136	47832	20.00	ng	0.00
39) Acenaphthene-d10	14.65	164	33445	20.00	ng	0.00
64) Phenanthrene-d10	17.40	188	93285	20.00	ng	0.00
76) Chrysene-d12	21.67	240	139207	20.00	ng	-0.01
87) Perylene-d12	24.93	264	141842	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	91439	142.96	ng	0.00
7) Phenol-d6	7.17	99	165586	179.89	ng	0.00
23) Nitrobenzene-d5	9.18	82	71621	81.93	ng	0.00
42) 2,4,6-Tribromophenol	16.14	330	67939	121.18	ng	-0.01
45) 2-Fluorobiphenyl	13.27	172	213652	87.43	ng	0.00
79) Terphenyl-d14	20.00	244	522927	69.49	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.19	70	9689	16.030	ng	# 67
51) 2,6-Dinitrotoluene	14.65	165	3930	6.220	ng	# 24
57) 2,4-Dinitrotoluene	14.65	165	3930	4.335	ng	# 26
67) 4-Bromophenyl-phenylether	16.14	248	4383	3.655	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012519\
Data File : BG039281.D
Acq On : 25 Jan 2019 16:42
Operator : JU/SJ
Sample : PB116613BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB116613BL

Quant Time: Jan 28 03:13:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

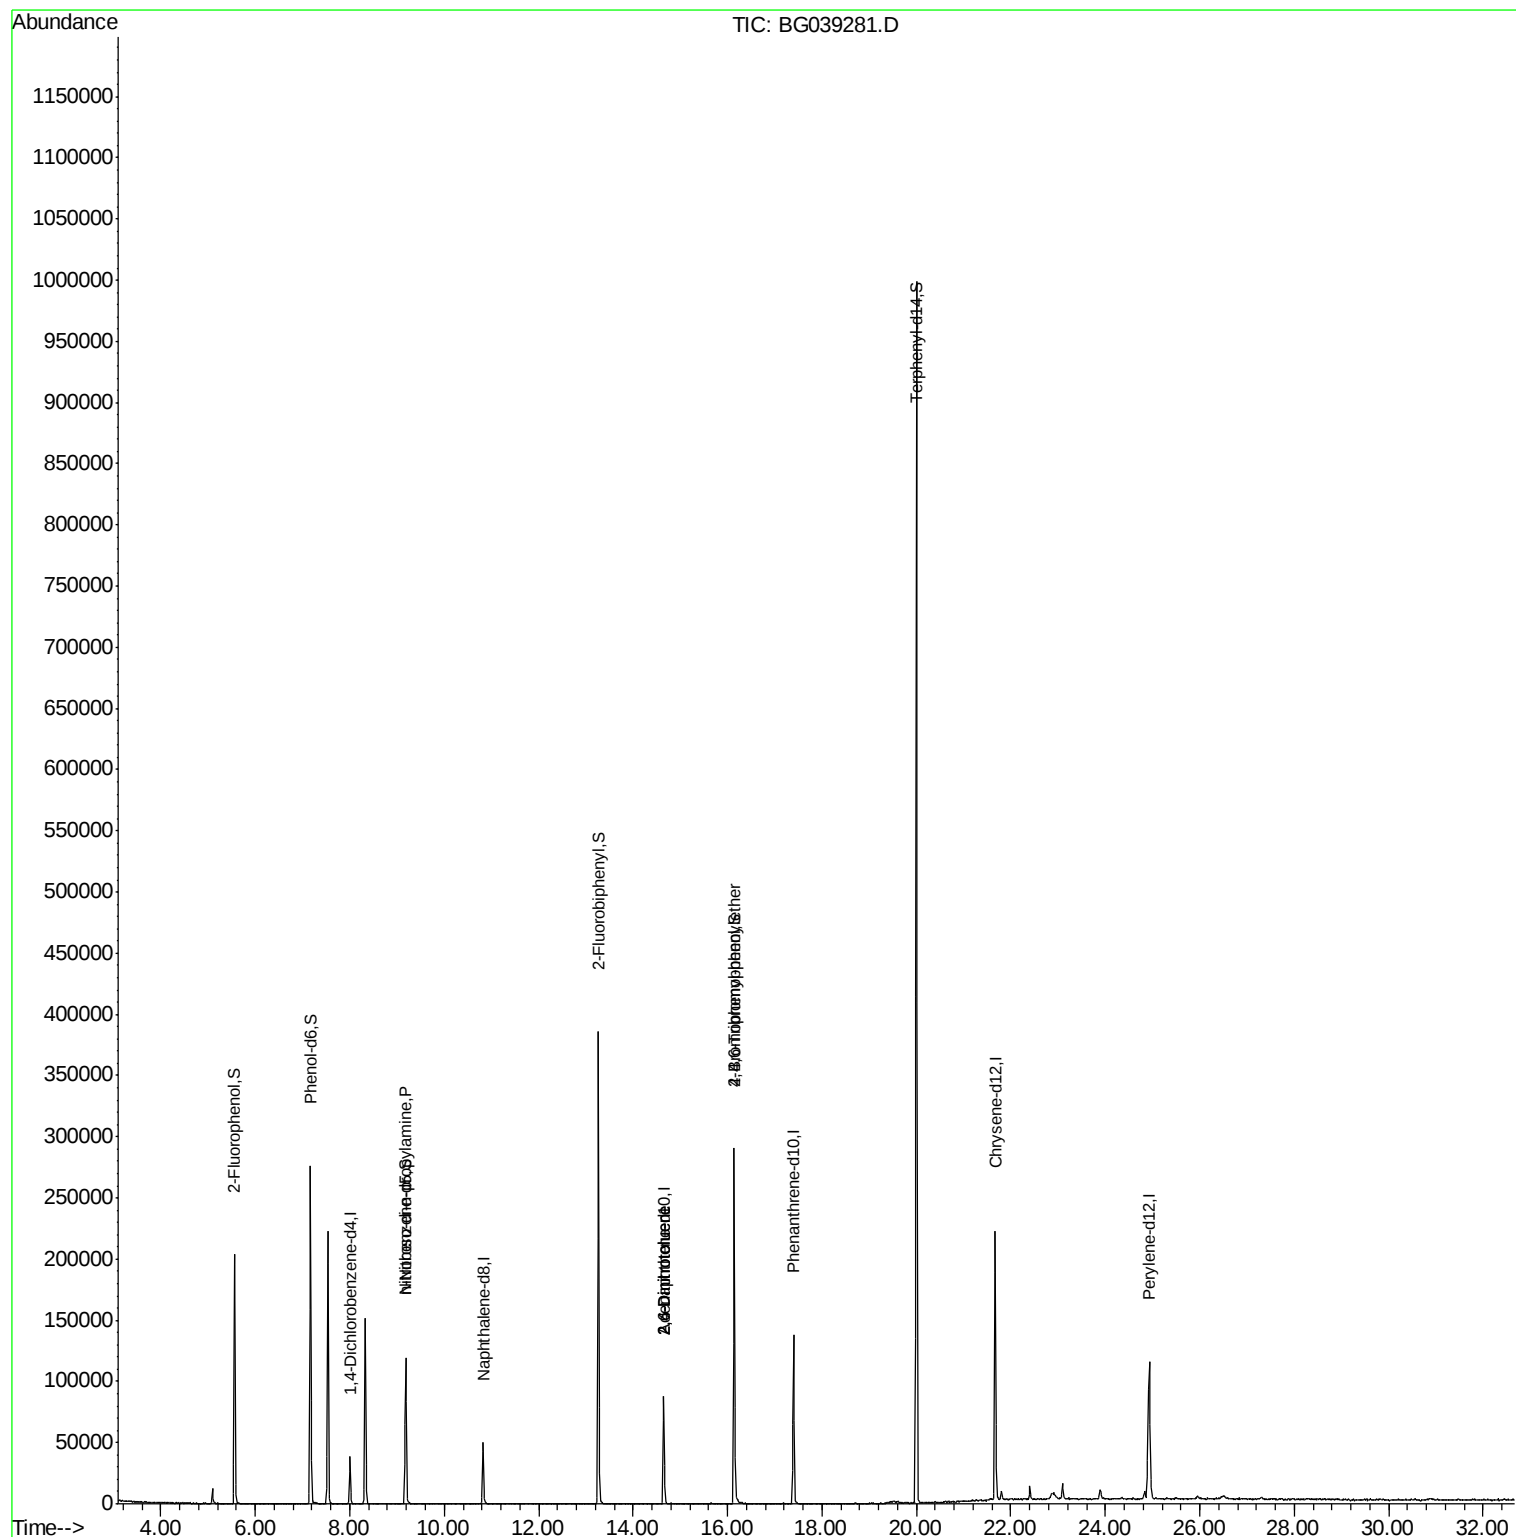

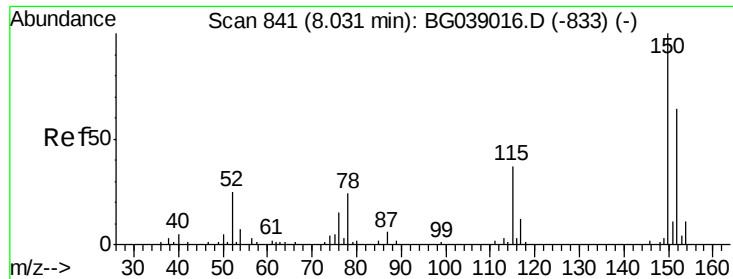


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 837
Delta R.T. -0.01 min
Lab File: BG039281.D
Acq: 25 Jan 2019 16:42

Instrument :
BNA_G
ClientSampleId :
PB116613BL

Tgt Ion	Ratio	Lower	Upper
152	100		
150	150.8	124.7	187.1
115	46.3	46.5	69.7

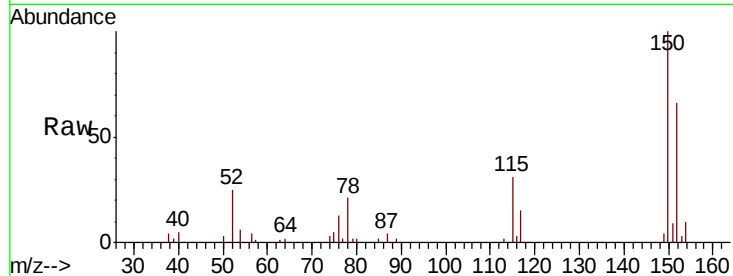


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

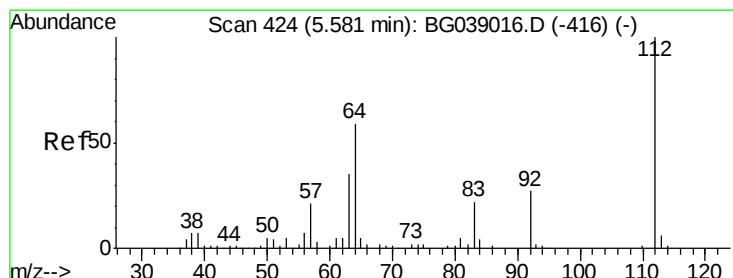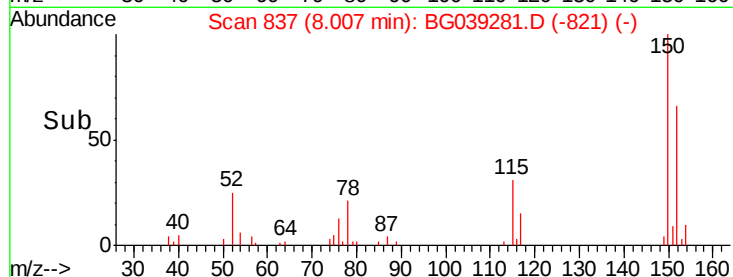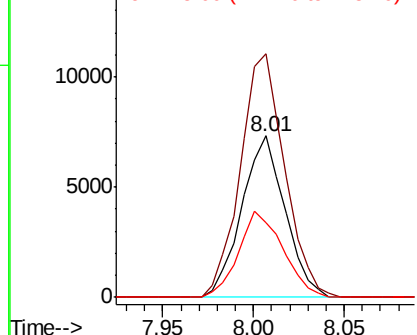



#5


2-Fluorophenol
Concen: 142.964 ng
RT: 5.56 min Scan# 420
Delta R.T. -0.01 min
Lab File: BG039281.D
Acq: 25 Jan 2019 16:42

Tgt Ion	Ratio	Lower	Upper
112	100		
64	63.0	47.0	70.6
63	35.9	28.0	42.0

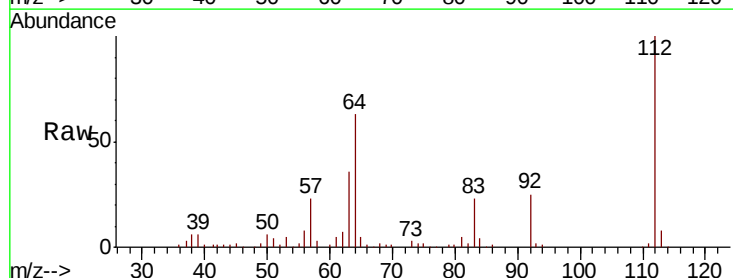

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

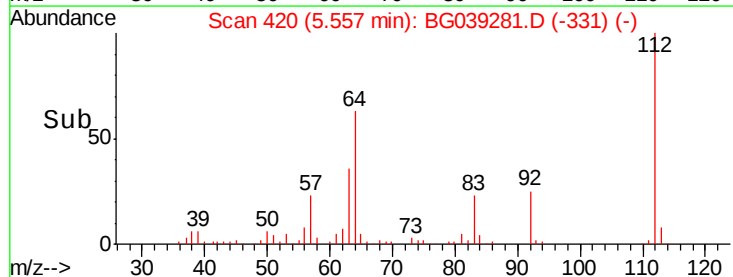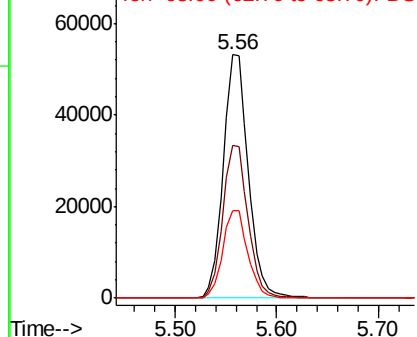

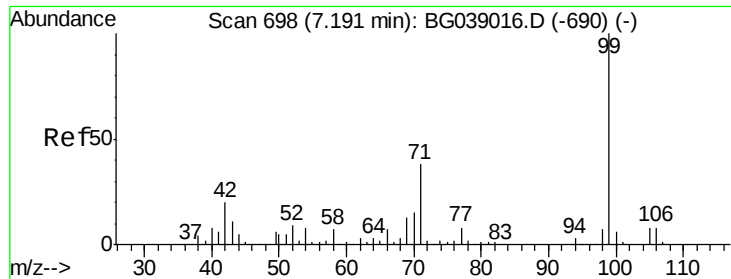

#7

Phenol-d6

Concen: 179.895 ng

RT: 7.17 min Scan# 694

Delta R.T. -0.01 min

Lab File: BG039281.D

Acq: 25 Jan 2019 16:42

Instrument :

BNA_G

ClientSampleId :

PB116613BL


Tgt Ion: 99 Resp: 165586

Ion Ratio Lower Upper




99 100

42 19.1 15.8 23.6

71 35.0 30.2 45.4

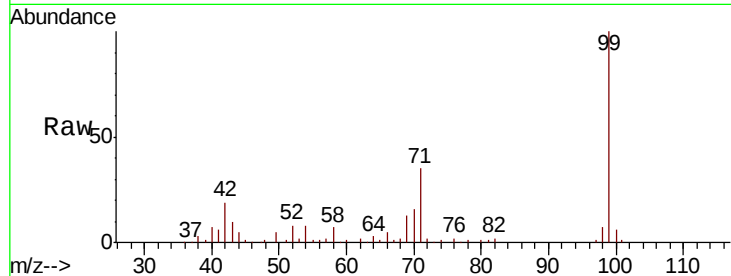

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

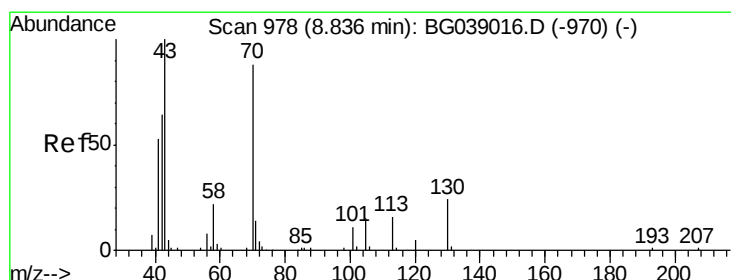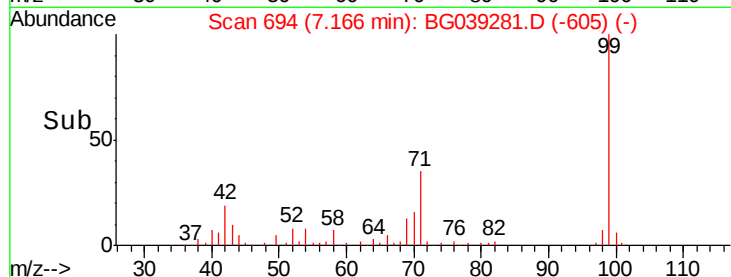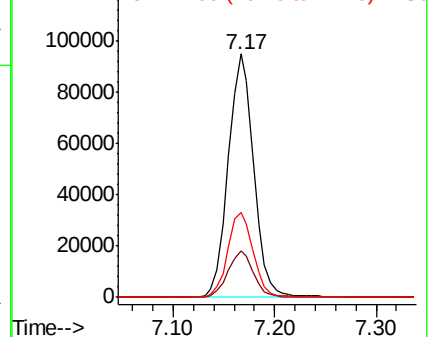

#19

n-Nitroso-di-n-propylamine

Concen: 16.030 ng

RT: 9.19 min Scan# 1038

Delta R.T. 0.37 min

Lab File: BG039281.D

Acq: 25 Jan 2019 16:42

Tgt Ion: 70 Resp: 9689


Ion Ratio Lower Upper

70 100



42 51.5 59.0 88.4#


101 0.0 10.4 15.6#

130 0.0 21.6 32.4#

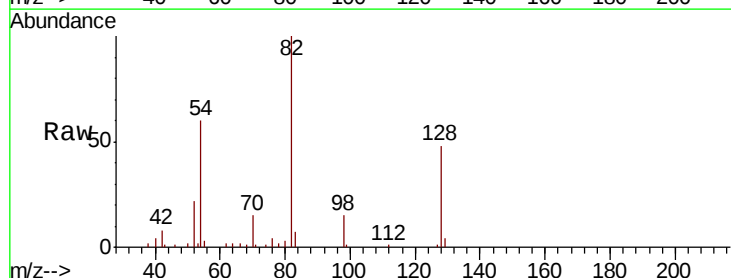

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

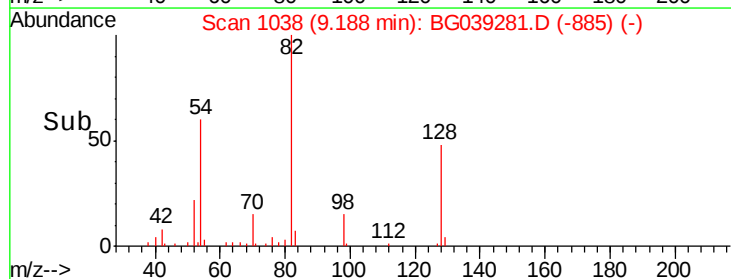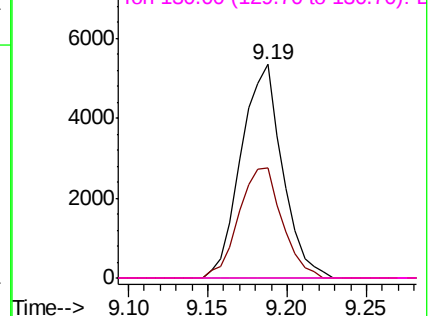


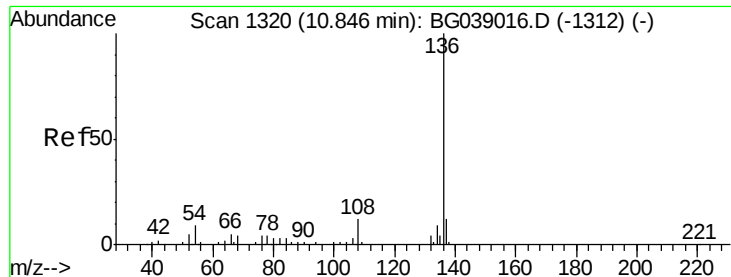




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.82 min Scan# 1316
Delta R.T. -0.01 min
Lab File: BG039281.D
Acq: 25 Jan 2019 16:42

Instrument :
BNA_G
ClientSampleId :
PB116613BL

Tgt Ion:	136	Resp:	47832
Ion	Ratio	Lower	Upper
136	100		
137	10.9	9.4	14.2
54	9.5	7.2	10.8
68	4.1	3.5	5.3

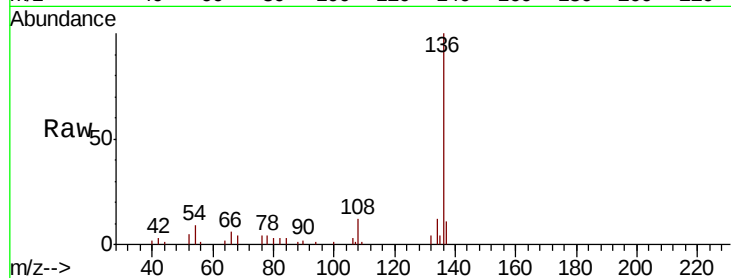


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BG
Ion 68.00 (67.70 to 68.70): BG

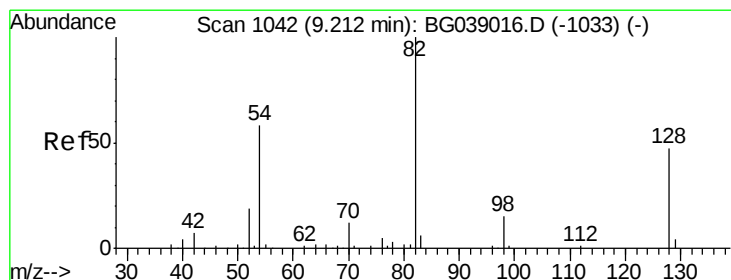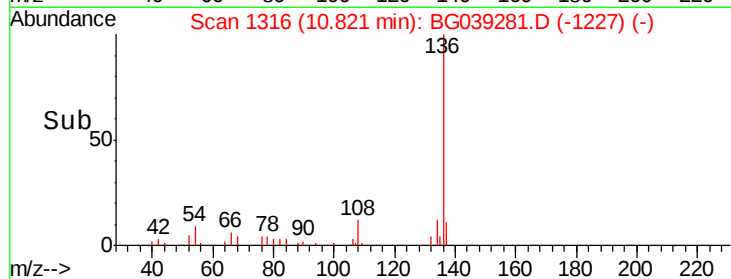
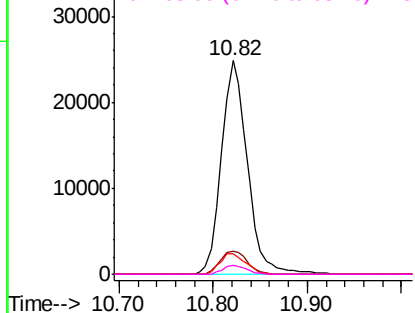



#23
Nitrobenzene-d5
Concen: 81.934 ng
RT: 9.18 min Scan# 1037
Delta R.T. -0.01 min
Lab File: BG039281.D
Acq: 25 Jan 2019 16:42

Tgt Ion:	82	Resp:	71621
Ion	Ratio	Lower	Upper
82	100		
128	46.3	37.3	55.9
54	63.4	46.4	69.6

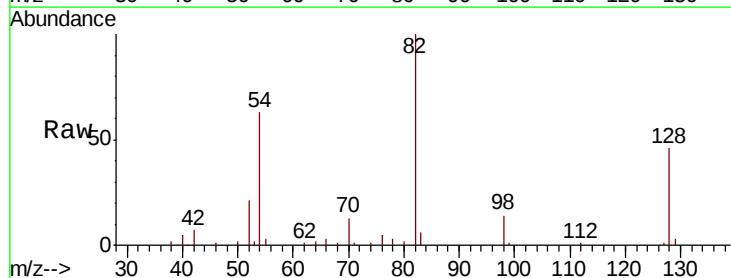

Abundance Ion 82.00 (81.70 to 82.70): BG
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BG

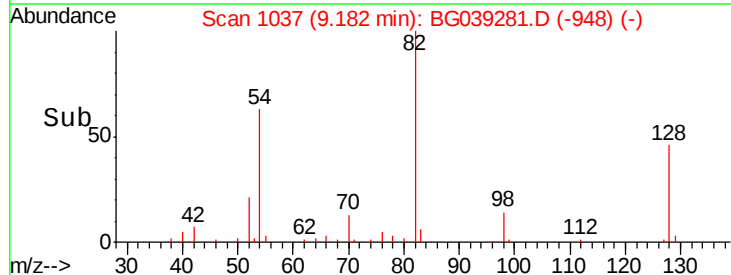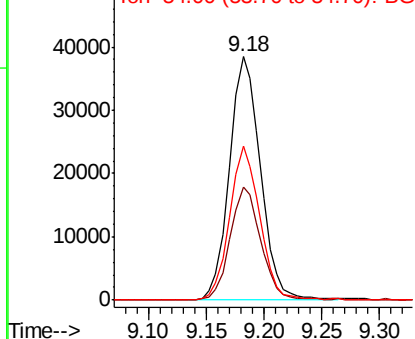

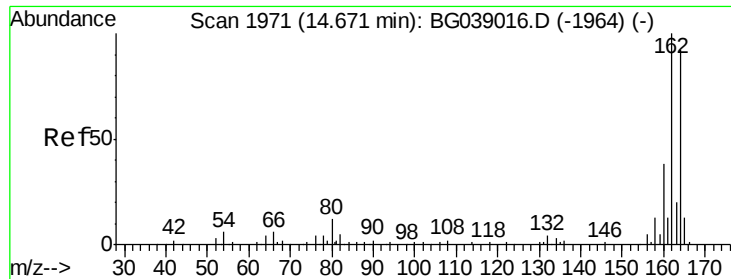

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.65 min Scan# 1967

Delta R.T. -0.01 min

Lab File: BG039281.D

Acq: 25 Jan 2019 16:42

Instrument :

BNA_G

ClientSampleId :

PB116613BL


Tgt Ion:164 Resp: 33445

Ion Ratio Lower Upper




164 100

162 102.4 87.2 130.8

160 44.4 33.3 49.9

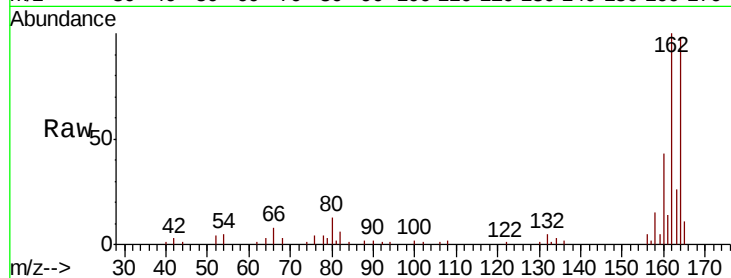

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

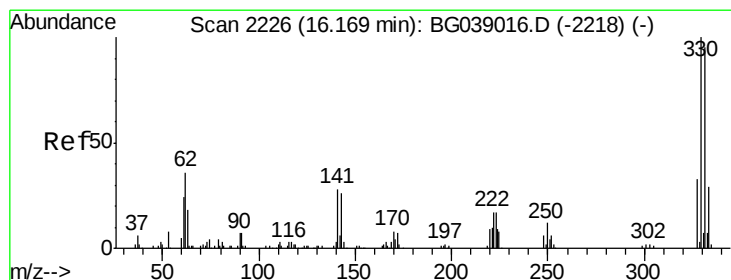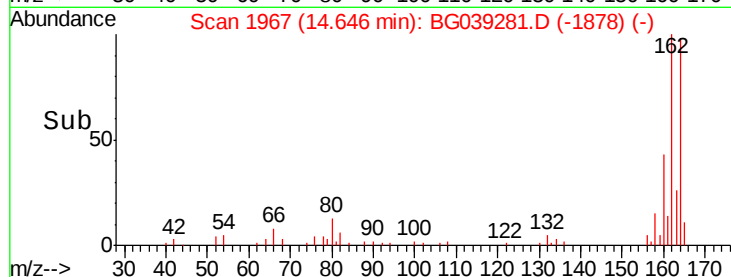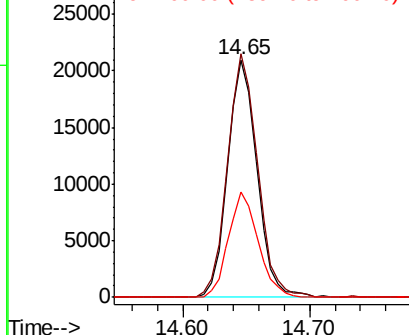

#42

2,4,6-Tribromophenol

Concen: 121.183 ng

RT: 16.14 min Scan# 2221

Delta R.T. -0.01 min

Lab File: BG039281.D

Acq: 25 Jan 2019 16:42


Tgt Ion:330 Resp: 67939

Ion Ratio Lower Upper



330 100


332 96.5 75.7 113.5

141 30.6 24.9 37.3

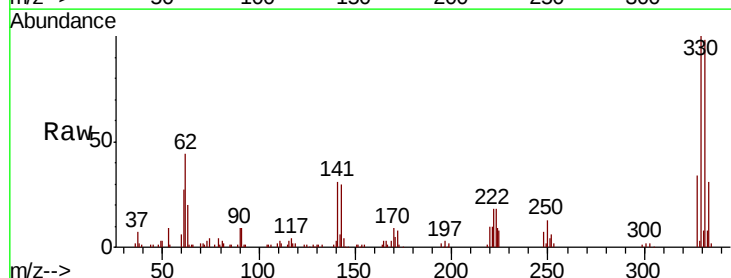

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

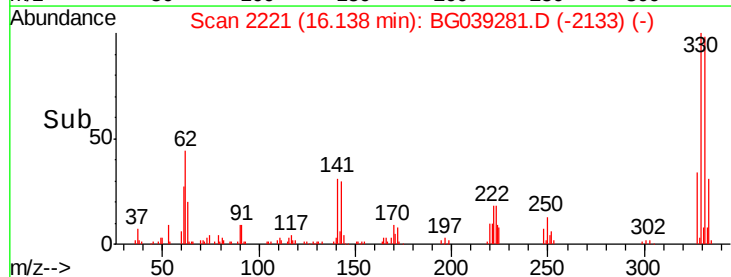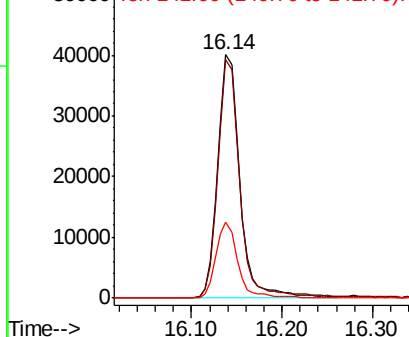


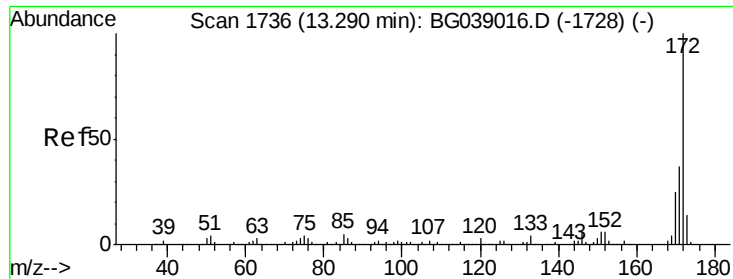




#45
 2-Fluorobiphenyl
 Concen: 87.426 ng
 RT: 13.27 min Scan# 1732
 Delta R.T. -0.01 min
 Lab File: BG039281.D
 Acq: 25 Jan 2019 16:42

Instrument :
 BNA_G
 ClientSampleId :
 PB116613BL

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	29.4	44.0
170	23.2	20.1	30.1

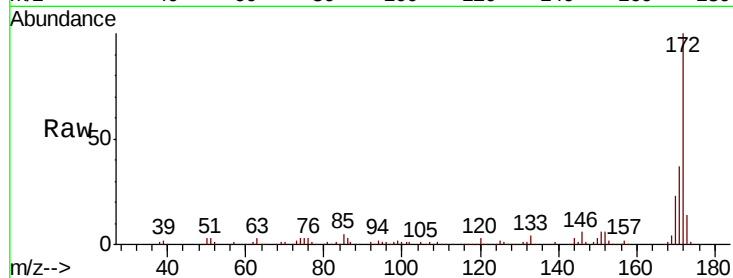


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

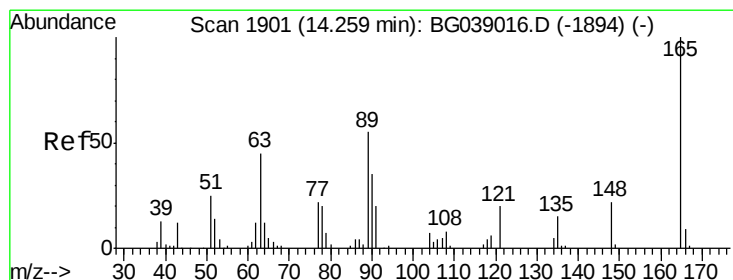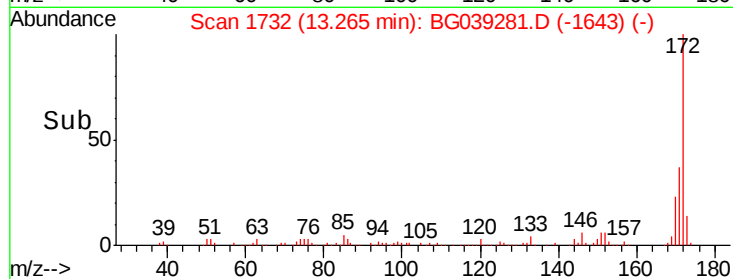
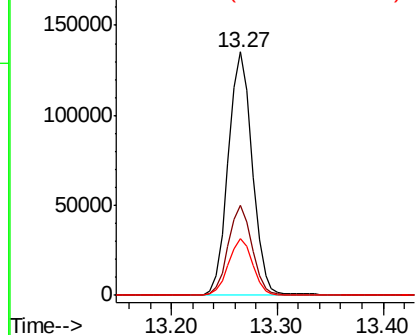



#51
 2,6-Dinitrotoluene
 Concen: 6.220 ng
 RT: 14.65 min Scan# 1967
 Delta R.T. 0.40 min
 Lab File: BG039281.D
 Acq: 25 Jan 2019 16:42

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	43.6	65.4#
89	0.0	43.7	65.5#

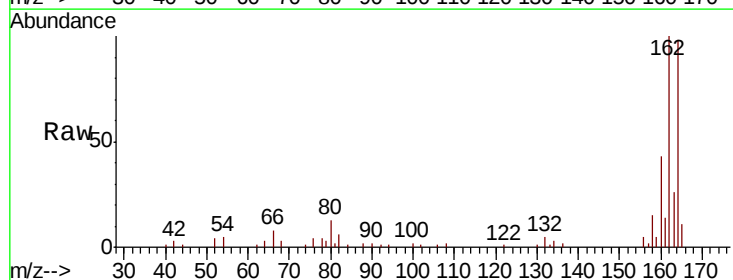

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BG
 Ion 89.00 (88.70 to 89.70): BG

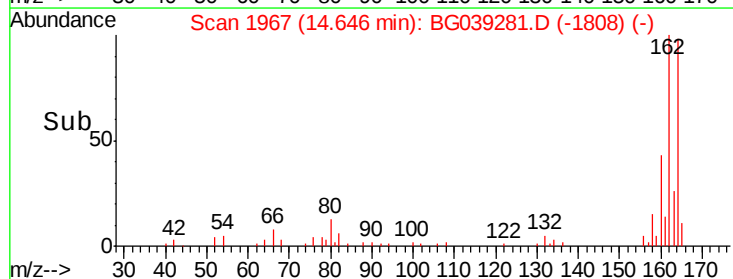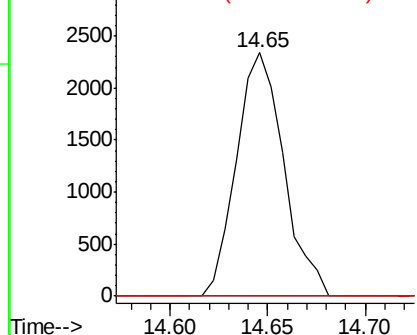


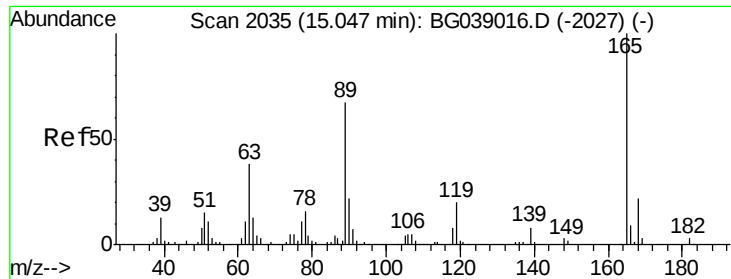




#57
 2,4-Dinitrotoluene
 Concen: 4.335 ng
 RT: 14.65 min Scan# 1967
 Delta R.T. -0.38 min
 Lab File: BG039281.D
 Acq: 25 Jan 2019 16:42

Instrument :
 BNA_G
 ClientSampleId :
 PB116613BL

Tgt Ion:165 Resp: 3930
 Ion Ratio Lower Upper
 165 100
 63 0.0 30.2 45.4#
 89 0.0 53.2 79.8#
 182 0.0 2.7 4.1#

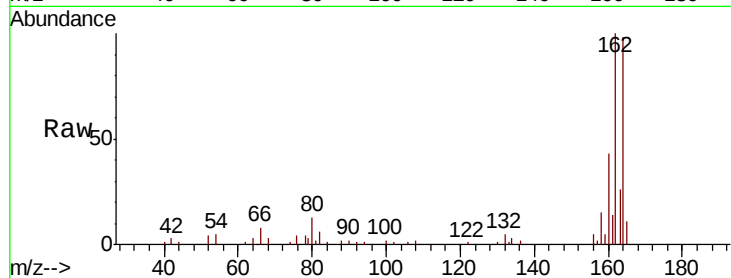


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

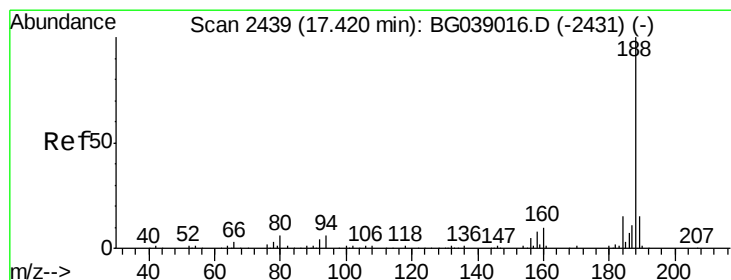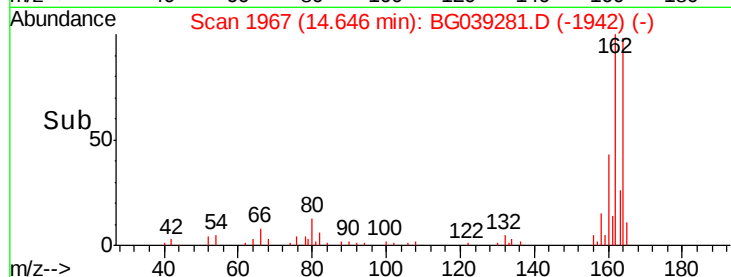
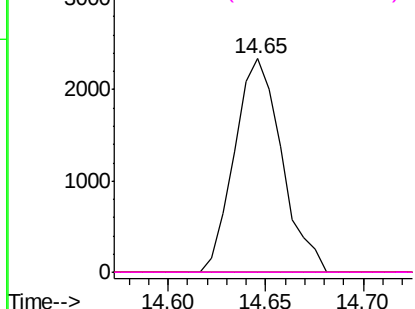



#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.40 min Scan# 2435
 Delta R.T. -0.01 min
 Lab File: BG039281.D
 Acq: 25 Jan 2019 16:42

Tgt Ion:188 Resp: 93285
 Ion Ratio Lower Upper
 188 100
 94 6.2 5.0 7.4
 80 6.0 4.7 7.1

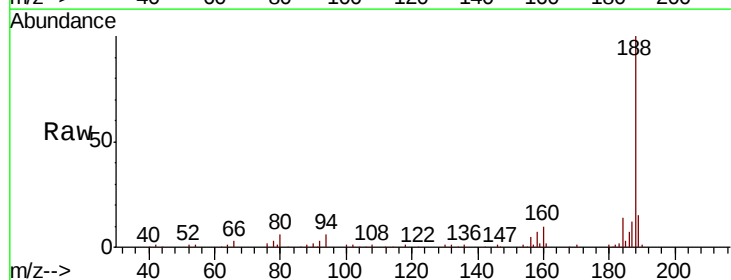

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

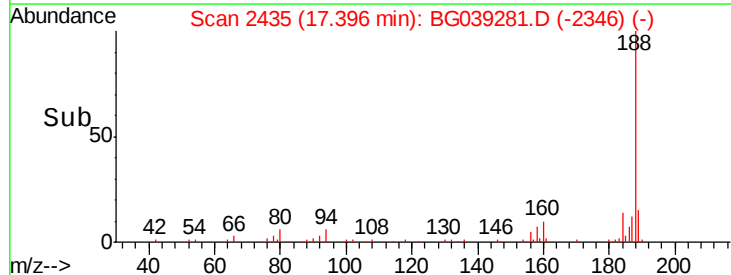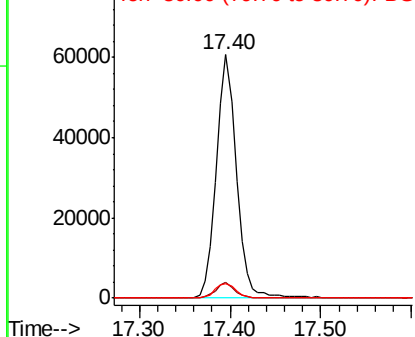


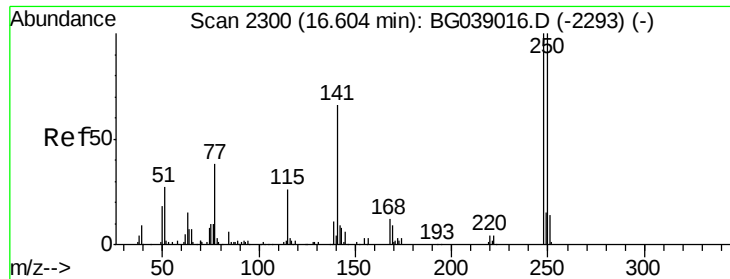




#67
 4-Bromophenyl-phenylether
 Concen: 3.655 ng
 RT: 16.14 min Scan# 2221
 Delta R.T. -0.45 min
 Lab File: BG039281.D
 Acq: 25 Jan 2019 16:42

Instrument :
 BNA_G
 ClientSampleId :
 PB116613BL

Tgt Ion:248 Resp: 4383
 Ion Ratio Lower Upper
 248 100
 250 189.3 79.9 119.9#
 141 350.3 52.7 79.1#

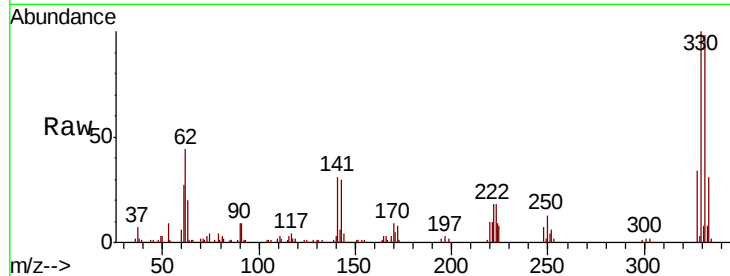


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

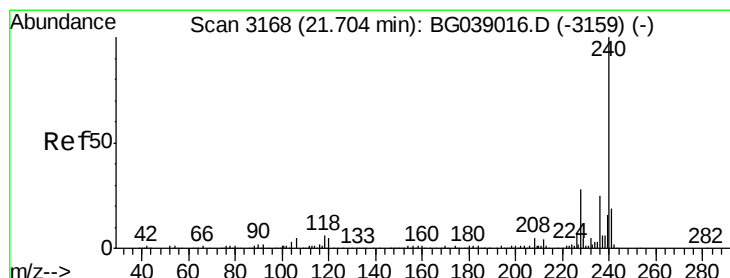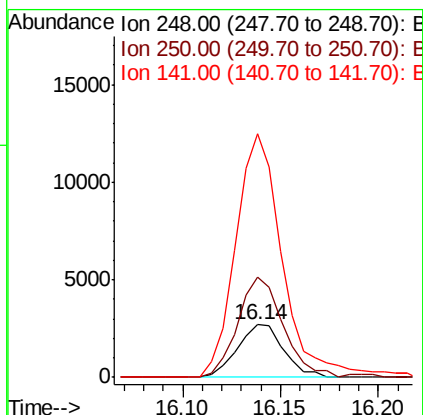
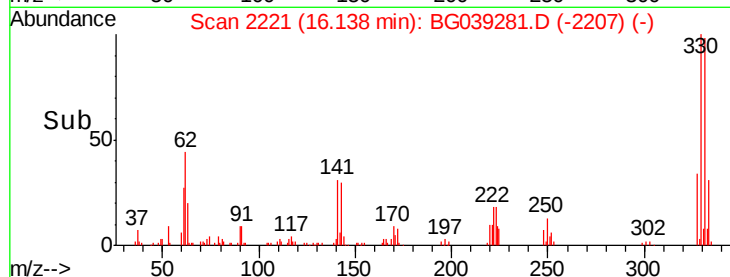



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.67 min Scan# 3162
 Delta R.T. -0.01 min
 Lab File: BG039281.D
 Acq: 25 Jan 2019 16:42

Tgt Ion:240 Resp: 139207
 Ion Ratio Lower Upper
 240 100
 120 8.5 4.3 6.5#
 236 27.4 20.1 30.1

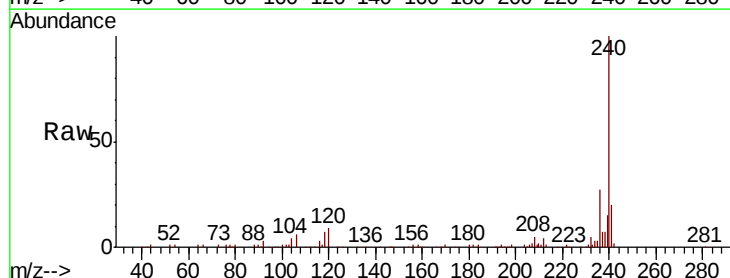

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

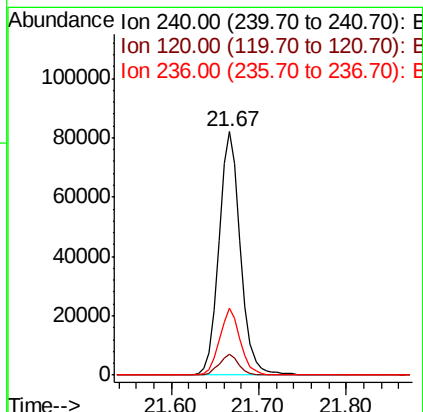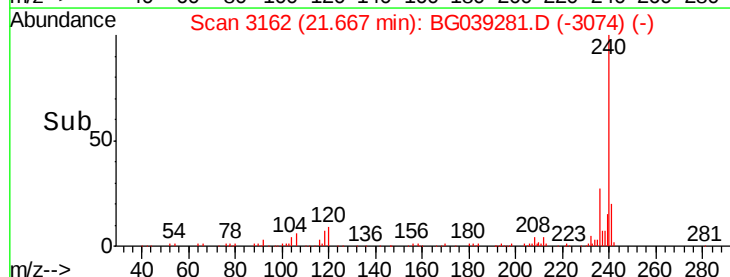

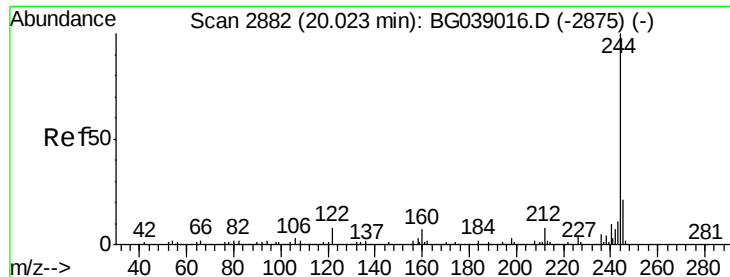

#79

Terphenyl-d14

Concen: 69.491 ng

RT: 20.00 min Scan# 2878

Delta R.T. -0.01 min

Lab File: BG039281.D

Acq: 25 Jan 2019 16:42

Instrument :

BNA_G

ClientSampleId :

PB116613BL


Tgt Ion:244 Resp: 522927

Ion Ratio Lower Upper

244 100

212 7.1 6.1 9.1




122 6.8 6.1 9.1

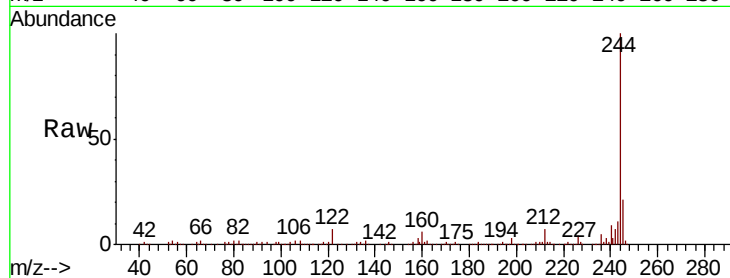

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

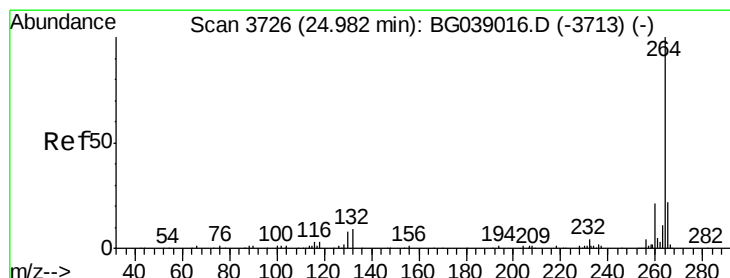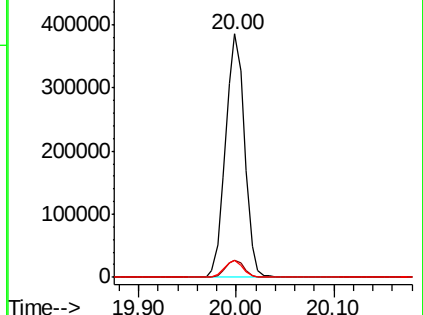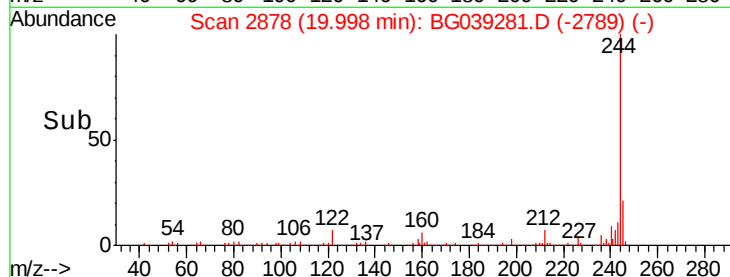

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3717

Delta R.T. -0.02 min

Lab File: BG039281.D

Acq: 25 Jan 2019 16:42


Tgt Ion:264 Resp: 141842

Ion Ratio Lower Upper

264 100

260 22.2 17.0 25.6

265 22.9 17.2 25.8

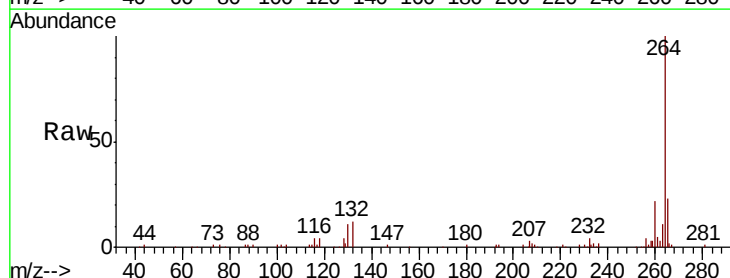

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

