

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012519\
 Data File : BG039290.D
 Acq On : 25 Jan 2019 22:38
 Operator : JU/SJ
 Sample : PB116630TB
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB116630TB

Quant Time: Jan 28 03:15:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	14381	20.00	ng	0.00
21) Naphthalene-d8	10.82	136	56093	20.00	ng	0.00
39) Acenaphthene-d10	14.64	164	36124	20.00	ng	0.00
64) Phenanthrene-d10	17.39	188	100986	20.00	ng	0.00
76) Chrysene-d12	21.67	240	123412	20.00	ng	-0.02
87) Perylene-d12	24.92	264	139734	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	85747	113.11	ng	0.00
7) Phenol-d6	7.16	99	119274	109.33	ng	0.00
23) Nitrobenzene-d5	9.18	82	69560	67.86	ng	0.00
42) 2,4,6-Tribromophenol	16.14	330	51184	84.53	ng	-0.02
45) 2-Fluorobiphenyl	13.26	172	193173	73.18	ng	0.00
79) Terphenyl-d14	20.00	244	473956	71.04	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.18	70	8828	12.322	ng	# 68
51) 2,6-Dinitrotoluene	14.64	165	4819	7.061	ng	# 24
57) 2,4-Dinitrotoluene	14.64	165	4819	4.922	ng	# 26
67) 4-Bromophenyl-phenylether	16.14	248	3038	2.340	ng	# 1
77) Benzidine	20.00	184	7607	2.015	ng	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012519\
Data File : BG039290.D
Acq On : 25 Jan 2019 22:38
Operator : JU/SJ
Sample : PB116630TB
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB116630TB

Quant Time: Jan 28 03:15:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

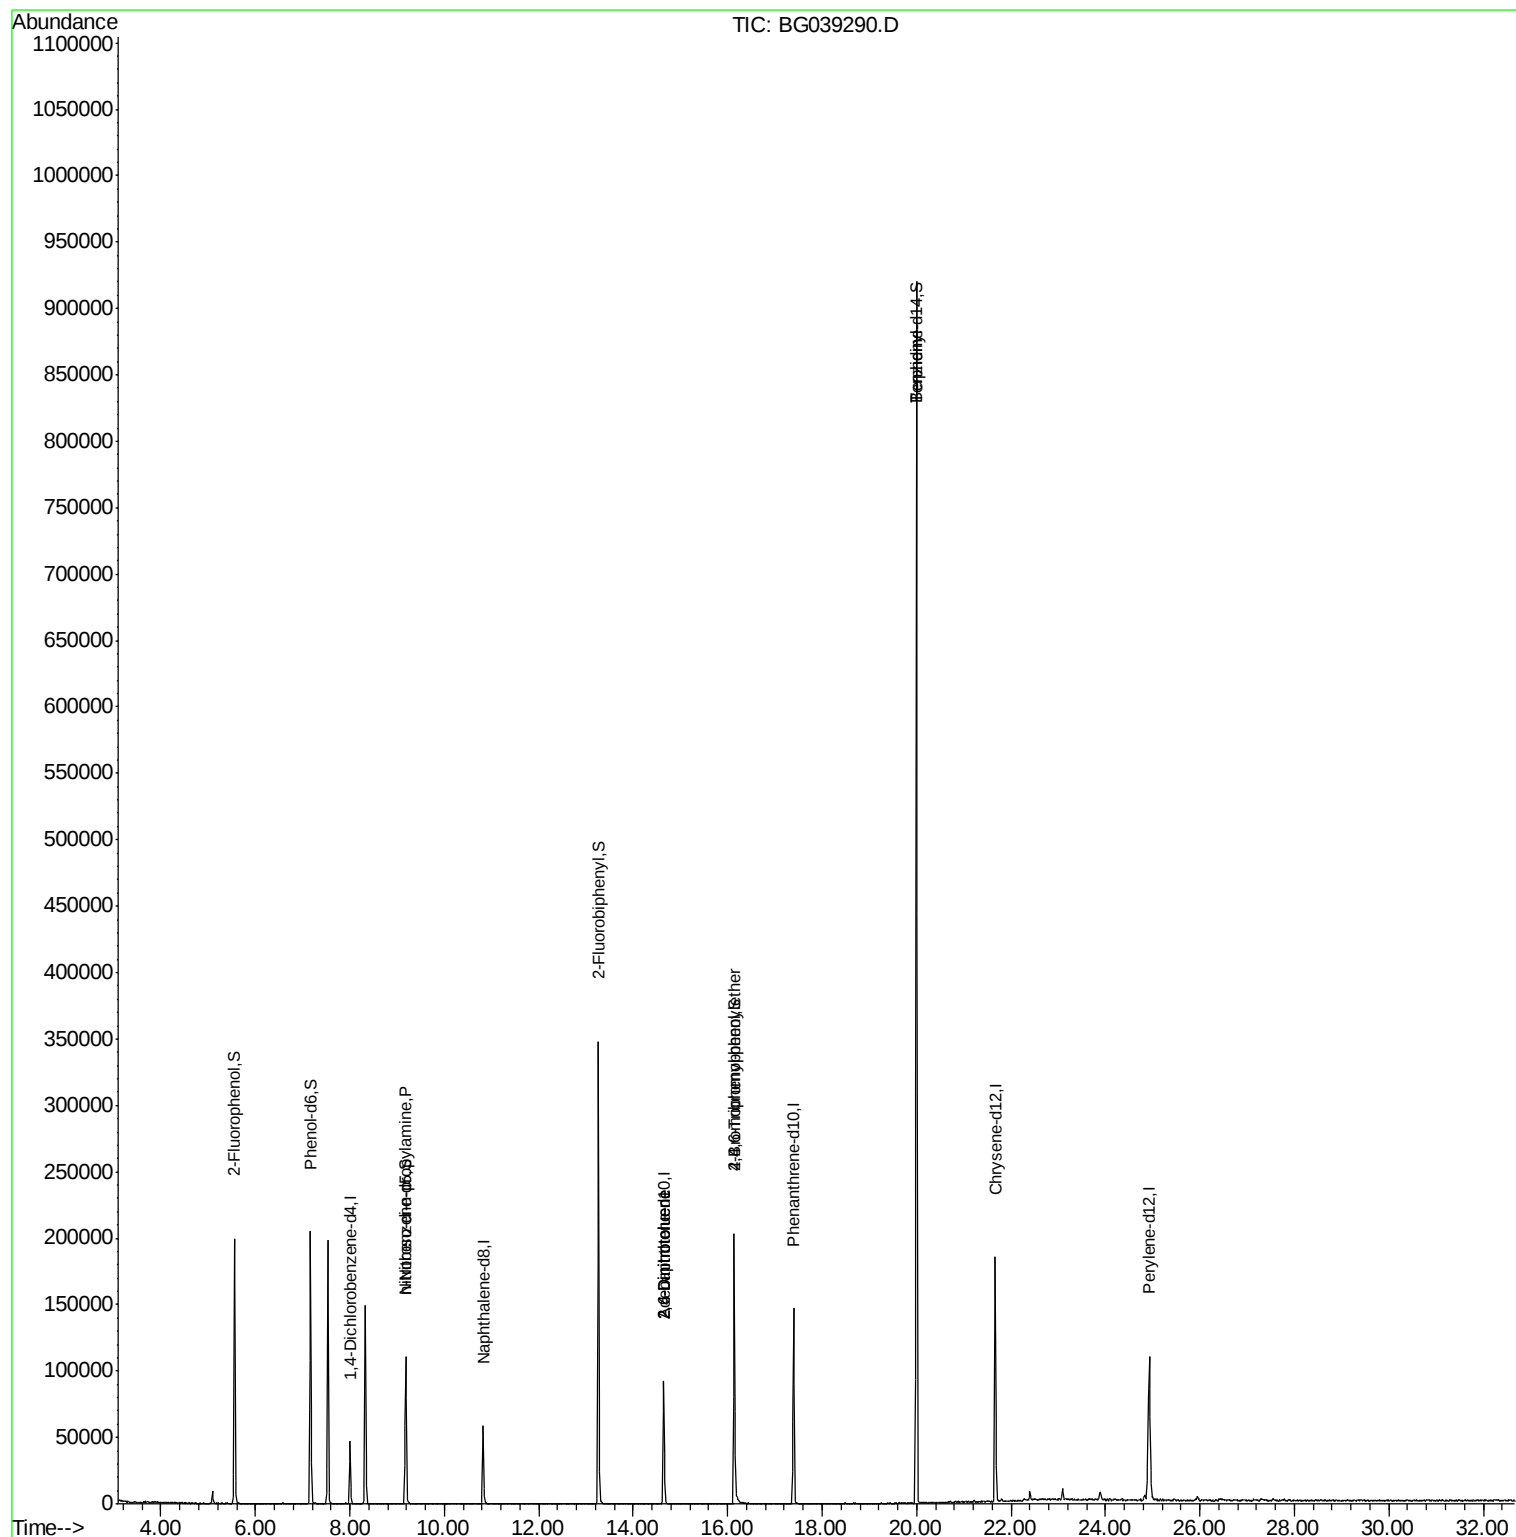

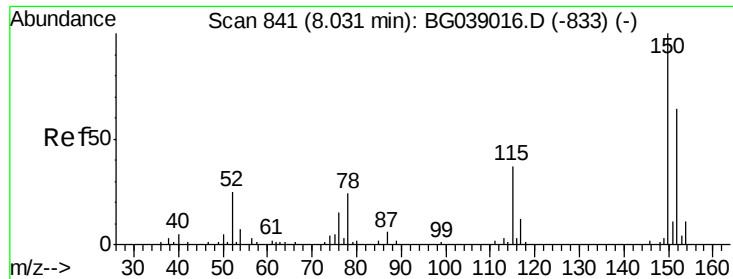


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 837
Delta R.T. -0.01 min
Lab File: BG039290.D
Acq: 25 Jan 2019 22:38

Instrument :
BNA_G
ClientSampleId :
PB116630TB

Tgt Ion:152 Resp: 14381
Ion Ratio Lower Upper
152 100
150 167.0 124.7 187.1
115 55.0 46.5 69.7

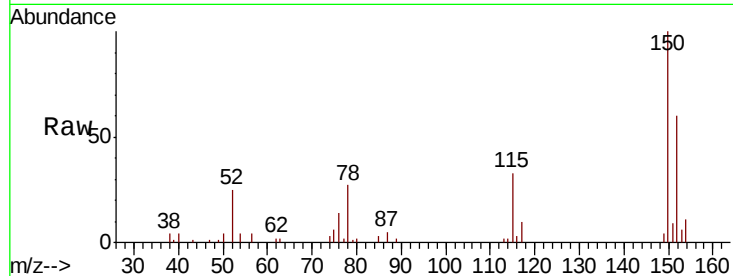


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

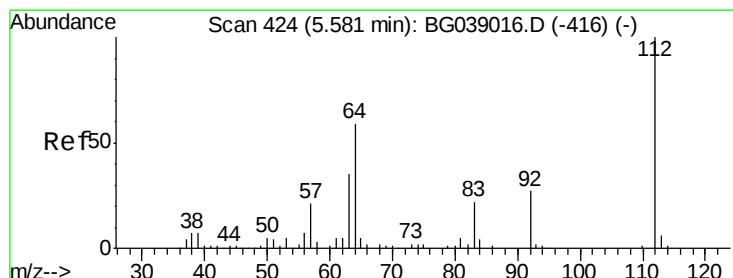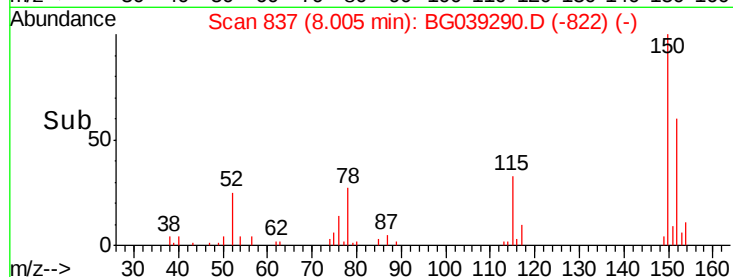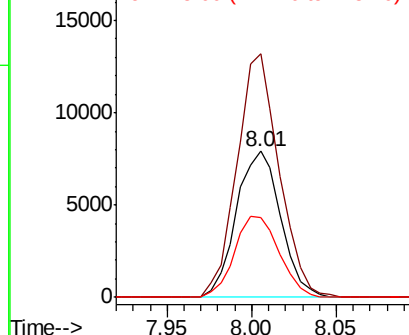



#5


2-Fluorophenol
Concen: 113.108 ng
RT: 5.56 min Scan# 420
Delta R.T. -0.01 min
Lab File: BG039290.D
Acq: 25 Jan 2019 22:38

Tgt Ion:112 Resp: 85747
Ion Ratio Lower Upper
112 100
64 64.6 47.0 70.6
63 34.3 28.0 42.0

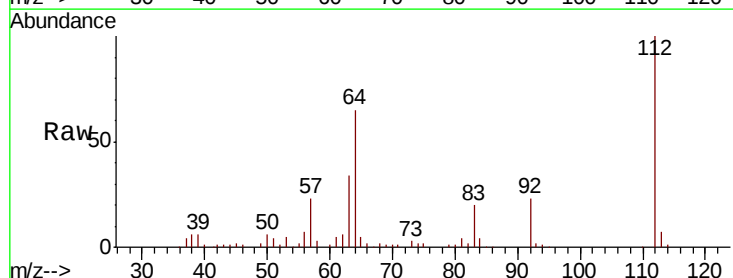

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

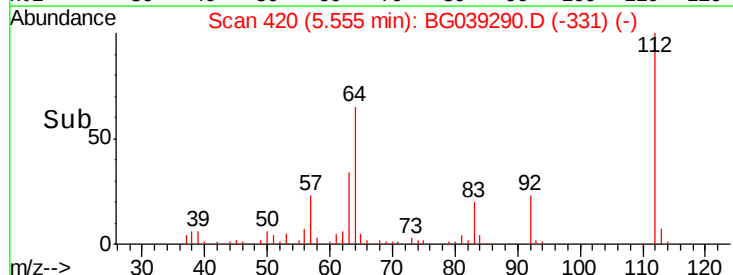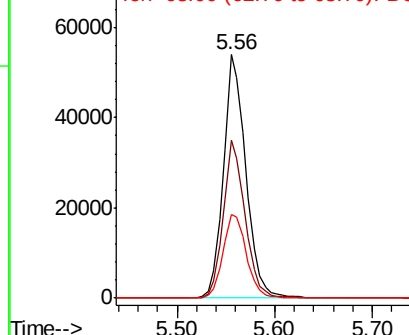

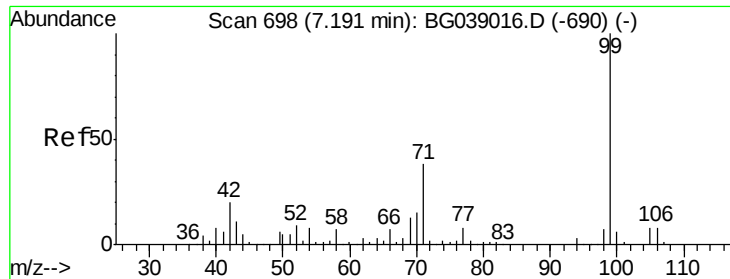

#7

Phenol-d6

Concen: 109.325 ng

RT: 7.16 min Scan# 694

Delta R.T. -0.01 min

Lab File: BG039290.D

Acq: 25 Jan 2019 22:38

Instrument :

BNA_G

ClientSampleId :

PB116630TB


Tgt Ion: 99 Resp: 119274

Ion Ratio Lower Upper




99 100

42 20.0 15.8 23.6

71 38.6 30.2 45.4

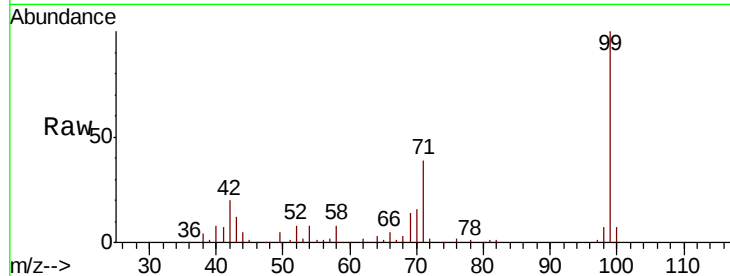

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

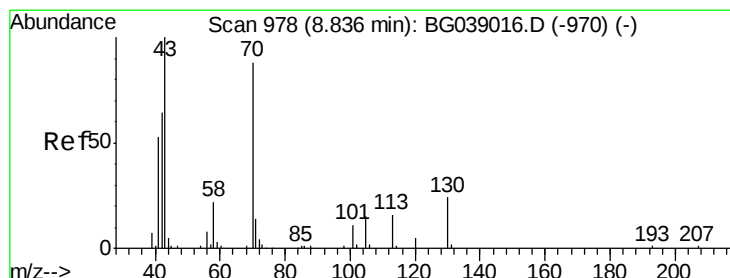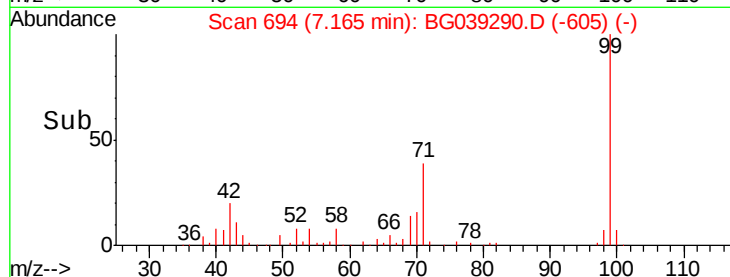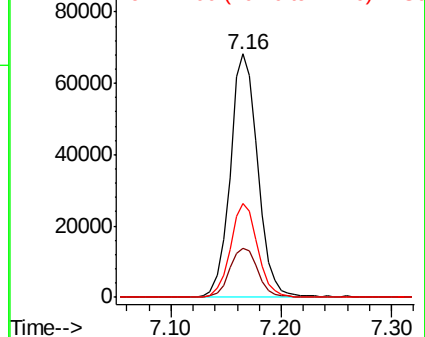

#19

n-Nitroso-di-n-propylamine

Concen: 12.322 ng

RT: 9.18 min Scan# 1037

Delta R.T. 0.36 min

Lab File: BG039290.D

Acq: 25 Jan 2019 22:38

Tgt Ion: 70 Resp: 8828


Ion Ratio Lower Upper

70 100



42 52.4 59.0 88.4#


101 0.0 10.4 15.6#

130 0.0 21.6 32.4#

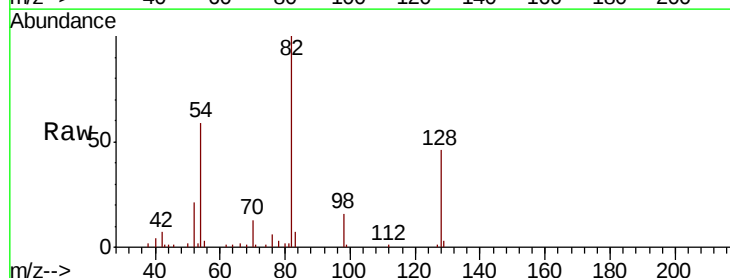

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

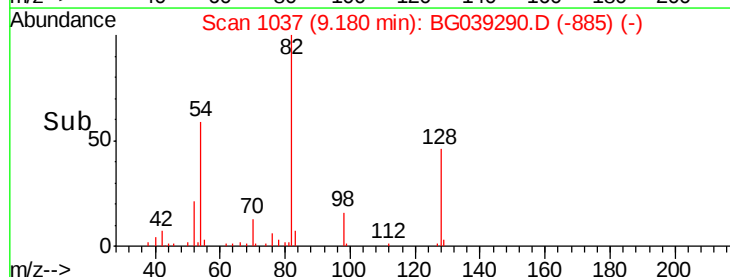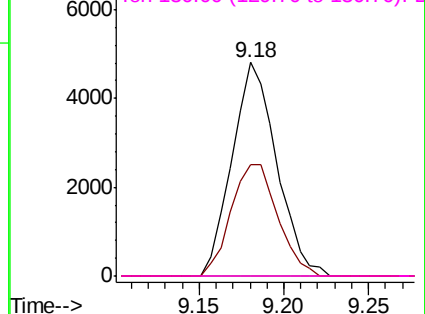


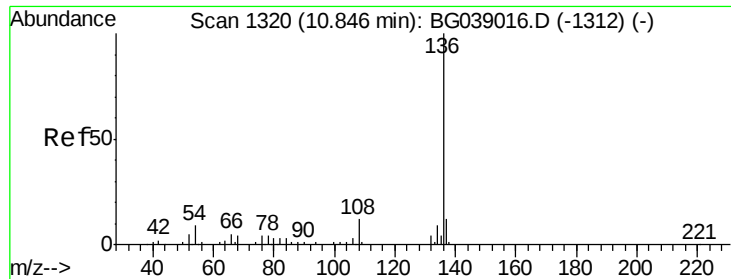




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.82 min Scan# 1316
Delta R.T. -0.01 min
Lab File: BG039290.D
Acq: 25 Jan 2019 22:38

Instrument :
BNA_G
ClientSampleId :
PB116630TB

Tgt Ion:	136	Resp:	56093
Ion	Ratio	Lower	Upper
136	100		
137	11.8	9.4	14.2
54	9.6	7.2	10.8
68	5.1	3.5	5.3

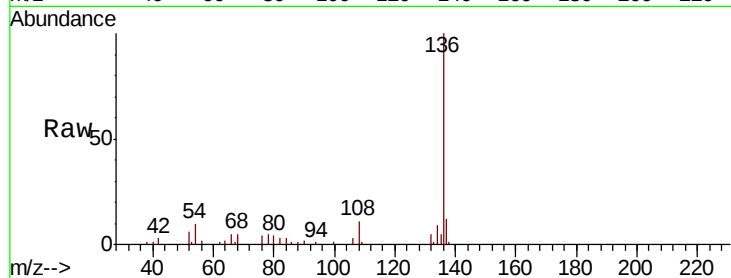


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

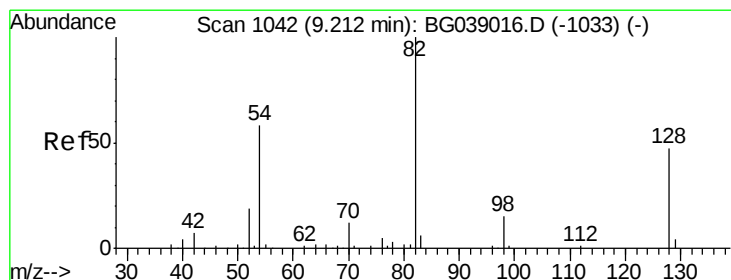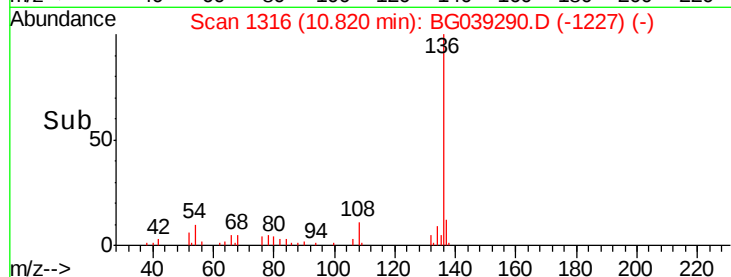
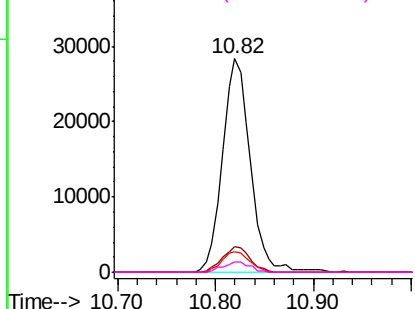



#23
Nitrobenzene-d5
Concen: 67.857 ng
RT: 9.18 min Scan# 1037
Delta R.T. -0.01 min
Lab File: BG039290.D
Acq: 25 Jan 2019 22:38

Tgt Ion:	82	Resp:	69560
Ion	Ratio	Lower	Upper
82	100		
128	46.1	37.3	55.9
54	59.1	46.4	69.6

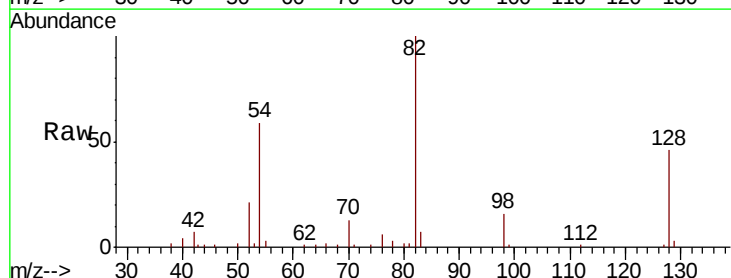

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

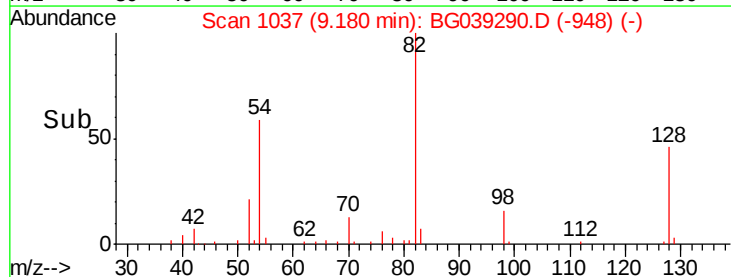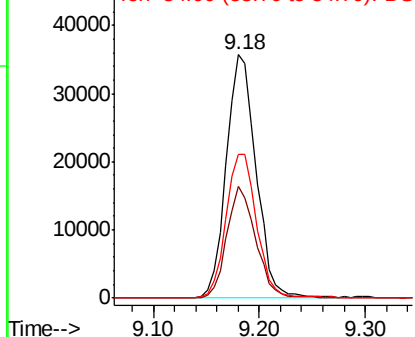

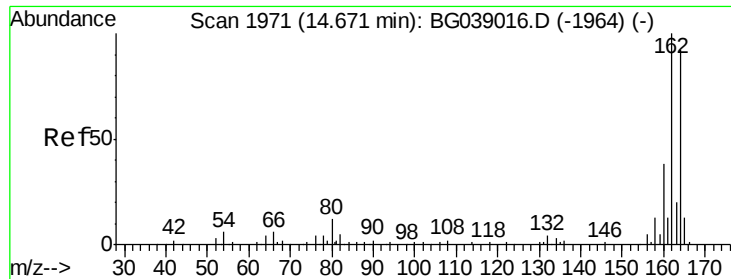

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.64 min Scan# 1967

Delta R.T. -0.01 min

Lab File: BG039290.D

Acq: 25 Jan 2019 22:38

Instrument :

BNA_G

ClientSampleId :

PB116630TB


Tgt Ion:164 Resp: 36124

Ion Ratio Lower Upper

164 100

162 99.6 87.2 130.8




160 45.7 33.3 49.9

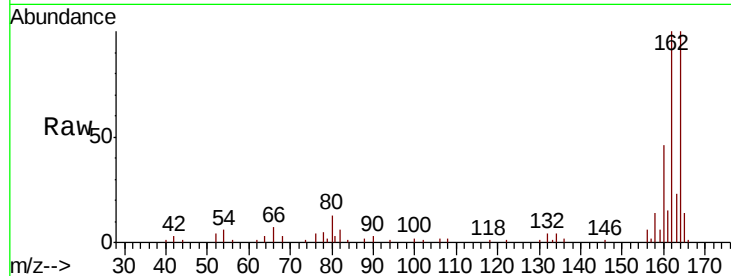

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

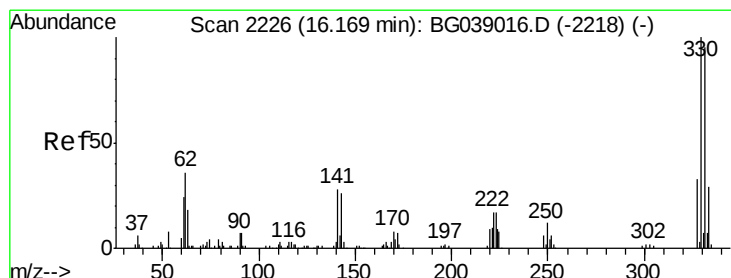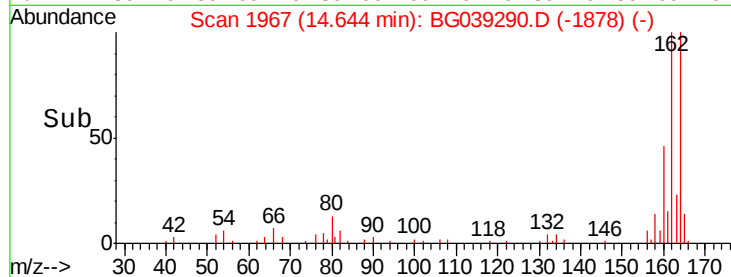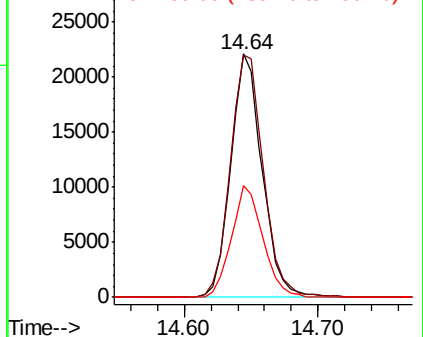

#42

2,4,6-Tribromophenol

Concen: 84.526 ng

RT: 16.14 min Scan# 2221

Delta R.T. -0.02 min

Lab File: BG039290.D

Acq: 25 Jan 2019 22:38


Tgt Ion:330 Resp: 51184

Ion Ratio Lower Upper

330 100

332 95.0 75.7 113.5



141 31.1 24.9 37.3

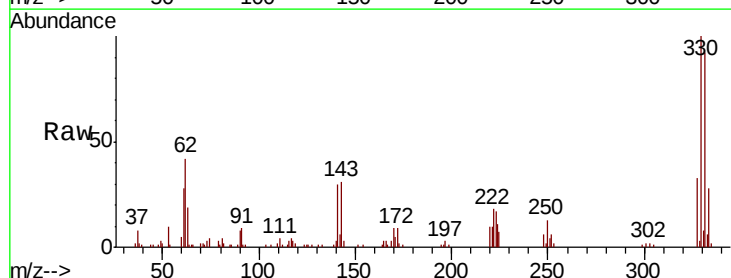


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



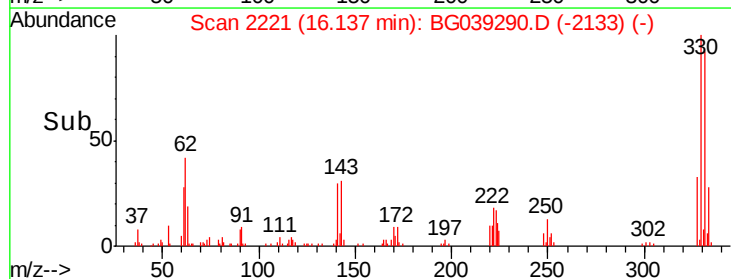
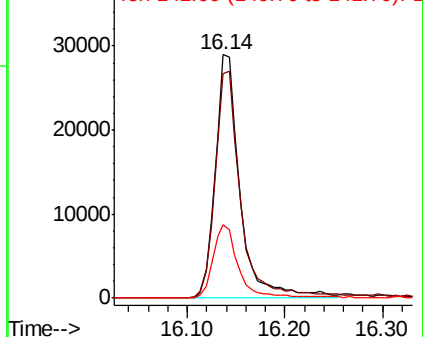


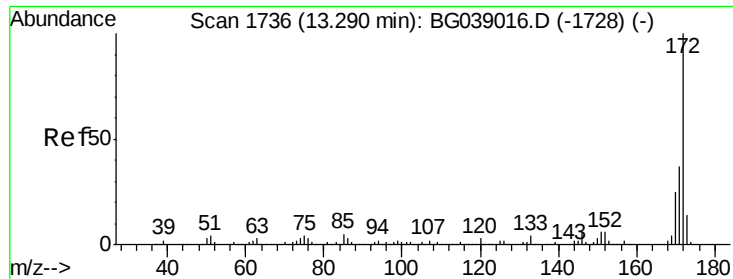

#45
 2-Fluorobiphenyl
 Concen: 73.184 ng
 RT: 13.26 min Scan# 1732
 Delta R.T. -0.01 min
 Lab File: BG039290.D
 Acq: 25 Jan 2019 22:38




Instrument :
 BNA_G
 ClientSampleId :
 PB116630TB


Tgt Ion:172 Resp: 193173
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.4 44.0
 170 23.1 20.1 30.1

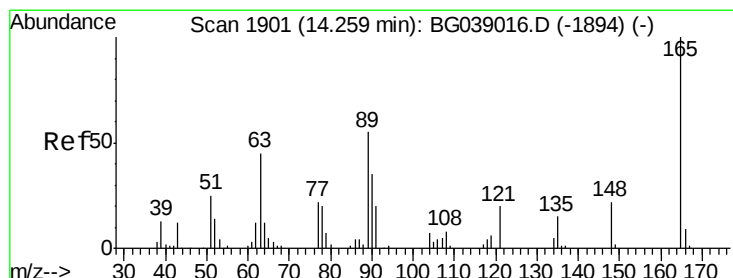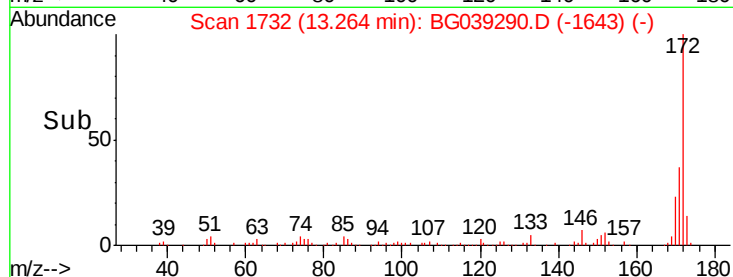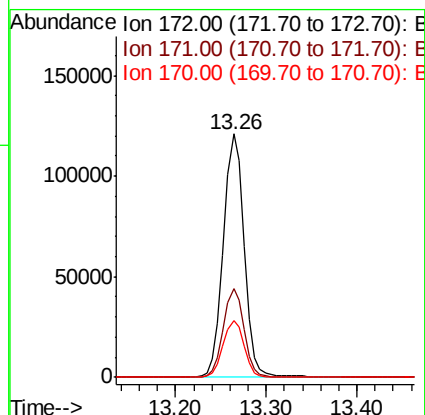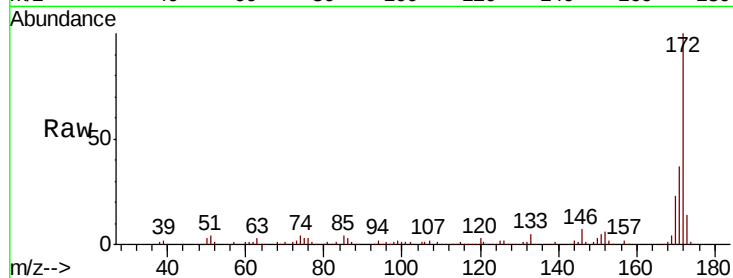

#51
 2,6-Dinitrotoluene
 Concen: 7.061 ng
 RT: 14.64 min Scan# 1967
 Delta R.T. 0.40 min
 Lab File: BG039290.D
 Acq: 25 Jan 2019 22:38

Tgt Ion:165 Resp: 4819
 Ion Ratio Lower Upper
 165 100
 63 0.0 43.6 65.4#
 89 0.0 43.7 65.5#


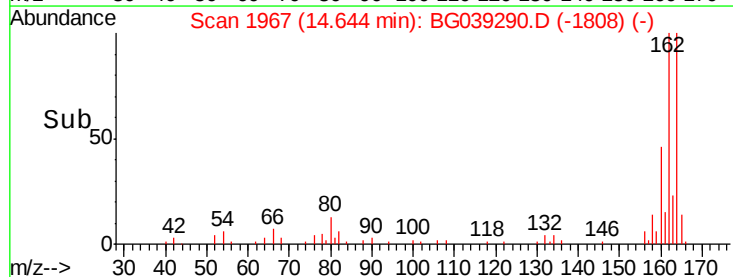
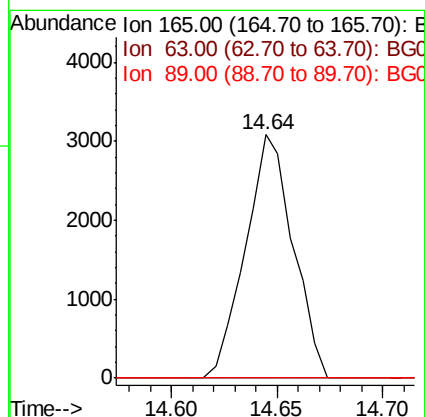
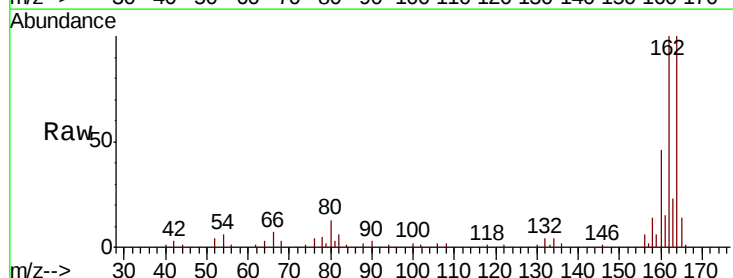


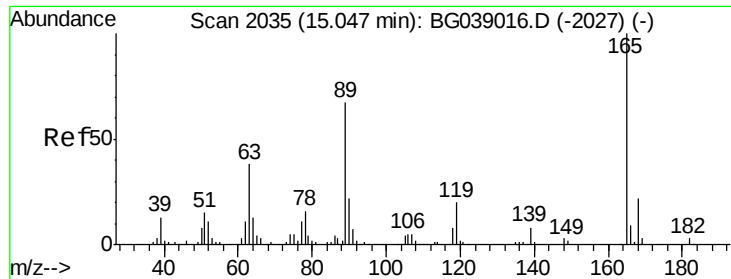

#57
 2,4-Dinitrotoluene
 Concen: 4.922 ng
 RT: 14.64 min Scan# 1967
 Delta R.T. -0.39 min
 Lab File: BG039290.D
 Acq: 25 Jan 2019 22:38




Instrument :
 BNA_G
 ClientSampleId :
 PB116630TB


Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	30.2	45.4#
89	0.0	53.2	79.8#
182	0.0	2.7	4.1#

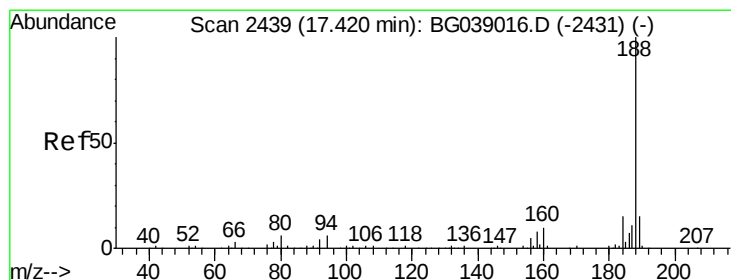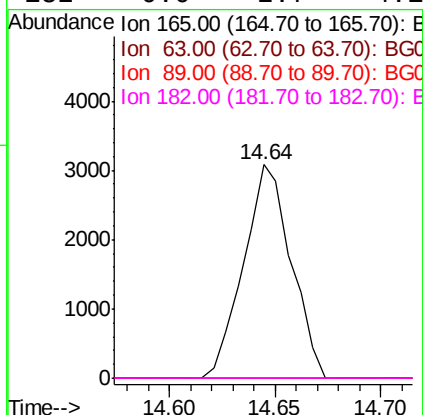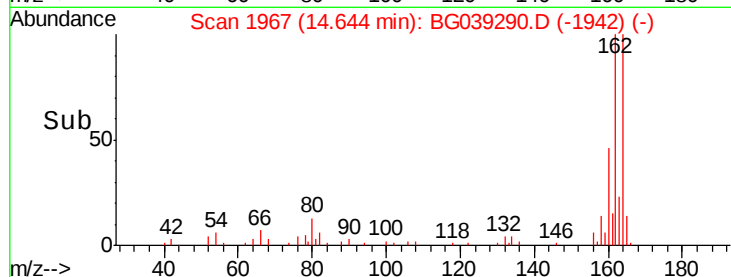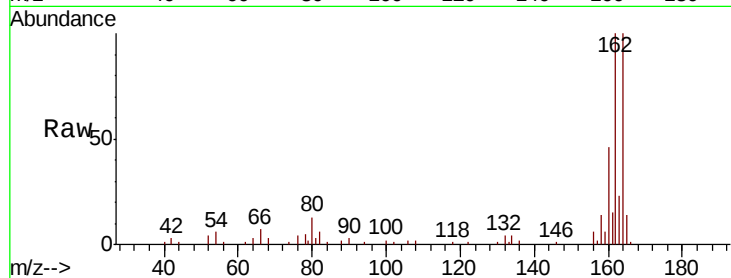

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.39 min Scan# 2435
 Delta R.T. -0.01 min
 Lab File: BG039290.D
 Acq: 25 Jan 2019 22:38

Tgt Ion	Ratio	Lower	Upper
188	100		
94	6.2	5.0	7.4
80	6.9	4.7	7.1

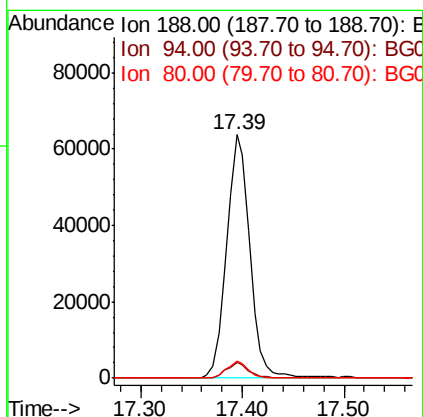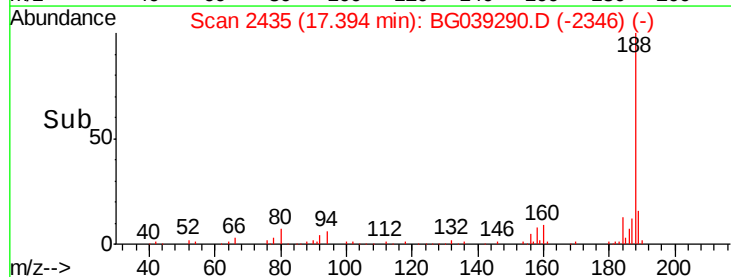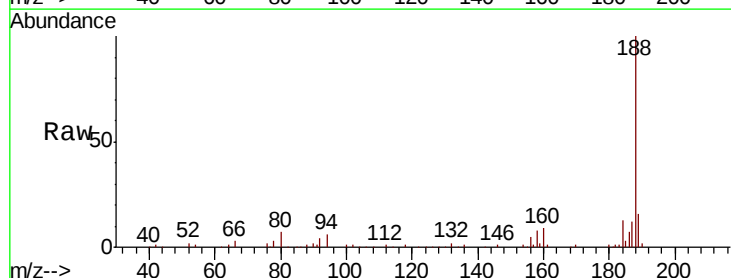


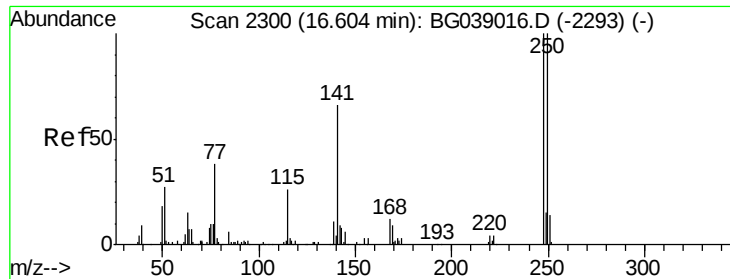




#67
 4-Bromophenyl-phenylether
 Concen: 2.340 ng
 RT: 16.14 min Scan# 2221
 Delta R.T. -0.45 min
 Lab File: BG039290.D
 Acq: 25 Jan 2019 22:38

Instrument :
 BNA_G
 ClientSampleId :
 PB116630TB

Tgt Ion:248 Resp: 3038
 Ion Ratio Lower Upper
 248 100
 250 196.3 79.9 119.9#
 141 353.8 52.7 79.1#

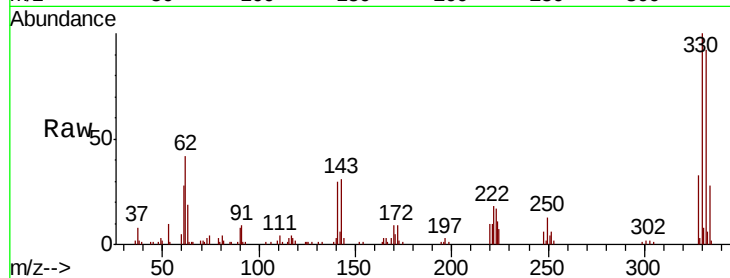


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

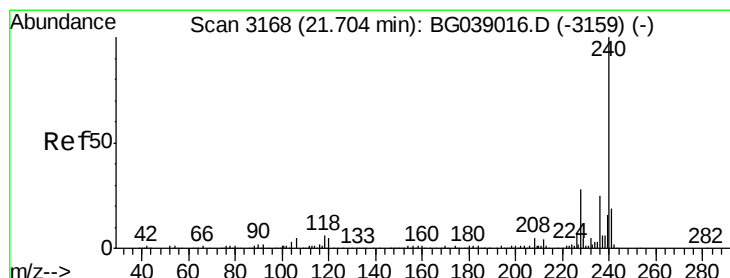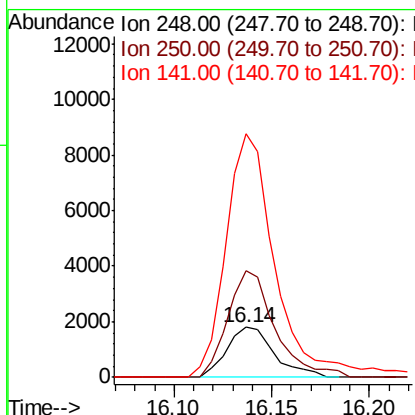
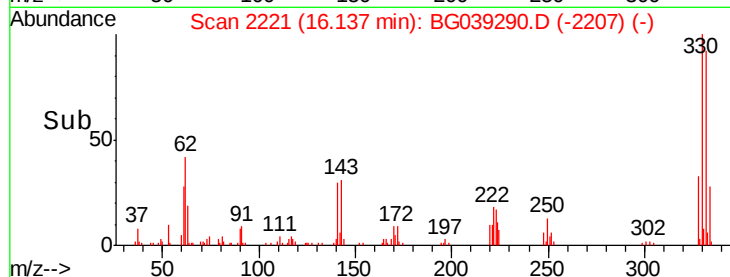



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.67 min Scan# 3162
 Delta R.T. -0.02 min
 Lab File: BG039290.D
 Acq: 25 Jan 2019 22:38

Tgt Ion:240 Resp: 123412
 Ion Ratio Lower Upper
 240 100
 120 6.1 4.3 6.5
 236 26.3 20.1 30.1

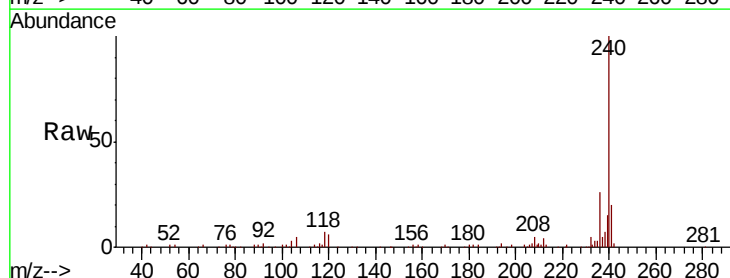

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

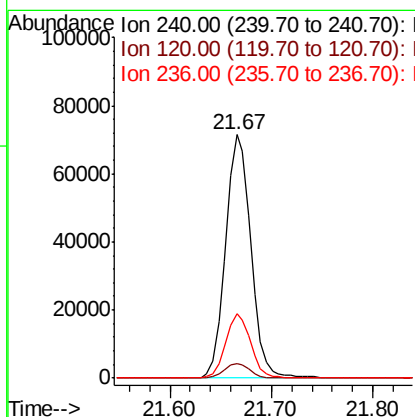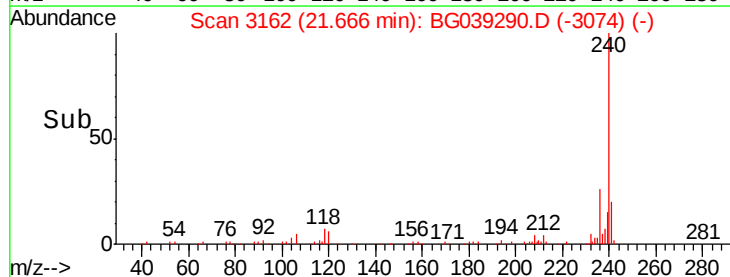

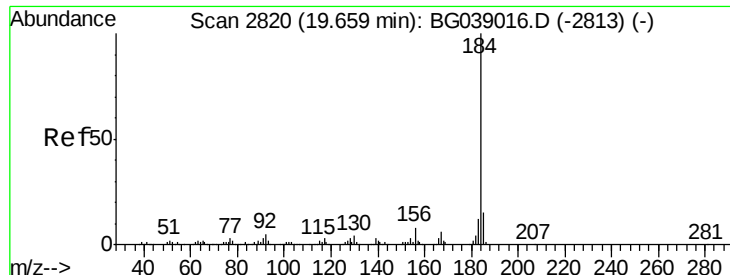

#77

Benzidine

Concen: 2.015 ng

RT: 20.00 min Scan# 2878

Delta R.T. 0.35 min

Lab File: BG039290.D

Acq: 25 Jan 2019 22:38

Instrument :

BNA_G

ClientSampleId :

PB116630TB


Tgt Ion:184 Resp: 7607

Ion Ratio Lower Upper

184 100

185 18.0 12.1 18.1




183 5.9 9.5 14.3#

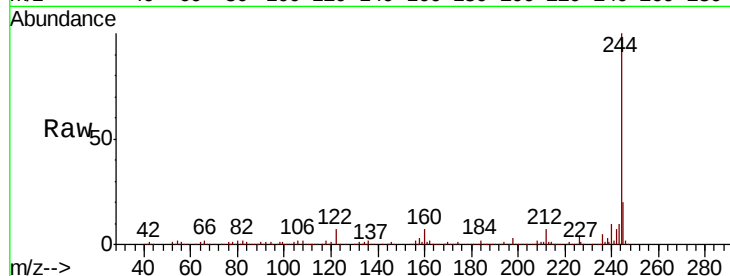

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

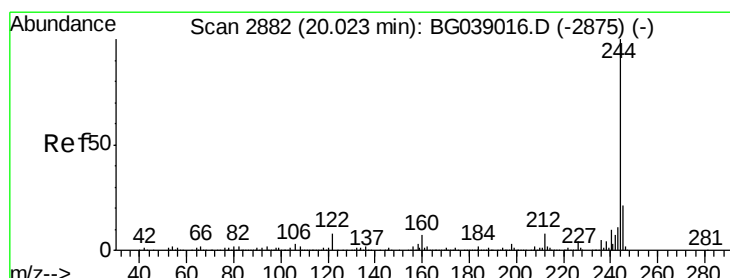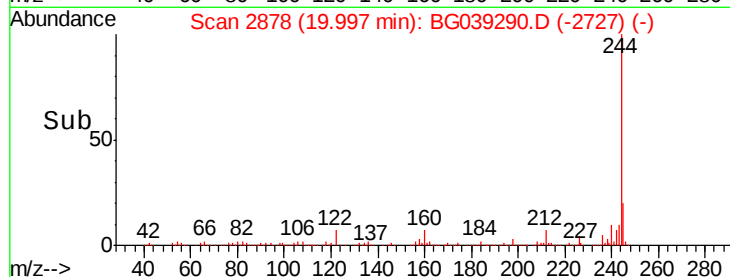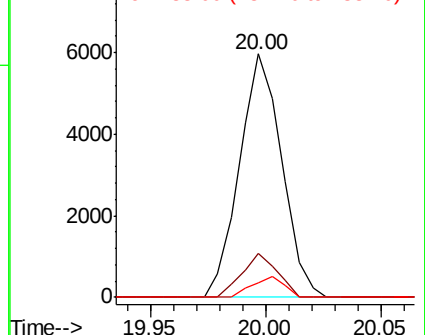

#79

Terphenyl-d14

Concen: 71.044 ng

RT: 20.00 min Scan# 2878

Delta R.T. -0.01 min

Lab File: BG039290.D

Acq: 25 Jan 2019 22:38


Tgt Ion:244 Resp: 473956

Ion Ratio Lower Upper

244 100

212 7.3 6.1 9.1



122 6.7 6.1 9.1

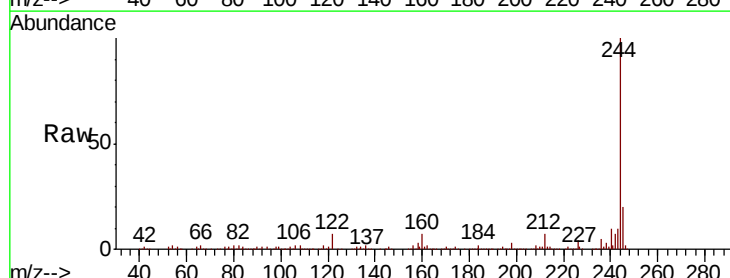


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

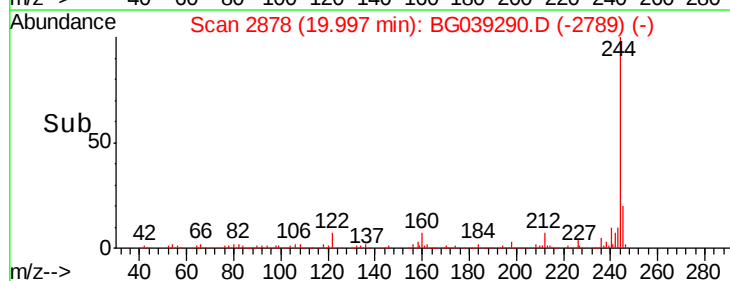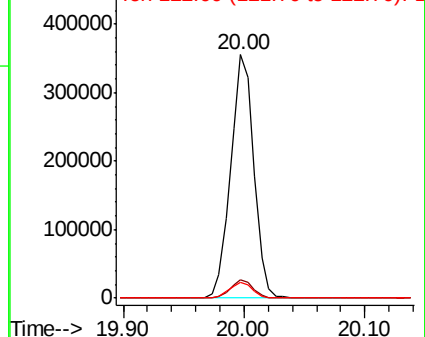

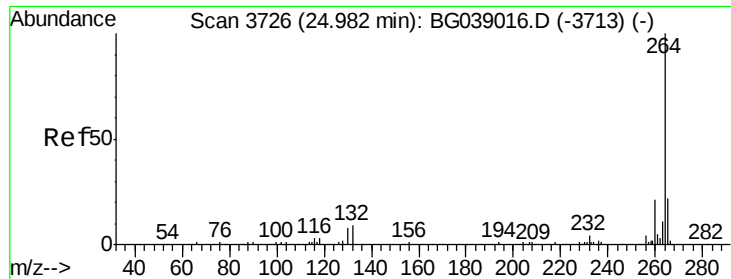

#87
Perylene-d12
Concen: 20.000 ng
RT: 24.92 min Scan# 3716
Delta R.T. -0.03 min
Lab File: BG039290.D
Acq: 25 Jan 2019 22:38

Instrument :
BNA_G
ClientSampleId :
PB116630TB

Tgt Ion: 264 Resp: 139734

Ion	Ratio	Lower	Upper
264	100		
260	24.9	17.0	25.6
265	21.7	17.2	25.8

