
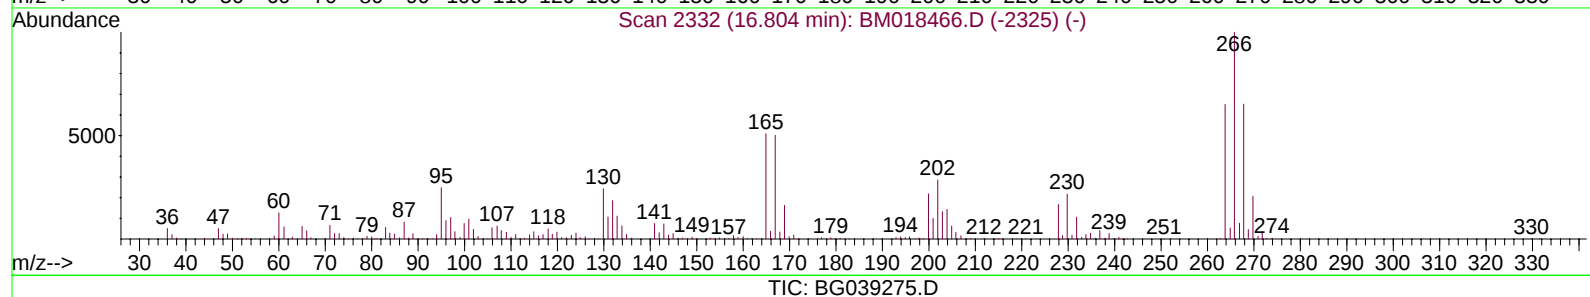
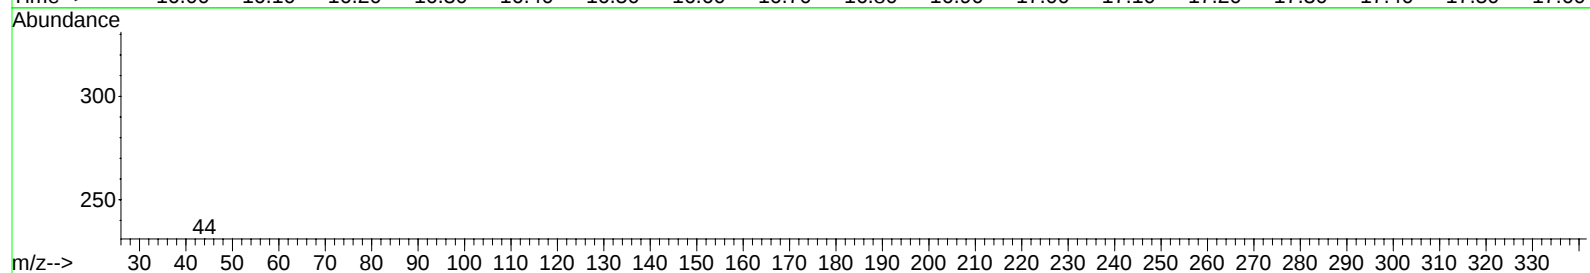


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012519\
Data File : BG039275.D
Acq On : 25 Jan 2019 12:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 18:06:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

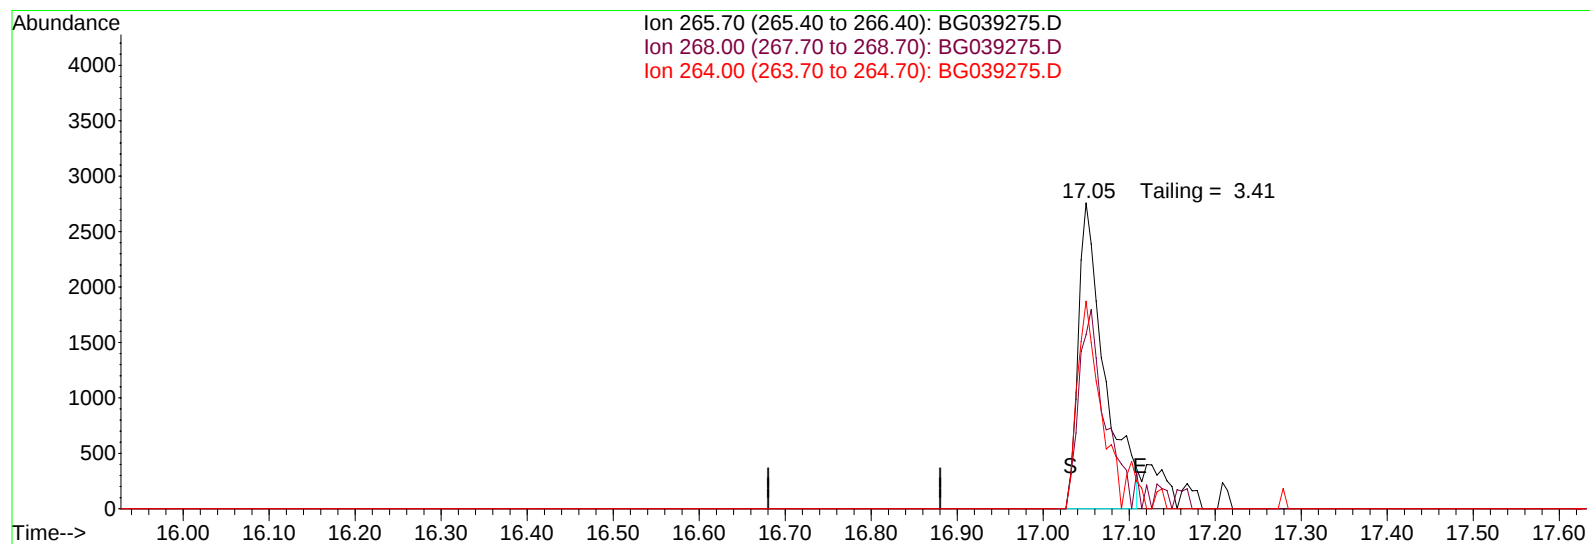

TIC: BG039275.D

(70) Pentachlorophenol (C)




16.780min (-16.780) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	62.20	0.00#
264.00	62.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012519\
Data File : BG039275.D
Acq On : 25 Jan 2019 12:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 18:06:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

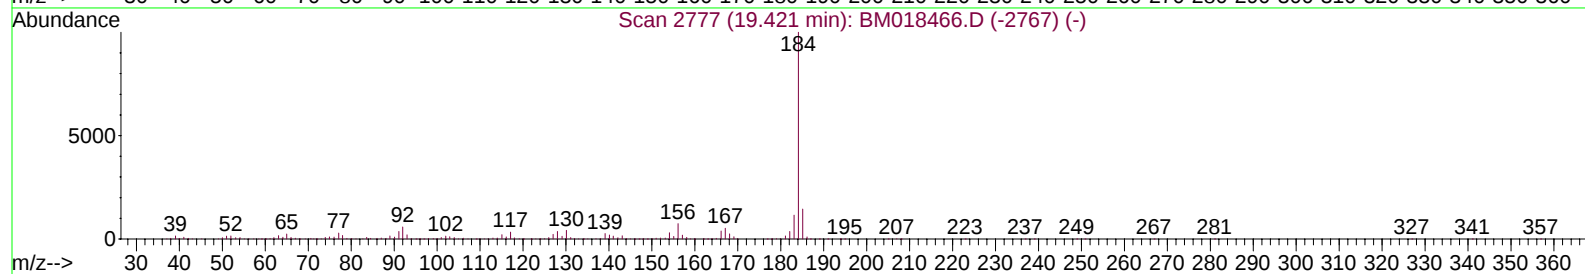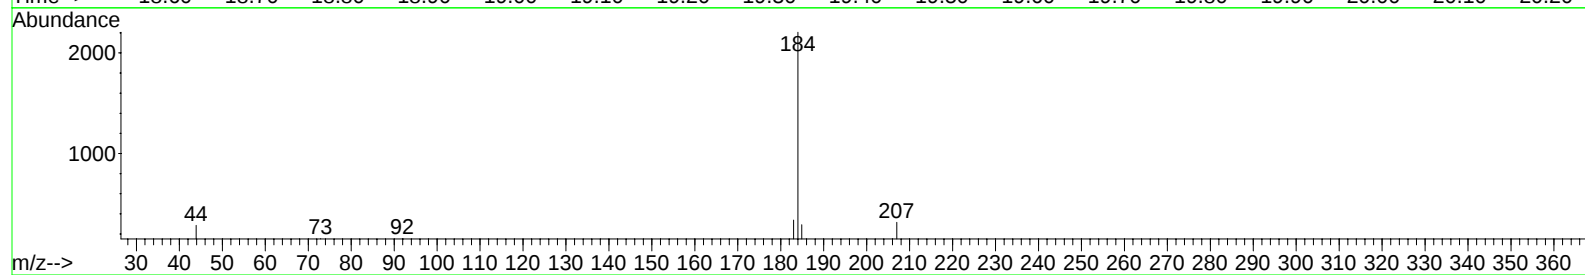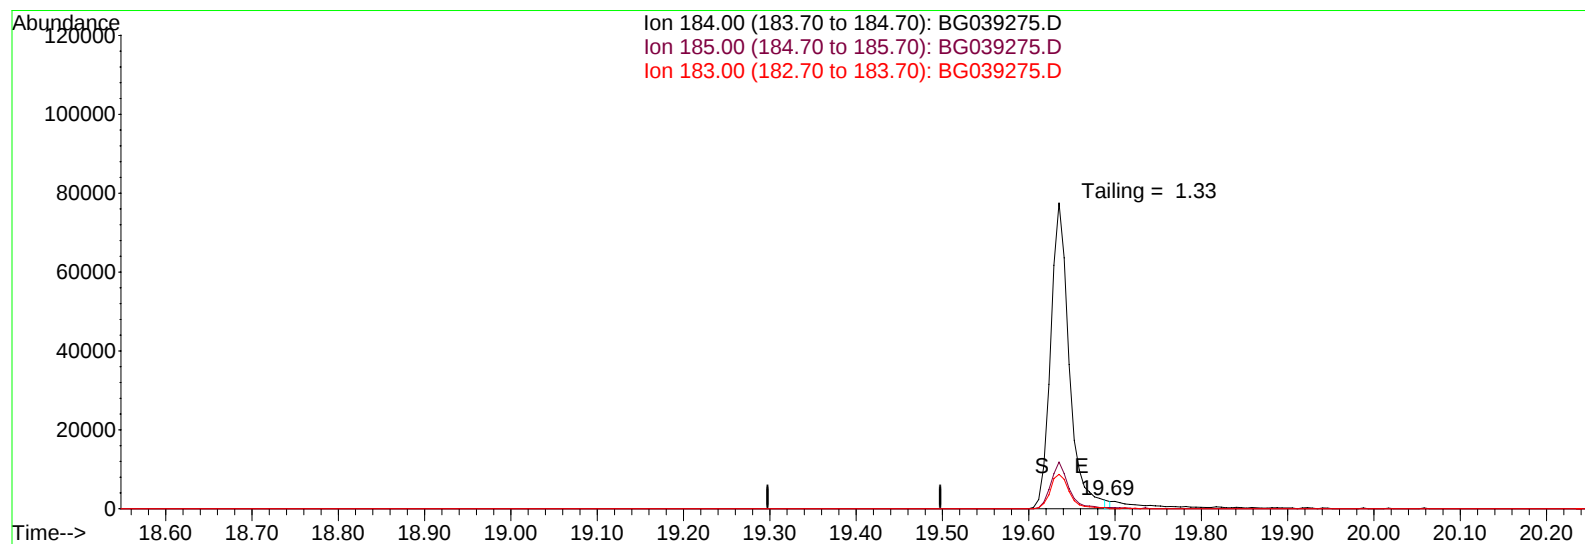

TIC: BG039275.D

(77) Benzidine

19.688min (+0.290) 0.00ng m

response 646

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.24
183.00	11.90	15.32#
0.00	0.00	0.00