
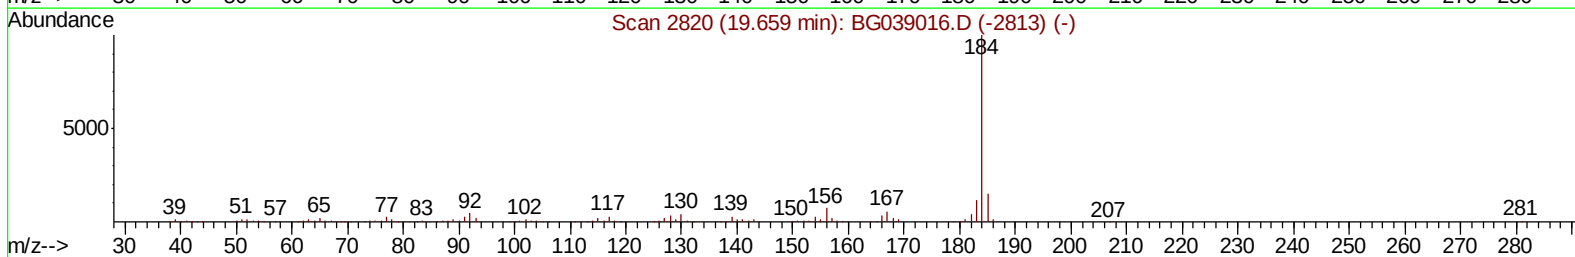
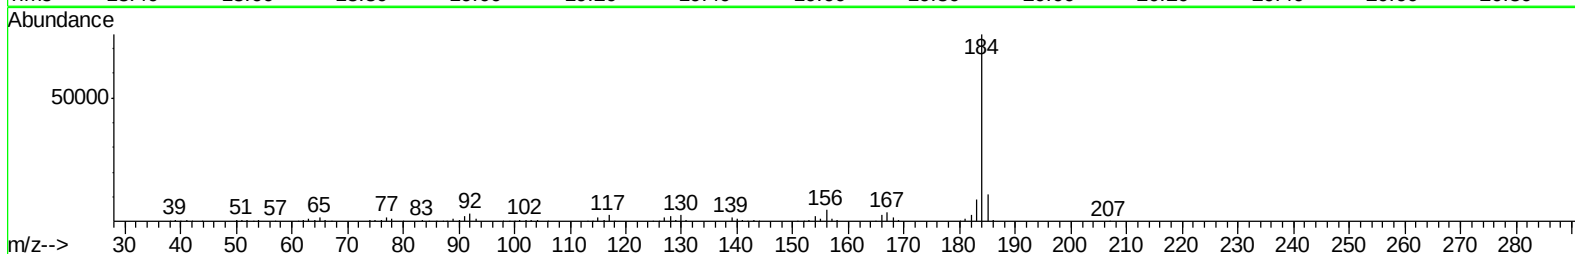


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012519\
 Data File : BG039293.D
 Acq On : 26 Jan 2019 1:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 05:56:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration

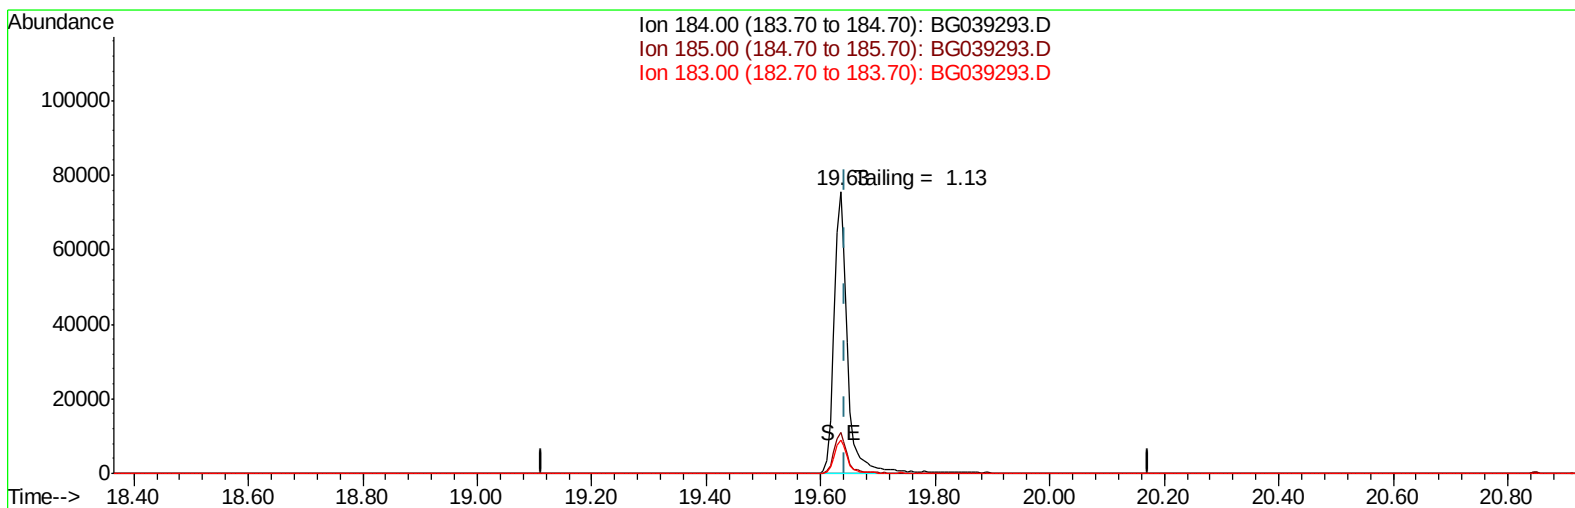

TIC: BG039293.D

(77) Benzidine




19.634min (-0.009) 0.00ng

response 121561

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.44
183.00	11.90	11.81
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012519\
Data File : BG039293.D
Acq On : 26 Jan 2019 1:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 05:56:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

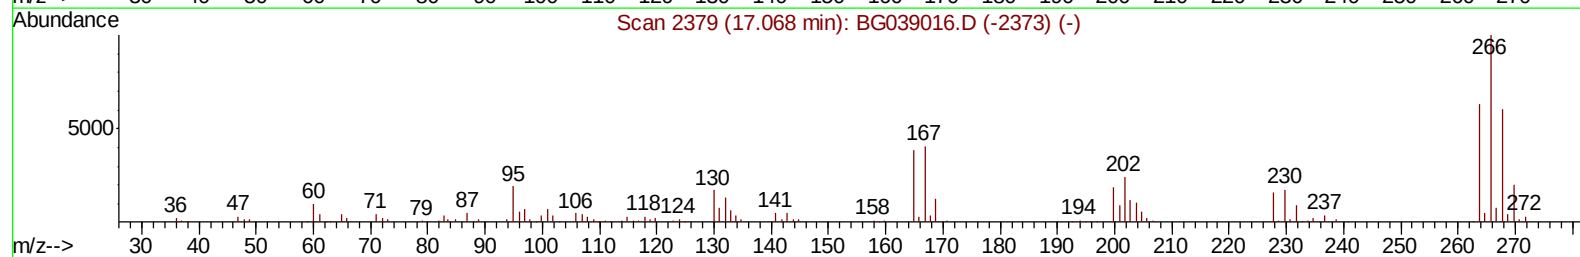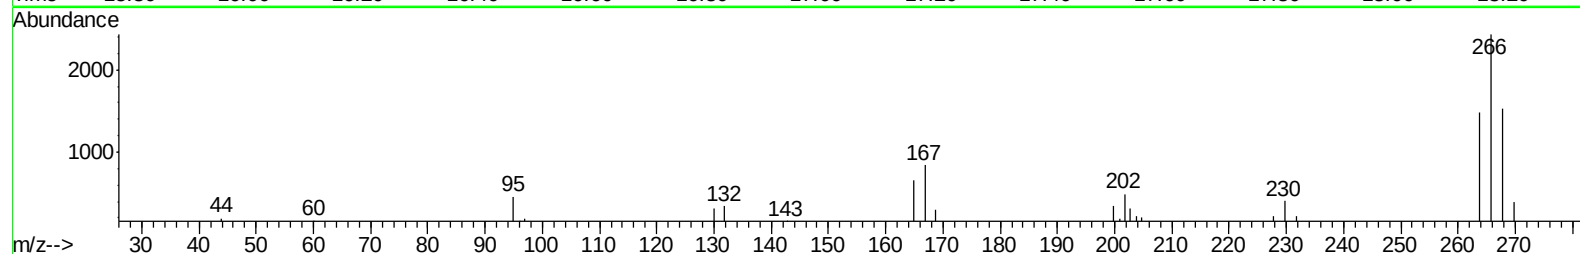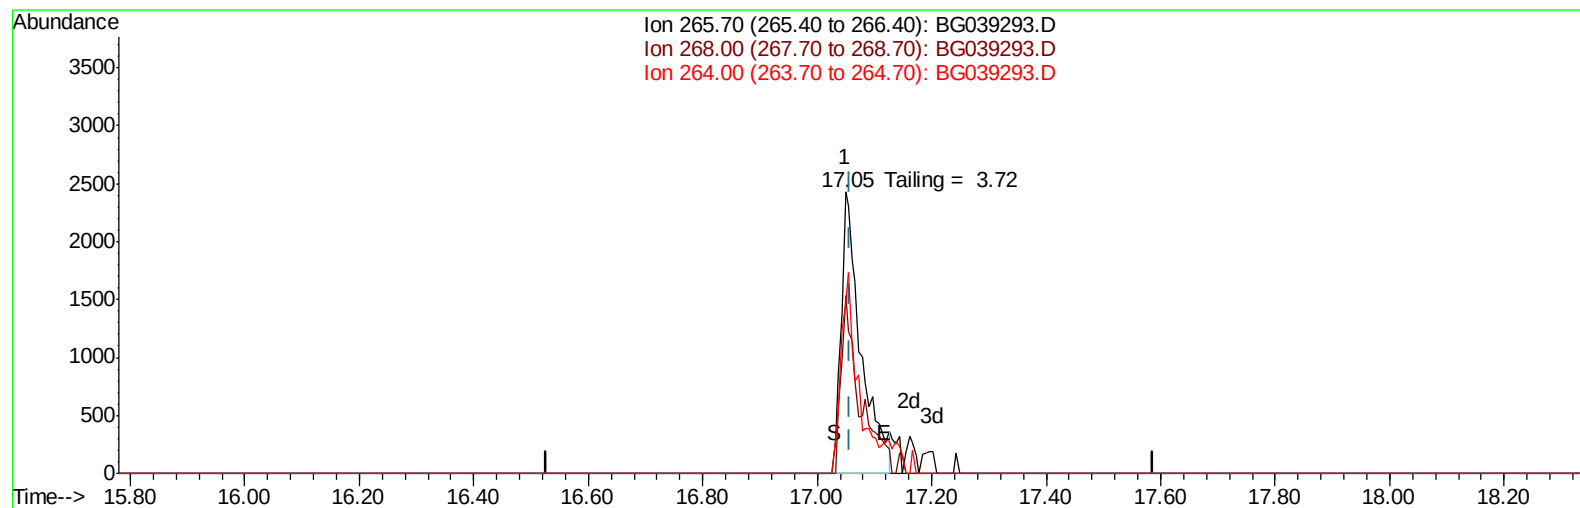

TIC: BG039293.D

(70) Pentachlorophenol (C)

17.049min (-0.009) 0.00ng

response 5748

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.21
264.00	68.20	60.74
0.00	0.00	0.00