

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012519\
 Data File : BG039285.D
 Acq On : 25 Jan 2019 19:21
 Operator : JU/SJ
 Sample : K1016-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TR-05-RO-2-012319

Quant Time: Jan 28 03:39:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	14186	20.00	ng	0.00
21) Naphthalene-d8	10.82	136	54346	20.00	ng	0.00
39) Acenaphthene-d10	14.65	164	37127	20.00	ng	0.00
64) Phenanthrene-d10	17.39	188	102166	20.00	ng	0.00
76) Chrysene-d12	21.67	240	120761	20.00	ng	-0.02
87) Perylene-d12	24.93	264	128249	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	144441	193.15	ng	0.00
7) Phenol-d6	7.17	99	157748	146.58	ng	0.00
23) Nitrobenzene-d5	9.18	82	89838	90.46	ng	0.00
42) 2,4,6-Tribromophenol	16.14	330	91268	146.65	ng	-0.02
45) 2-Fluorobiphenyl	13.26	172	256737	94.64	ng	0.00
79) Terphenyl-d14	20.00	244	580652	88.95	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012519\
Data File : BG039285.D
Acq On : 25 Jan 2019 19:21
Operator : JU/SJ
Sample : K1016-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-05-RO-2-012319

Quant Time: Jan 28 03:39:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

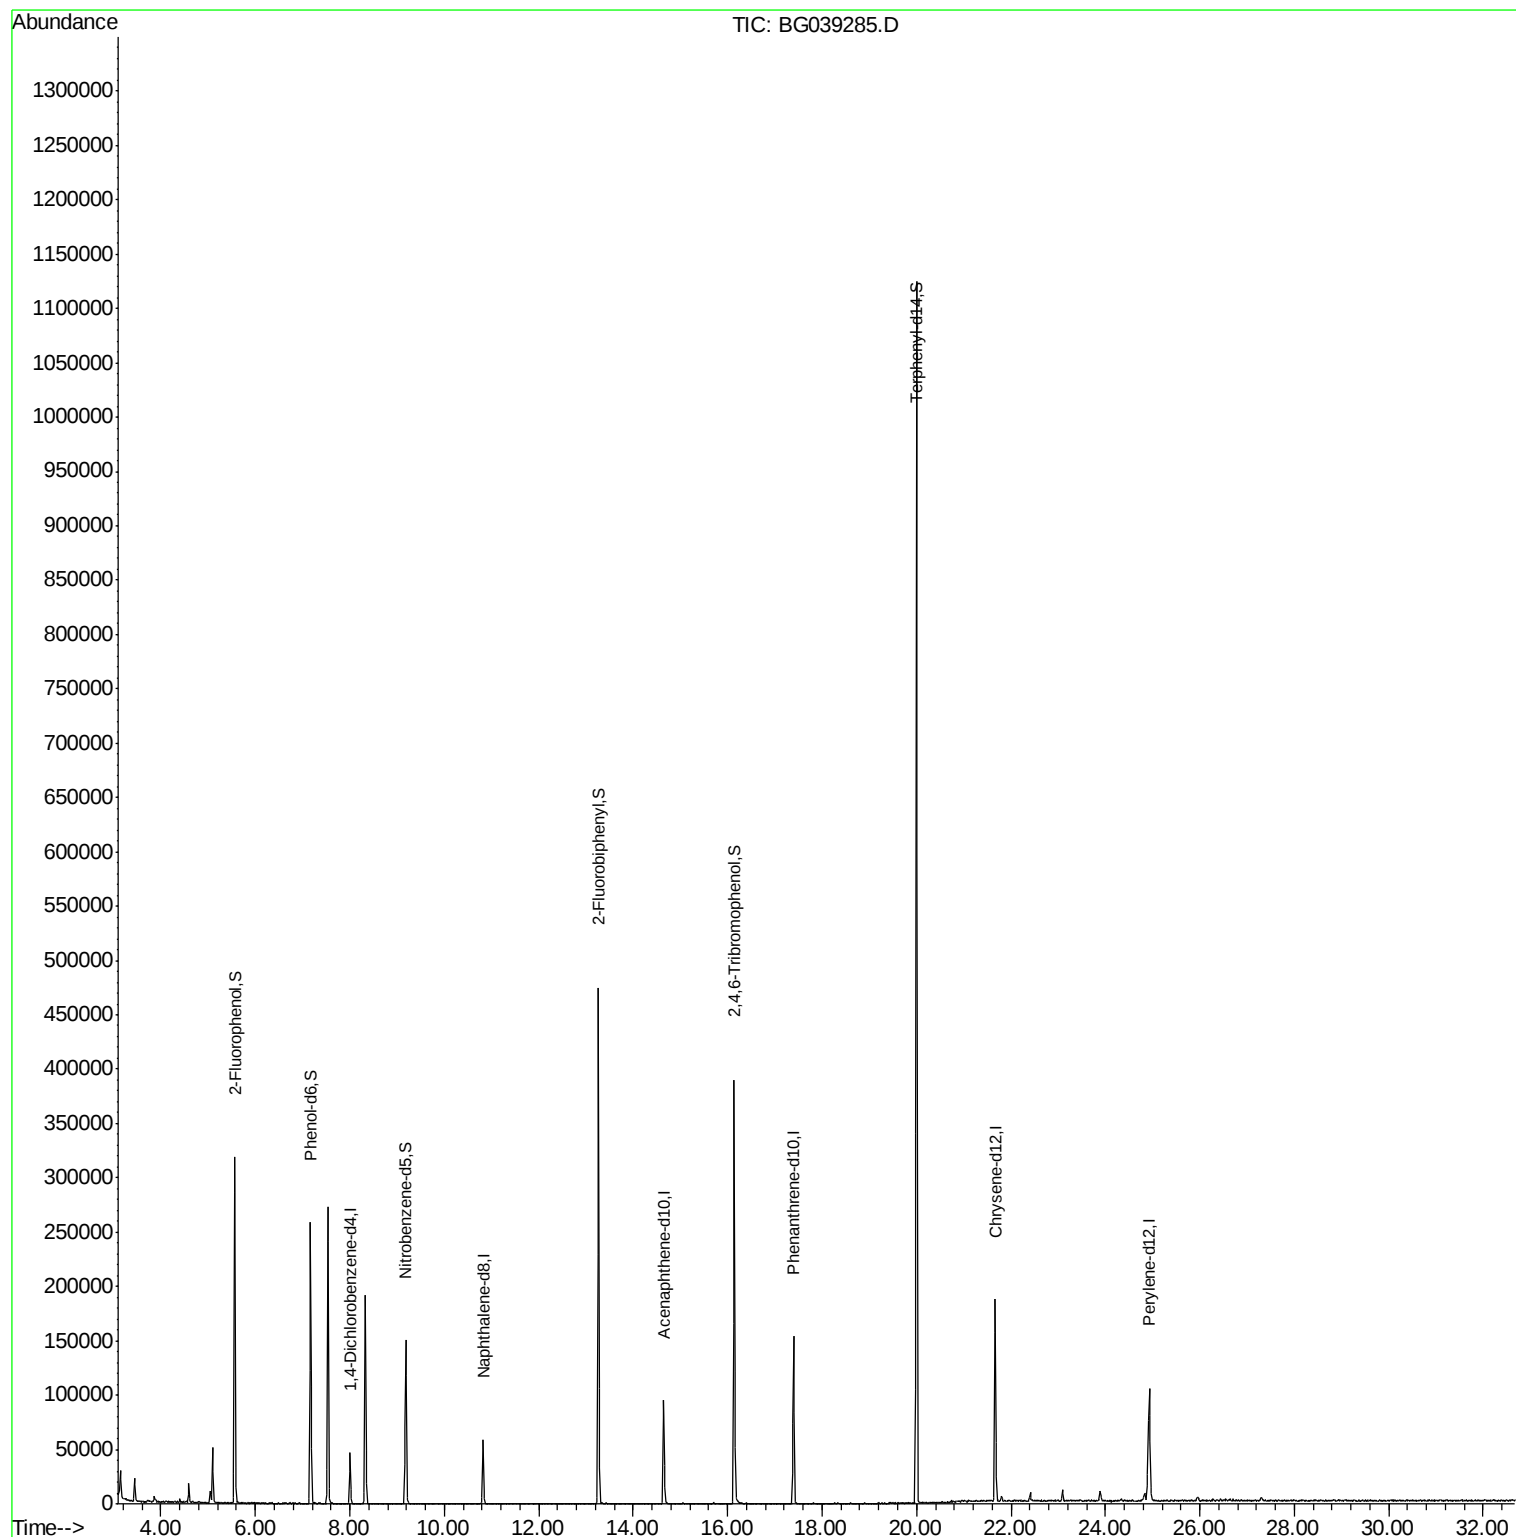

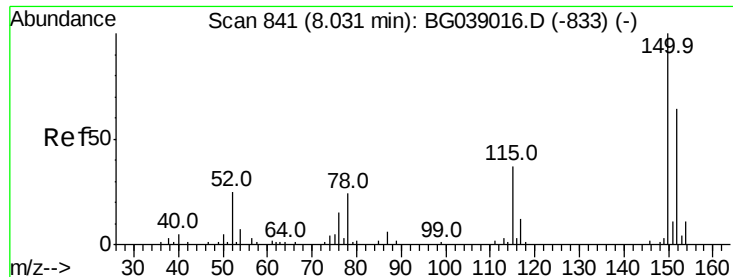


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 837
Delta R.T. -0.01 min
Lab File: BG039285.D
Acq: 25 Jan 2019 19:21

Instrument :
BNA_G
ClientSampleId :
TR-05-RO-2-012319

Tot Ion:152 Resp: 14186
Ion Ratio Lower Upper
152 100
150 149.3 124.7 187.1
115 54.7 46.5 69.7

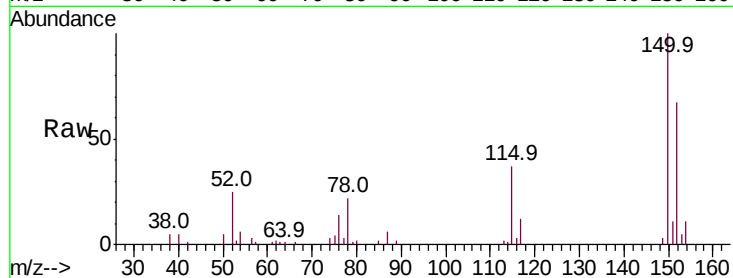


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

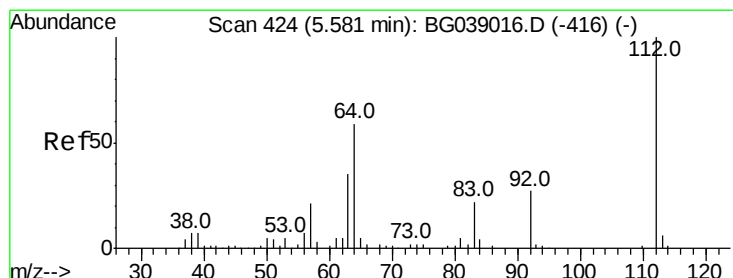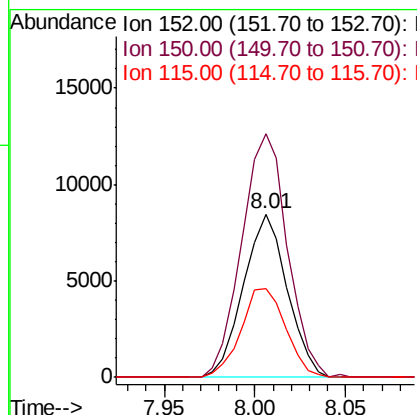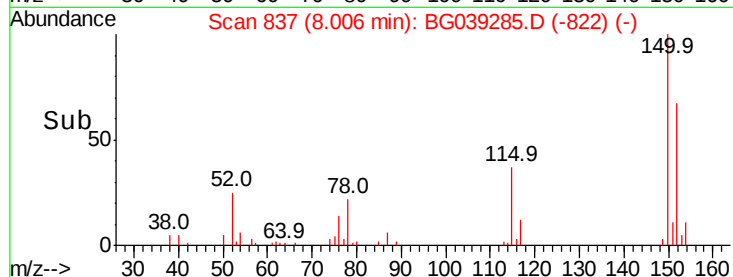



#5


2-Fluorophenol
Concen: 193.150 ng
RT: 5.56 min Scan# 421
Delta R.T. -0.00 min
Lab File: BG039285.D
Acq: 25 Jan 2019 19:21

Tgt Ion:112 Resp: 144441
Ion Ratio Lower Upper
112 100
64 61.2 47.0 70.6
63 32.8 28.0 42.0

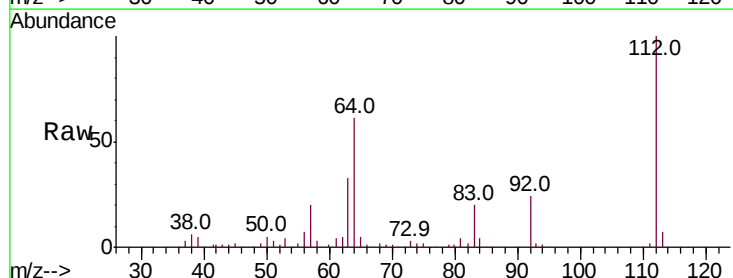

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

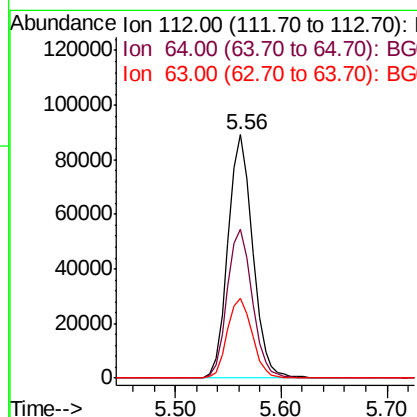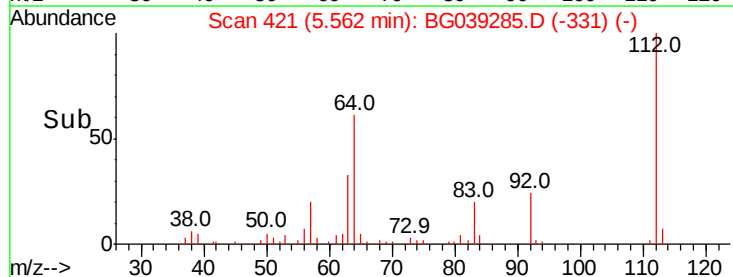

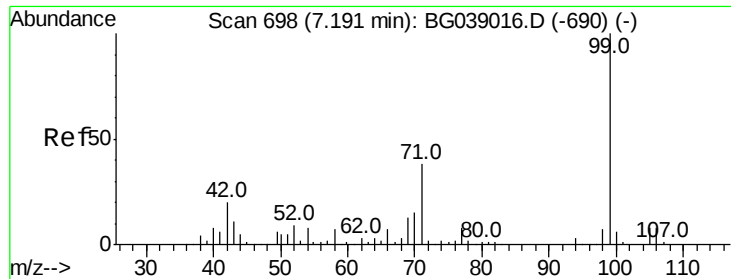

#7

Phenol-d6

Concen: 146.577 ng

RT: 7.17 min Scan# 695

Delta R.T. -0.00 min

Lab File: BG039285.D

Acq: 25 Jan 2019 19:21

Instrument :

BNA_G

ClientSampleId :

TR-05-RO-2-012319


Tot Ion: 99 Resp: 157748

Ion Ratio Lower Upper




99 100

42 19.2 15.8 23.6

71 35.9 30.2 45.4

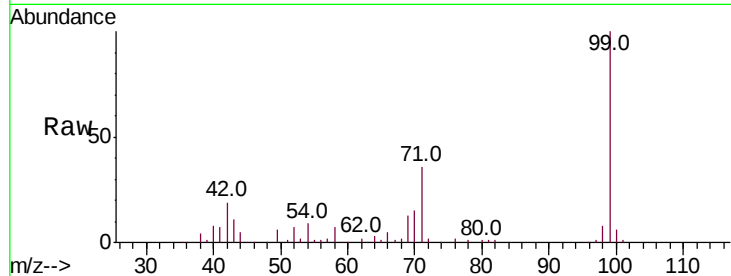

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

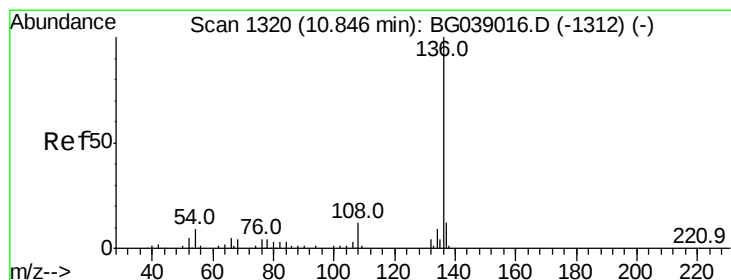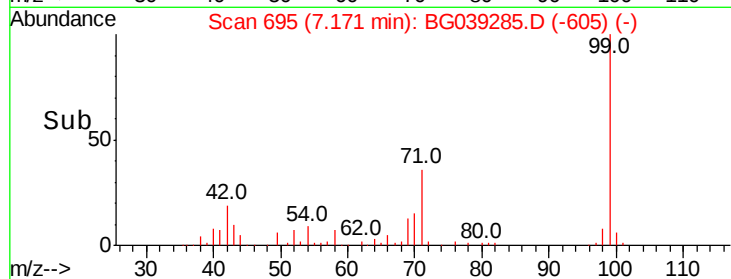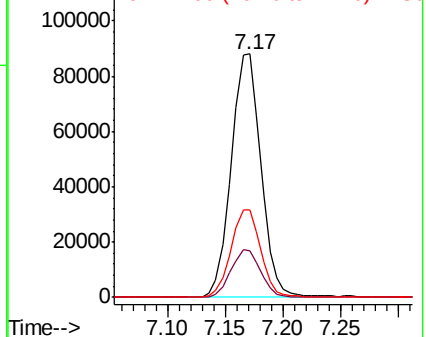

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1316

Delta R.T. -0.01 min

Lab File: BG039285.D

Acq: 25 Jan 2019 19:21

Tgt Ion: 136 Resp: 54346


Ion Ratio Lower Upper

136 100



137 11.4 9.4 14.2


54 10.8 7.2 10.8

68 5.2 3.5 5.3

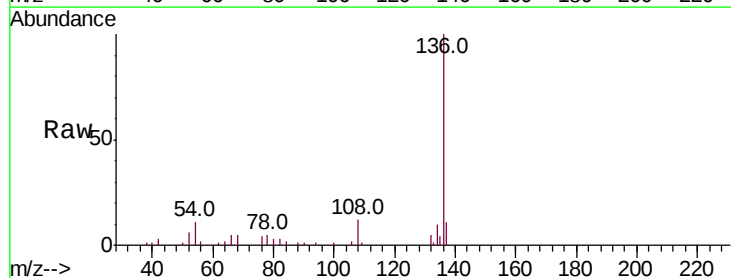

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



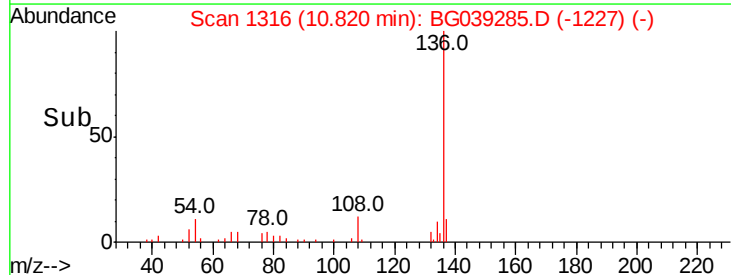
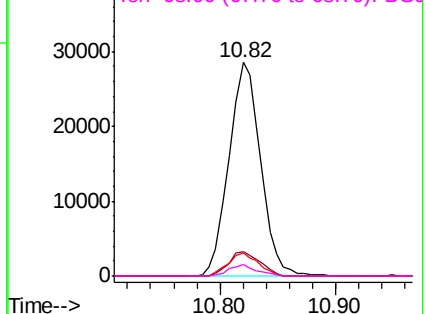


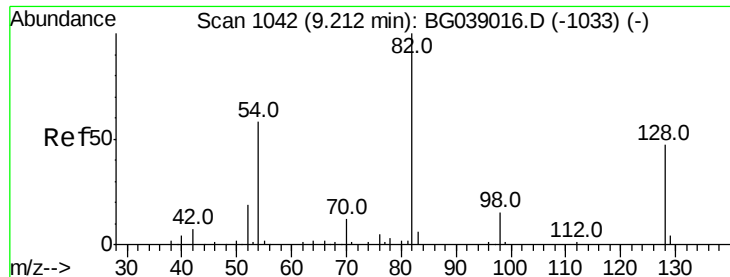

#23
Nitrobenzene-d5
Concen: 90.455 ng
RT: 9.18 min Scan# 1037
Delta R.T. -0.01 min
Lab File: BG039285.D
Acq: 25 Jan 2019 19:21




Instrument :
BNA_G
ClientSampleId :
TR-05-RO-2-012319


Tot Ion: 82 Resp: 89838
Ion Ratio Lower Upper
82 100
128 44.7 37.3 55.9
54 60.0 46.4 69.6

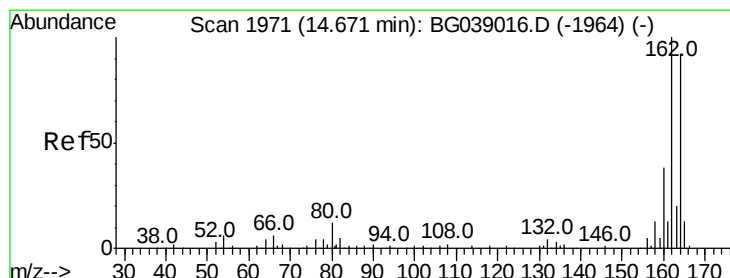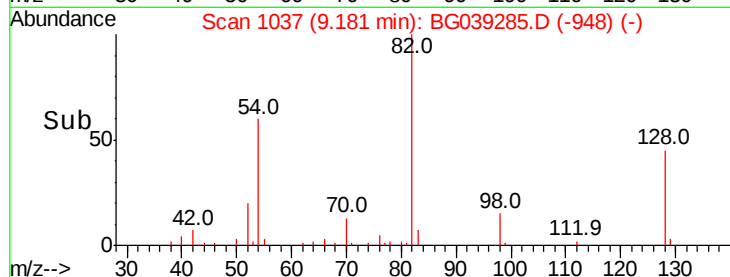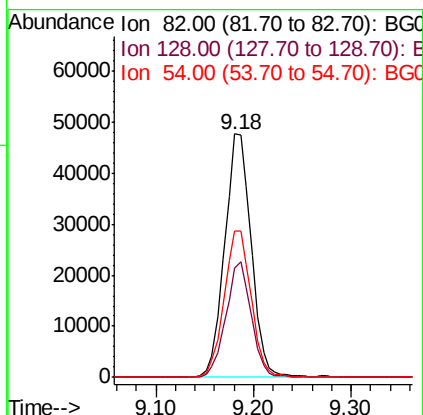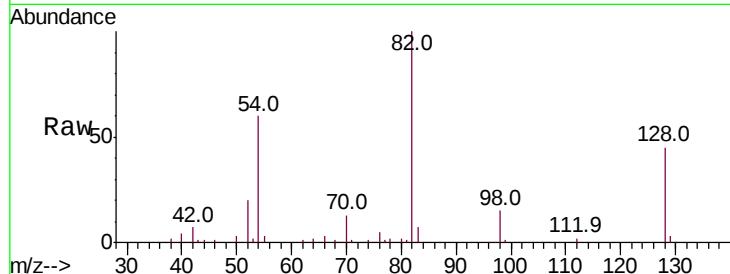

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.65 min Scan# 1967
Delta R.T. -0.01 min
Lab File: BG039285.D
Acq: 25 Jan 2019 19:21

Tgt Ion: 164 Resp: 37127
Ion Ratio Lower Upper
164 100
162 105.1 87.2 130.8
160 45.2 33.3 49.9

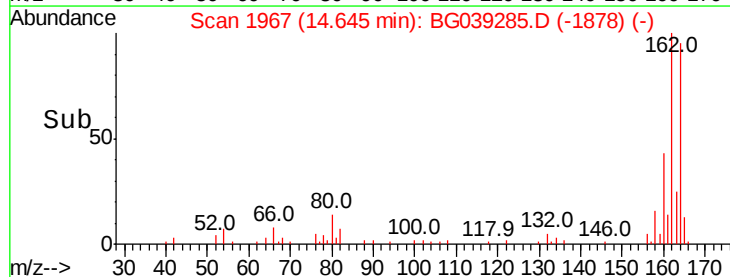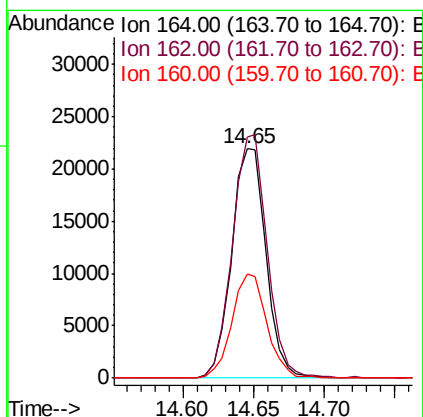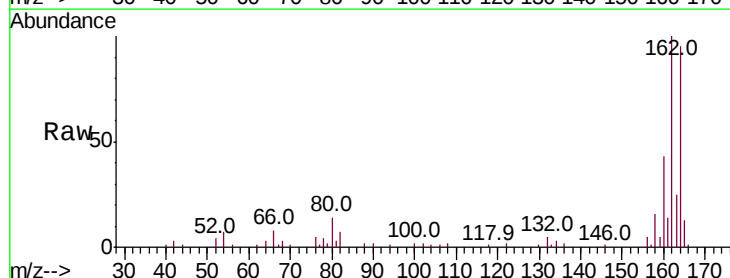


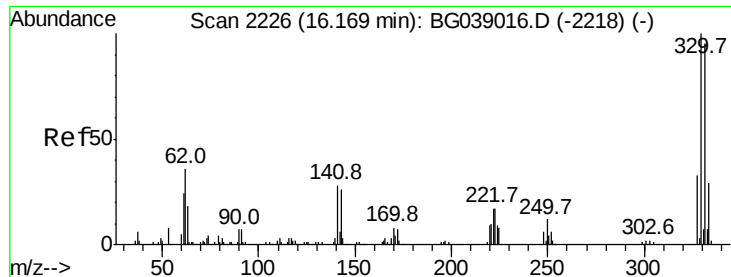




#42
 2,4,6-Tribromophenol
 Concen: 146.650 ng
 RT: 16.14 min Scan# 2221
 Delta R.T. -0.02 min
 Lab File: BG039285.D
 Acq: 25 Jan 2019 19:21

Instrument :
 BNA_G
 ClientSampleId :
 TR-05-RO-2-012319

Tot Ion	Ratio	Lower	Upper
330	100		
332	93.3	75.7	113.5
141	30.7	24.9	37.3

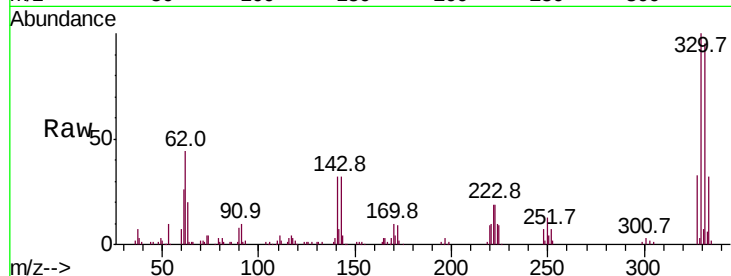


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

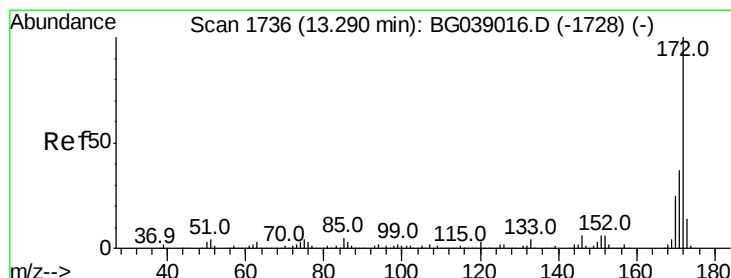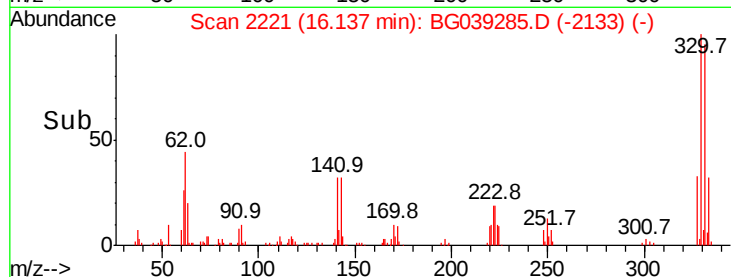
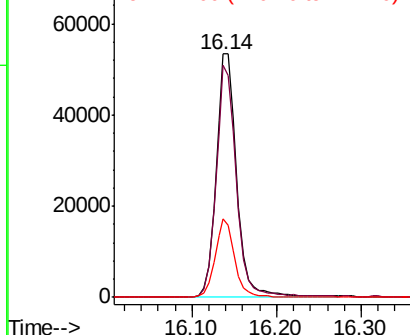



#45
 2-Fluorobiphenyl
 Concen: 94.638 ng
 RT: 13.26 min Scan# 1732
 Delta R.T. -0.01 min
 Lab File: BG039285.D
 Acq: 25 Jan 2019 19:21

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.3	29.4	44.0
170	23.3	20.1	30.1

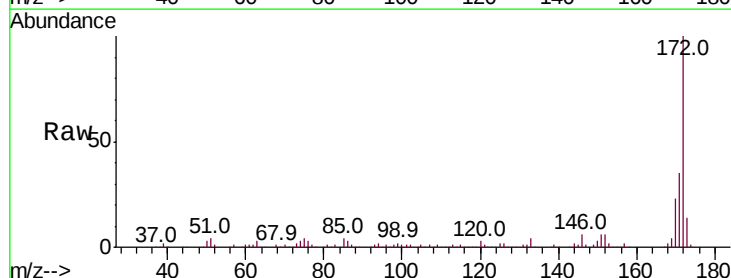

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

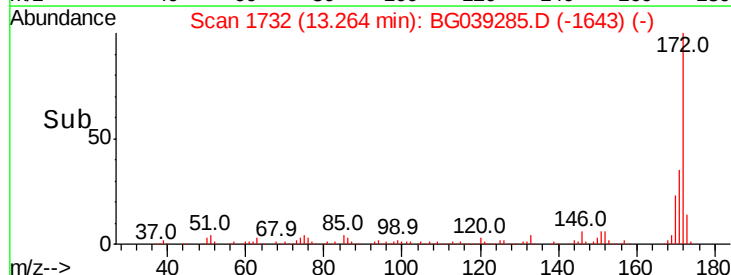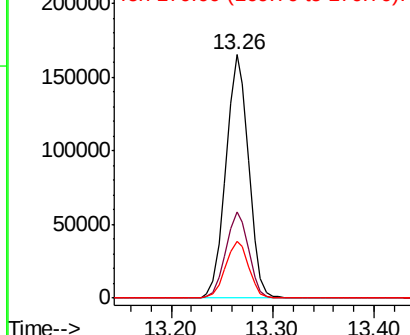


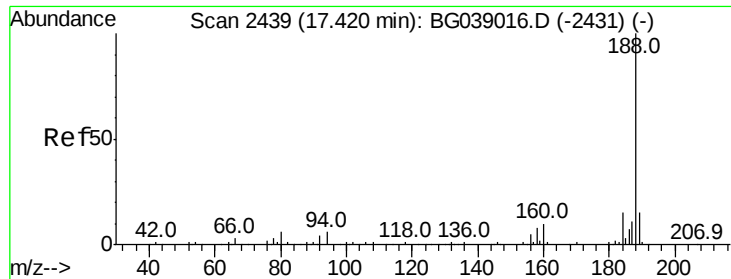




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.39 min Scan# 2435
Delta R.T. -0.01 min
Lab File: BG039285.D
Acq: 25 Jan 2019 19:21

Instrument :
BNA_G
ClientSampleId :
TR-05-RO-2-012319

Tot Ion:188 Resp: 102166
Ion Ratio Lower Upper
188 100
94 5.6 5.0 7.4
80 6.6 4.7 7.1

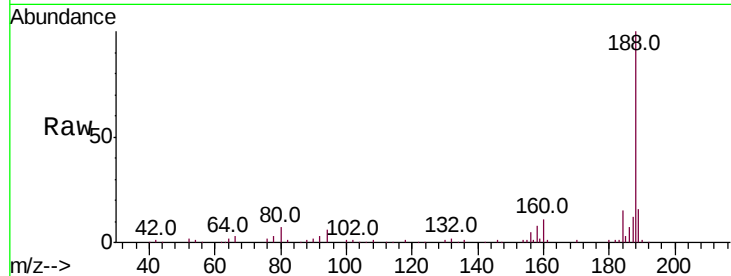


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

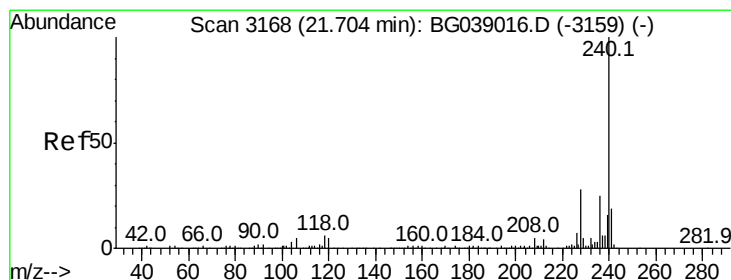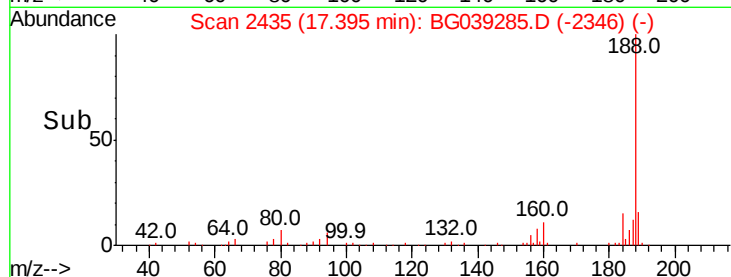
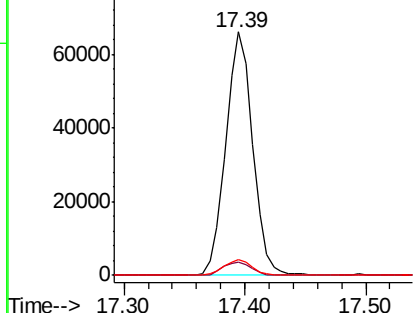



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.67 min Scan# 3162
Delta R.T. -0.02 min
Lab File: BG039285.D
Acq: 25 Jan 2019 19:21

Tgt Ion:240 Resp: 120761
Ion Ratio Lower Upper
240 100
120 5.7 4.3 6.5
236 26.0 20.1 30.1

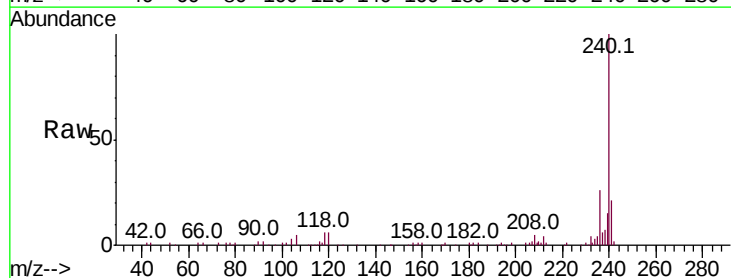

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

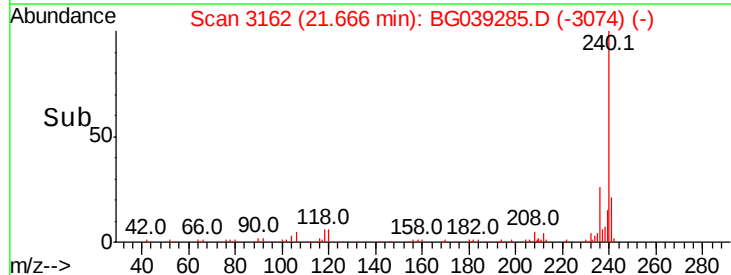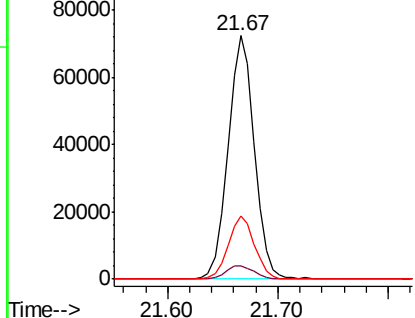

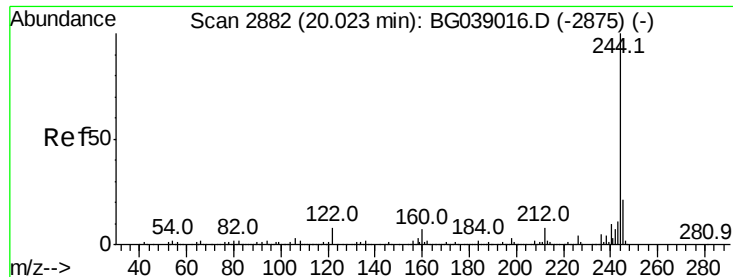

#79

Terphenyl-d14

Concen: 88.948 ng

RT: 20.00 min Scan# 2879

Delta R.T. -0.00 min

Lab File: BG039285.D

Acq: 25 Jan 2019 19:21

Instrument :

BNA_G

ClientSampleId :

TR-05-RO-2-012319





Tot Ion:244 Resp: 580652

Ion Ratio Lower Upper

244 100

212 7.5 6.1 9.1

122 6.3 6.1 9.1

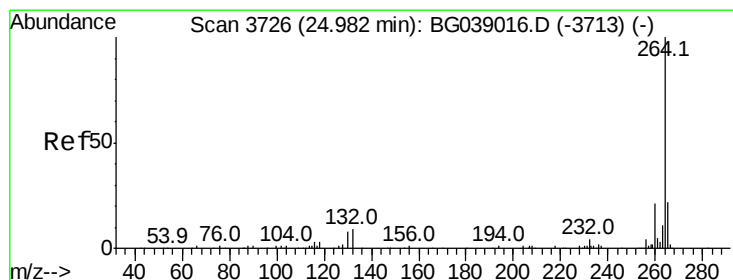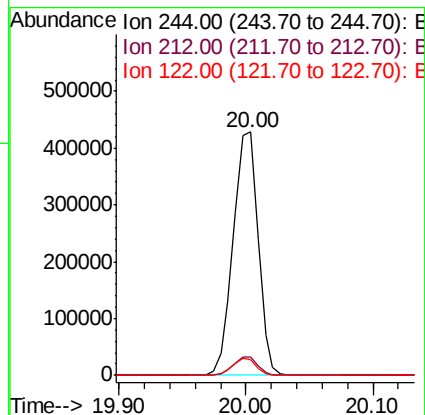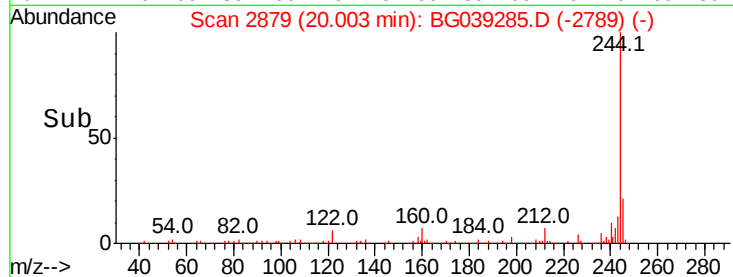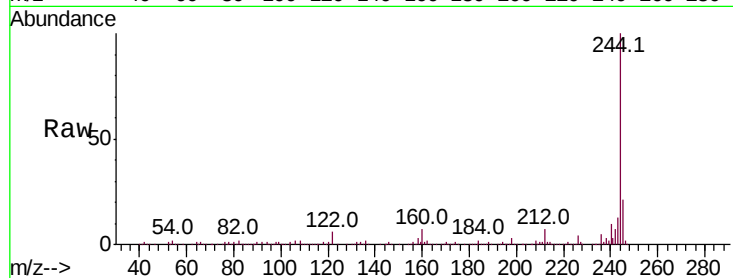

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3717

Delta R.T. -0.02 min

Lab File: BG039285.D

Acq: 25 Jan 2019 19:21

Tgt Ion:264 Resp: 128249

Ion Ratio Lower Upper

264 100

260 22.2 17.0 25.6

265 22.8 17.2 25.8

