

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012519\
 Data File : BG039305.D
 Acq On : 26 Jan 2019 10:24
 Operator : JU/SJ
 Sample : K1229-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 012319-TIPC-F-U-S

Quant Time: Jan 28 04:09:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	14911	20.00	ng	-0.01
21) Naphthalene-d8	10.82	136	53870	20.00	ng	0.00
39) Acenaphthene-d10	14.65	164	39578	20.00	ng	0.00
64) Phenanthrene-d10	17.40	188	116300	20.00	ng	0.00
76) Chrysene-d12	21.67	240	126318	20.00	ng	-0.01
87) Perylene-d12	24.92	264	124600	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	41823	53.21	ng	0.00
7) Phenol-d6	7.16	99	38834	34.33	ng	-0.01
23) Nitrobenzene-d5	9.18	82	97672	99.21	ng	0.00
42) 2,4,6-Tribromophenol	16.14	330	59472	89.64	ng	-0.01
45) 2-Fluorobiphenyl	13.26	172	295880	102.31	ng	-0.01
79) Terphenyl-d14	20.00	244	526788	77.15	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012519\
Data File : BG039305.D
Acq On : 26 Jan 2019 10:24
Operator : JU/SJ
Sample : K1229-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
012319-TIPC-F-U-S

Quant Time: Jan 28 04:09:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

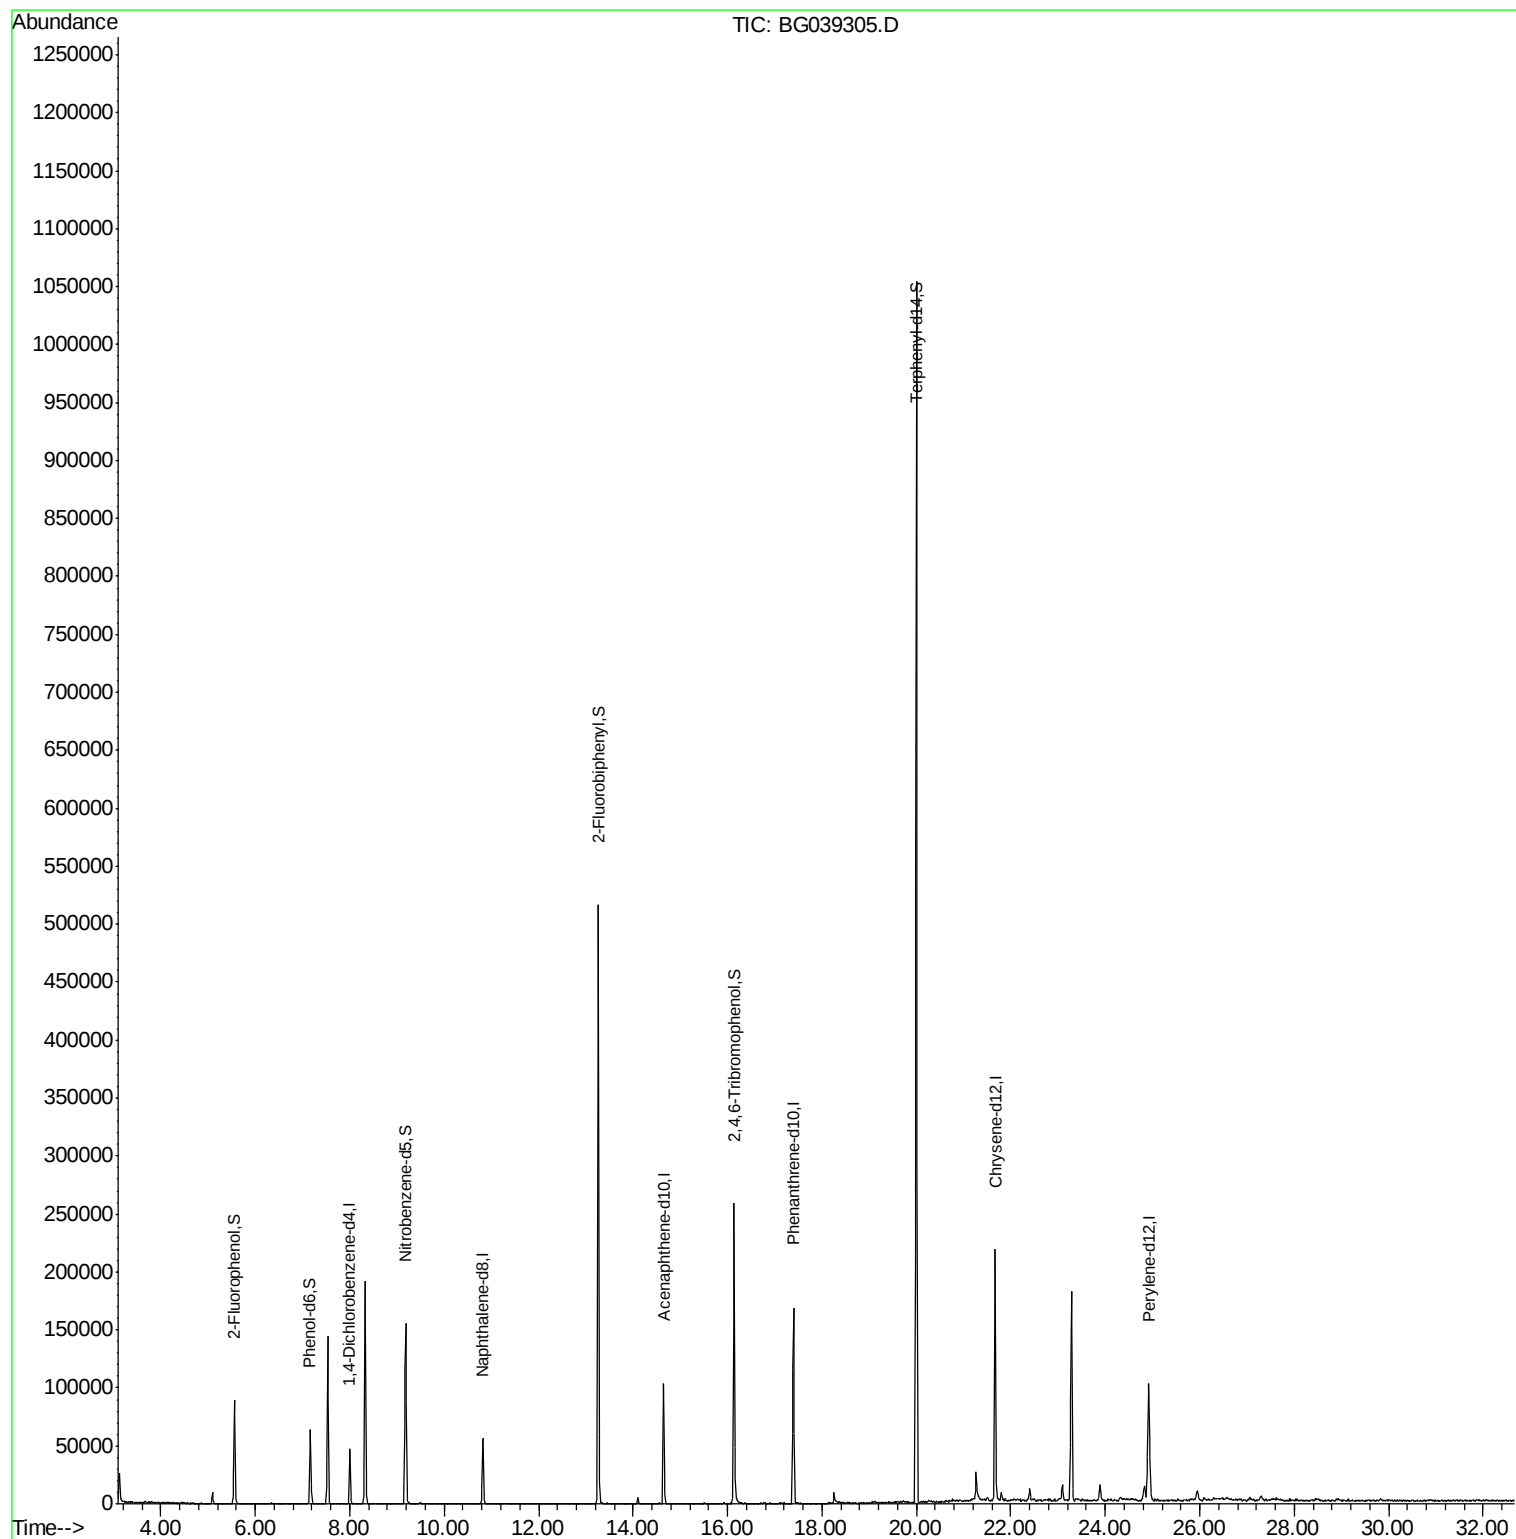

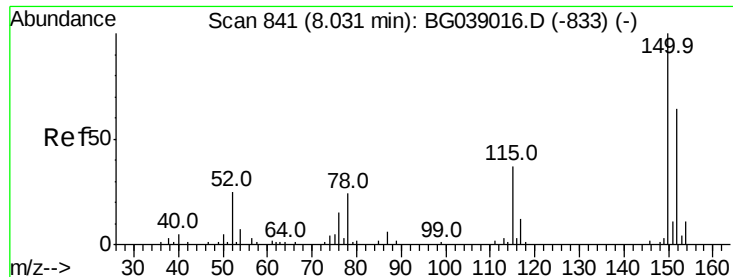


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.00 min Scan# 836
Delta R.T. -0.01 min
Lab File: BG039305.D
Acq: 26 Jan 2019 10:24

Instrument :
BNA_G
ClientSampleId :
012319-TIPC-F-U-S

Tot Ion:152 Resp: 14911
Ion Ratio Lower Upper
152 100
150 152.7 124.7 187.1
115 55.7 46.5 69.7

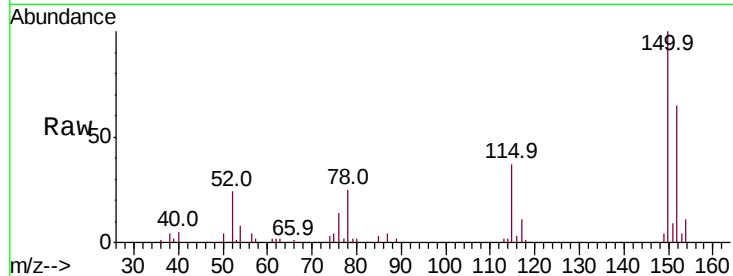


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

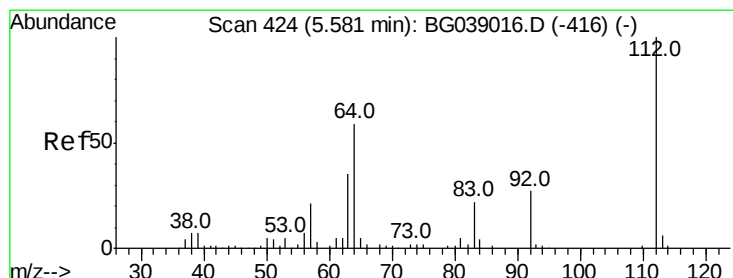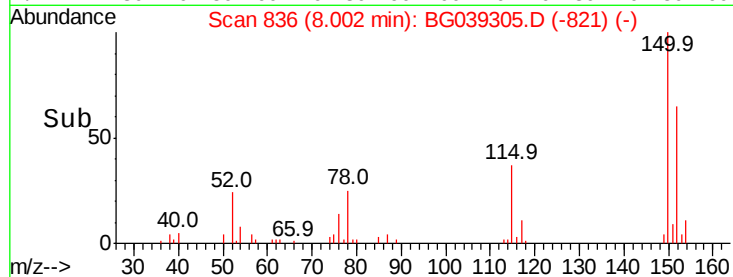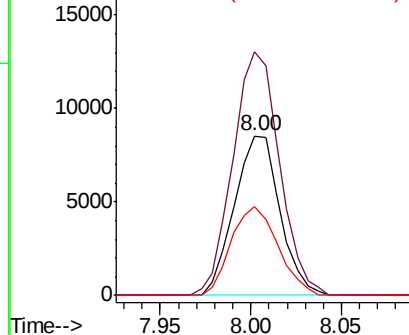



#5


2-Fluorophenol
Concen: 53.207 ng
RT: 5.56 min Scan# 420
Delta R.T. -0.01 min
Lab File: BG039305.D
Acq: 26 Jan 2019 10:24

Tgt Ion:112 Resp: 41823
Ion Ratio Lower Upper
112 100
64 61.9 47.0 70.6
63 34.4 28.0 42.0

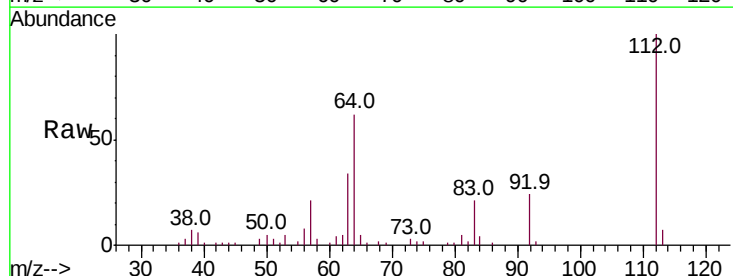

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

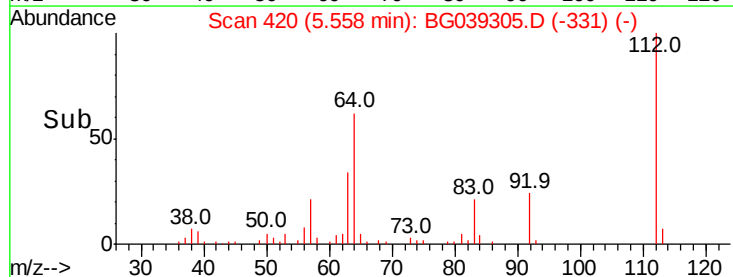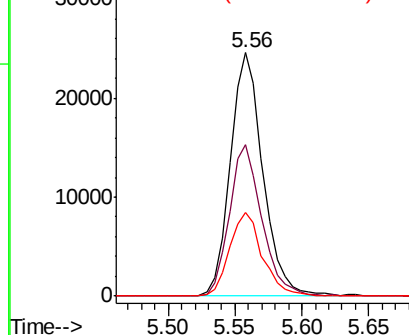

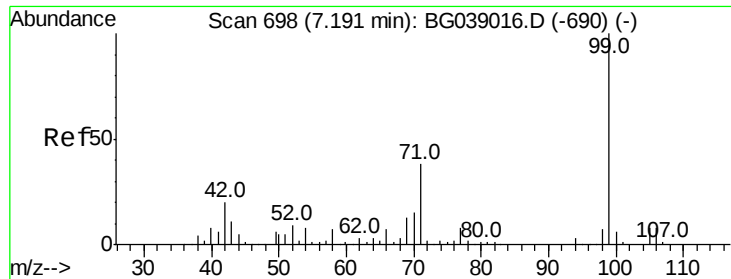

#7

Phenol-d6

Concen: 34.330 ng

RT: 7.16 min Scan# 693

Delta R.T. -0.01 min

Lab File: BG039305.D

Acq: 26 Jan 2019 10:24

Instrument :

BNA_G

ClientSampleId :

012319-TIPC-F-U-S


Tot Ion: 99 Resp: 38834

Ion Ratio Lower Upper




99 100

42 20.3 15.8 23.6

71 39.2 30.2 45.4

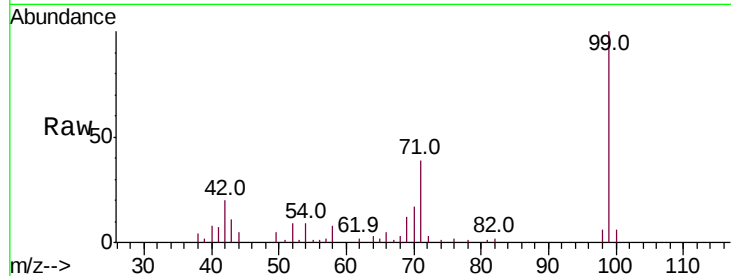

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

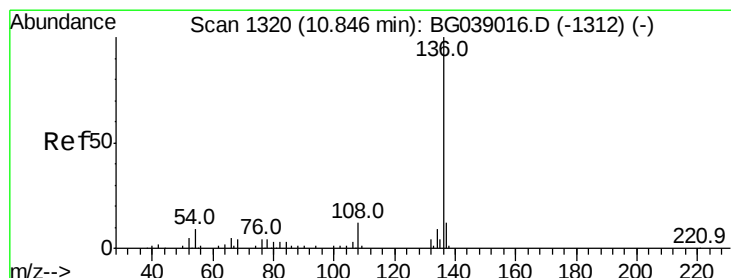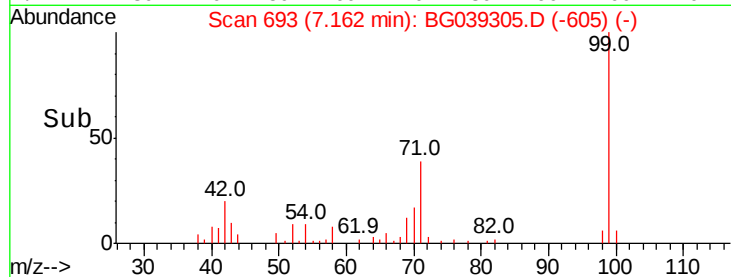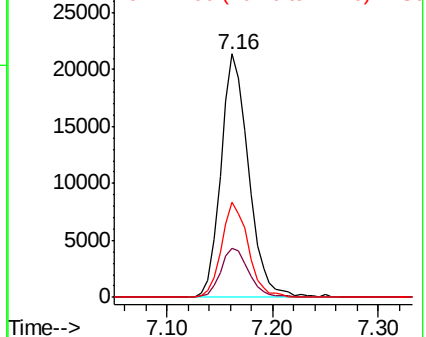

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1316

Delta R.T. -0.01 min

Lab File: BG039305.D

Acq: 26 Jan 2019 10:24

Tgt Ion: 136 Resp: 53870


Ion Ratio Lower Upper

136 100



137 11.2 9.4 14.2


54 10.0 7.2 10.8

68 4.1 3.5 5.3

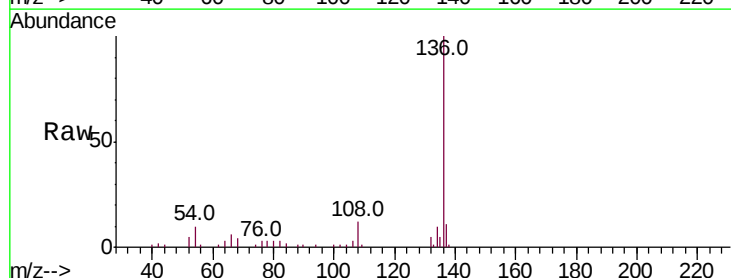

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

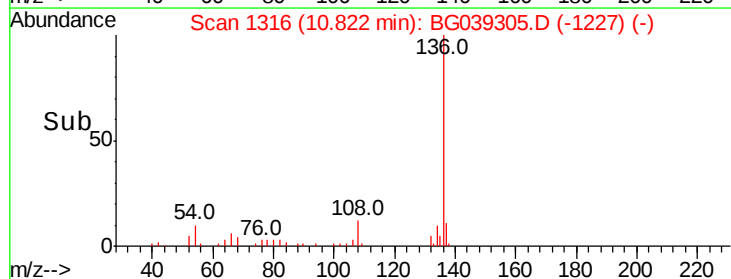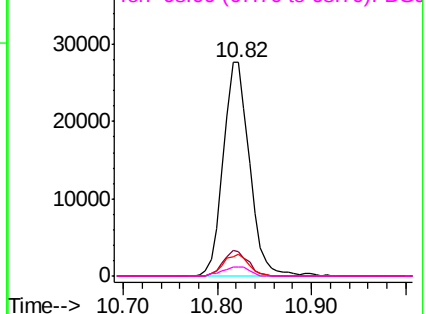


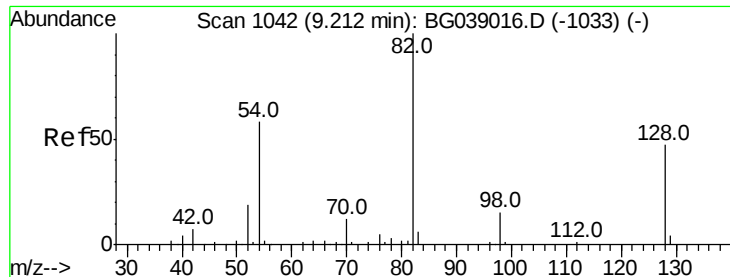




#23
 Nitrobenzene-d5
 Concen: 99.212 ng
 RT: 9.18 min Scan# 1037
 Delta R.T. -0.01 min
 Lab File: BG039305.D
 Acq: 26 Jan 2019 10:24

Instrument :
 BNA_G
 ClientSampleId :
 012319-TIPC-F-U-S

Tot Ion: 82 Resp: 97672
 Ion Ratio Lower Upper
 82 100
 128 45.7 37.3 55.9
 54 59.9 46.4 69.6

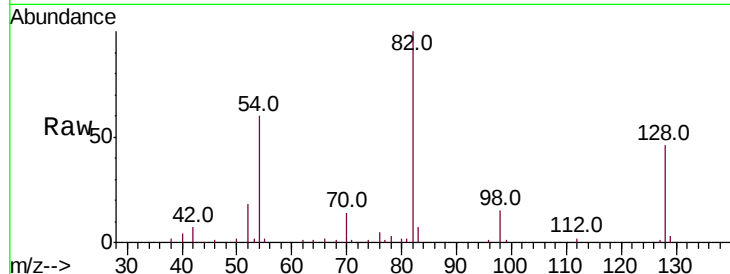


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

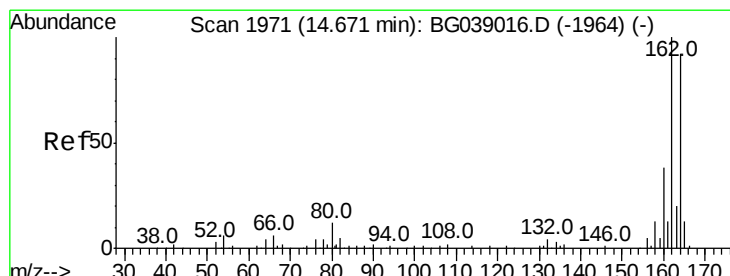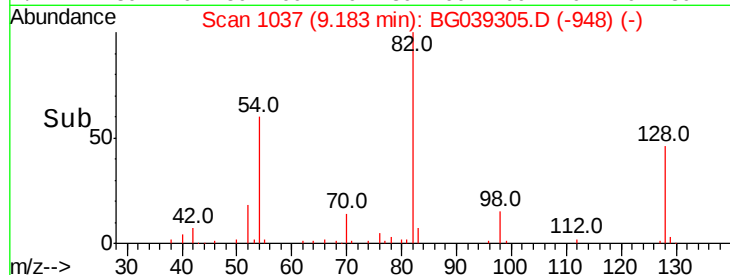
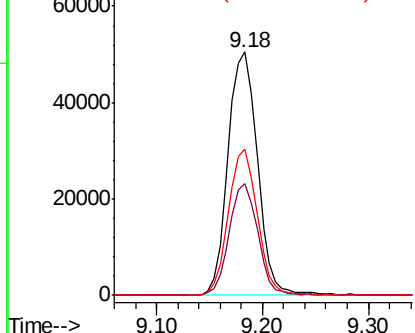



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.65 min Scan# 1967
 Delta R.T. -0.01 min
 Lab File: BG039305.D
 Acq: 26 Jan 2019 10:24

Tgt Ion: 164 Resp: 39578
 Ion Ratio Lower Upper
 164 100
 162 99.2 87.2 130.8
 160 44.7 33.3 49.9

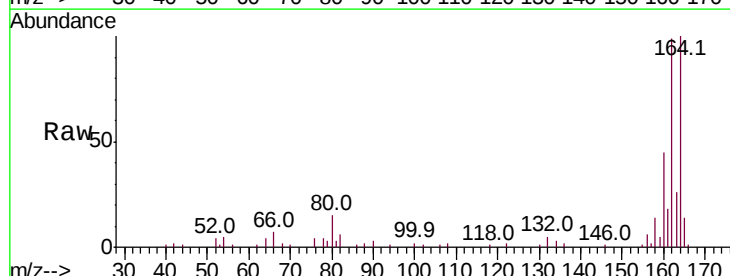

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

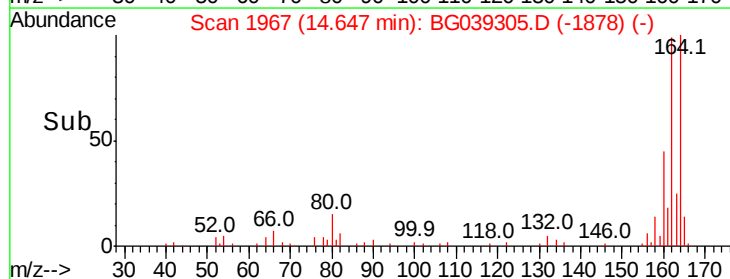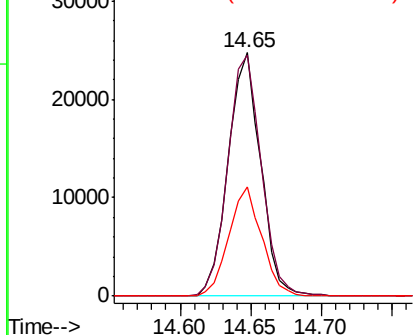

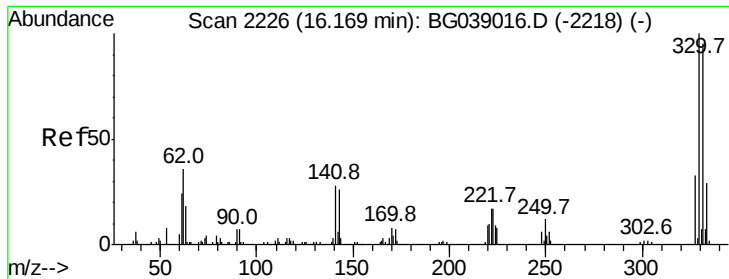

#42

2,4,6-Tribromophenol

Concen: 89.642 ng

RT: 16.14 min Scan# 2221

Delta R.T. -0.01 min

Lab File: BG039305.D

Acq: 26 Jan 2019 10:24

Instrument :

BNA_G

ClientSampleId :

012319-TIPC-F-U-S


Tot Ion:330 Resp: 59472

Ion Ratio Lower Upper




330 100

332 94.7 75.7 113.5

141 31.7 24.9 37.3

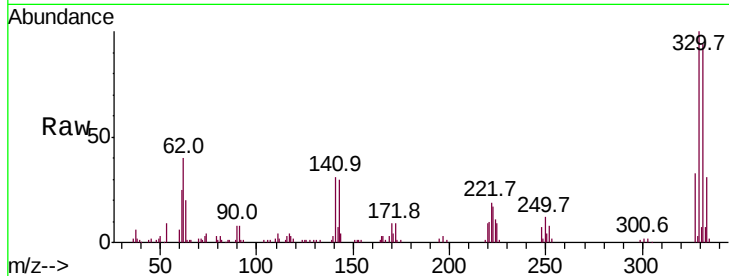

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

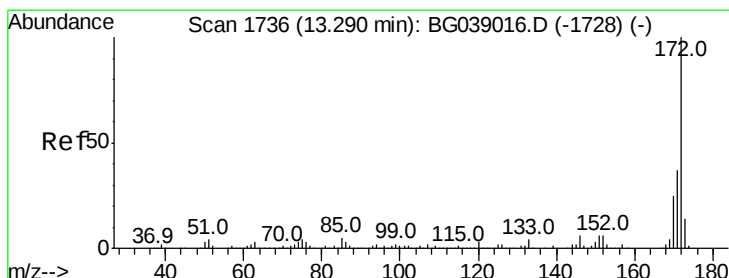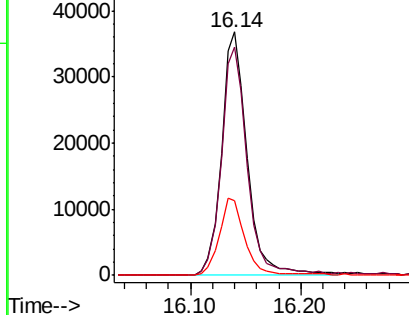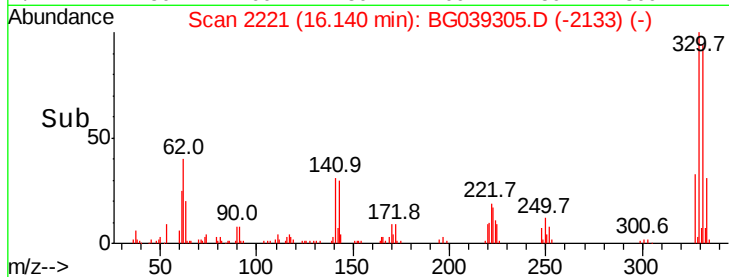

#45

2-Fluorobiphenyl

Concen: 102.312 ng

RT: 13.26 min Scan# 1731

Delta R.T. -0.01 min

Lab File: BG039305.D

Acq: 26 Jan 2019 10:24


Tgt Ion:172 Resp: 295880

Ion Ratio Lower Upper



172 100


171 35.1 29.4 44.0

170 23.4 20.1 30.1

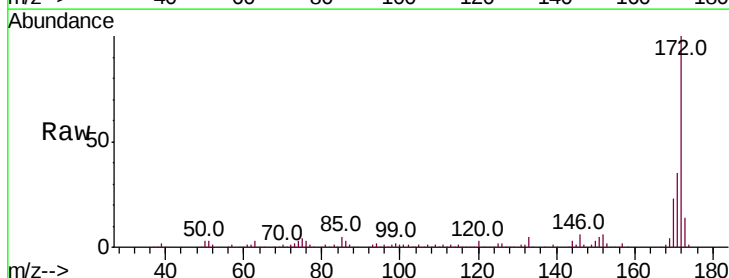

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

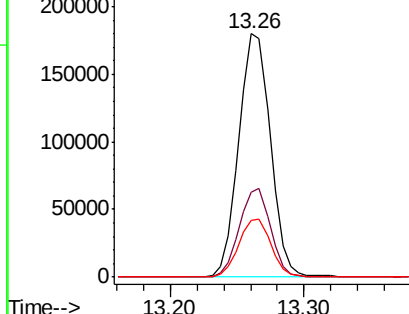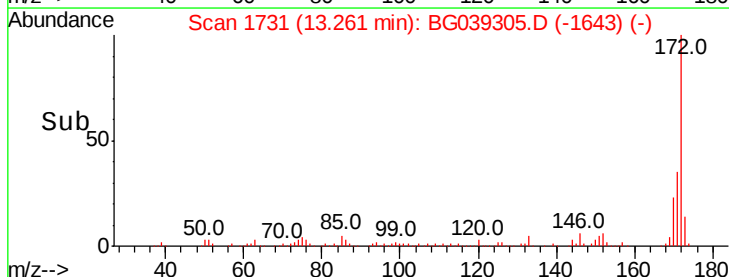

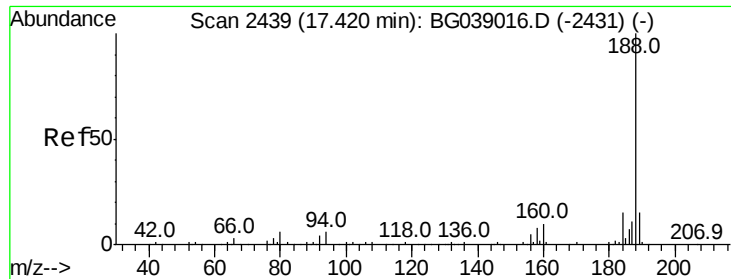

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.40 min Scan# 2435

Delta R.T. -0.01 min

Lab File: BG039305.D

Acq: 26 Jan 2019 10:24

Instrument :

BNA_G

ClientSampleId :

012319-TIPC-F-U-S


Tot Ion:188 Resp: 116300

Ion Ratio Lower Upper

188 100

94 6.7 5.0 7.4




80 7.2 4.7 7.1#

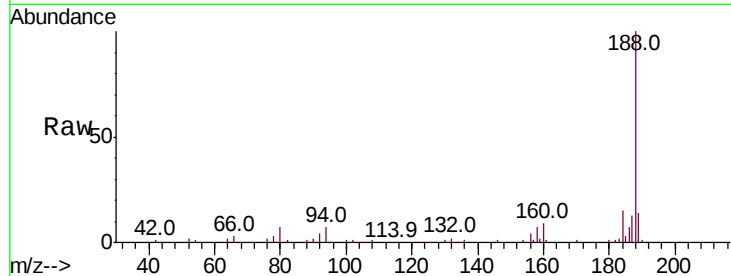

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

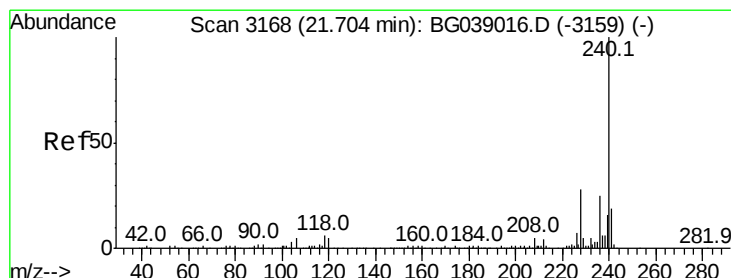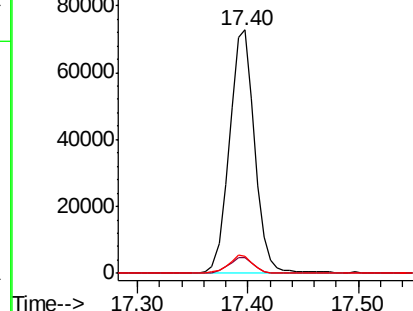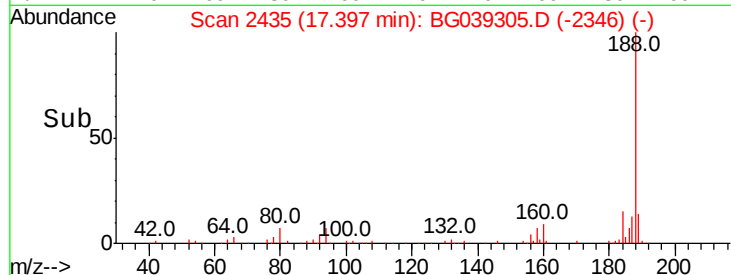

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.67 min Scan# 3162

Delta R.T. -0.01 min

Lab File: BG039305.D

Acq: 26 Jan 2019 10:24


Tgt Ion:240 Resp: 126318

Ion Ratio Lower Upper

240 100

120 7.7 4.3 6.5#



236 26.1 20.1 30.1

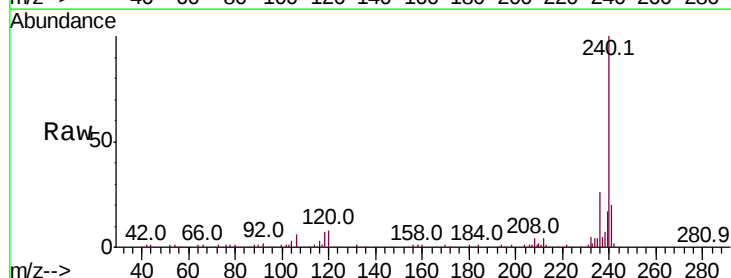


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

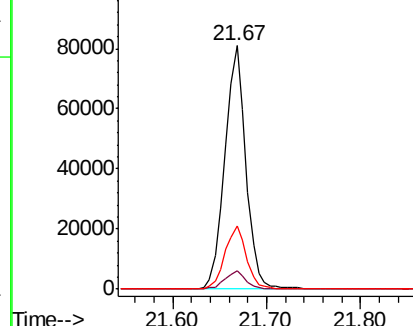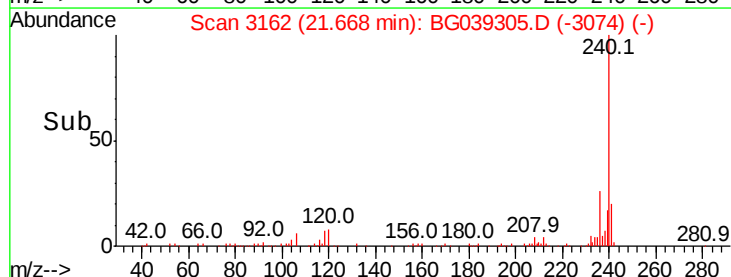

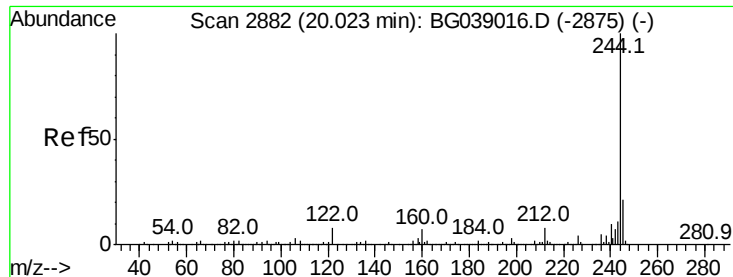

#79

Terphenyl-d14

Concen: 77.147 ng

RT: 20.00 min Scan# 2878

Delta R.T. -0.01 min

Lab File: BG039305.D

Acq: 26 Jan 2019 10:24

Instrument :

BNA_G

ClientSampleId :

012319-TIPC-F-U-S


Tot Ion:244 Resp: 526788

Ion Ratio Lower Upper

244 100

212 7.3 6.1 9.1




122 7.0 6.1 9.1

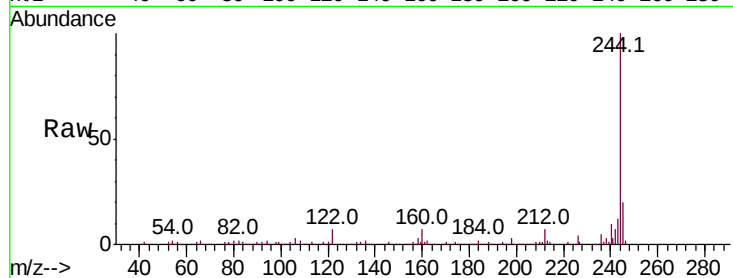

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

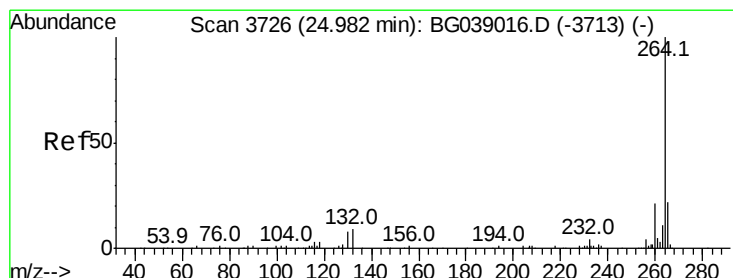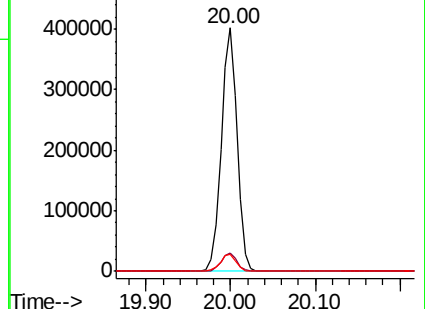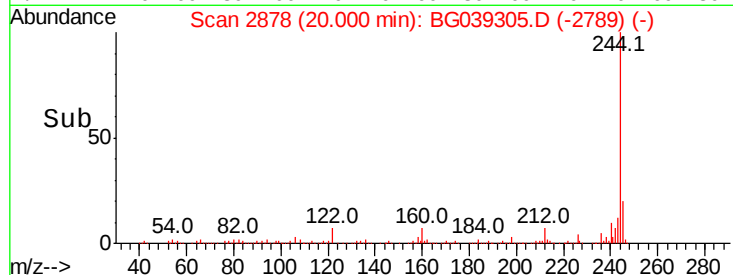

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.92 min Scan# 3715

Delta R.T. -0.03 min

Lab File: BG039305.D

Acq: 26 Jan 2019 10:24


Tgt Ion:264 Resp: 124600

Ion Ratio Lower Upper

264 100

260 23.5 17.0 25.6

265 21.4 17.2 25.8

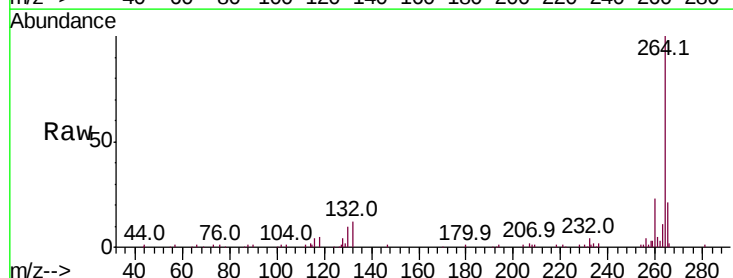

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

