


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012519\
 Data File : BG039293.D
 Acq On : 26 Jan 2019 1:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 18 04:20:14 2019

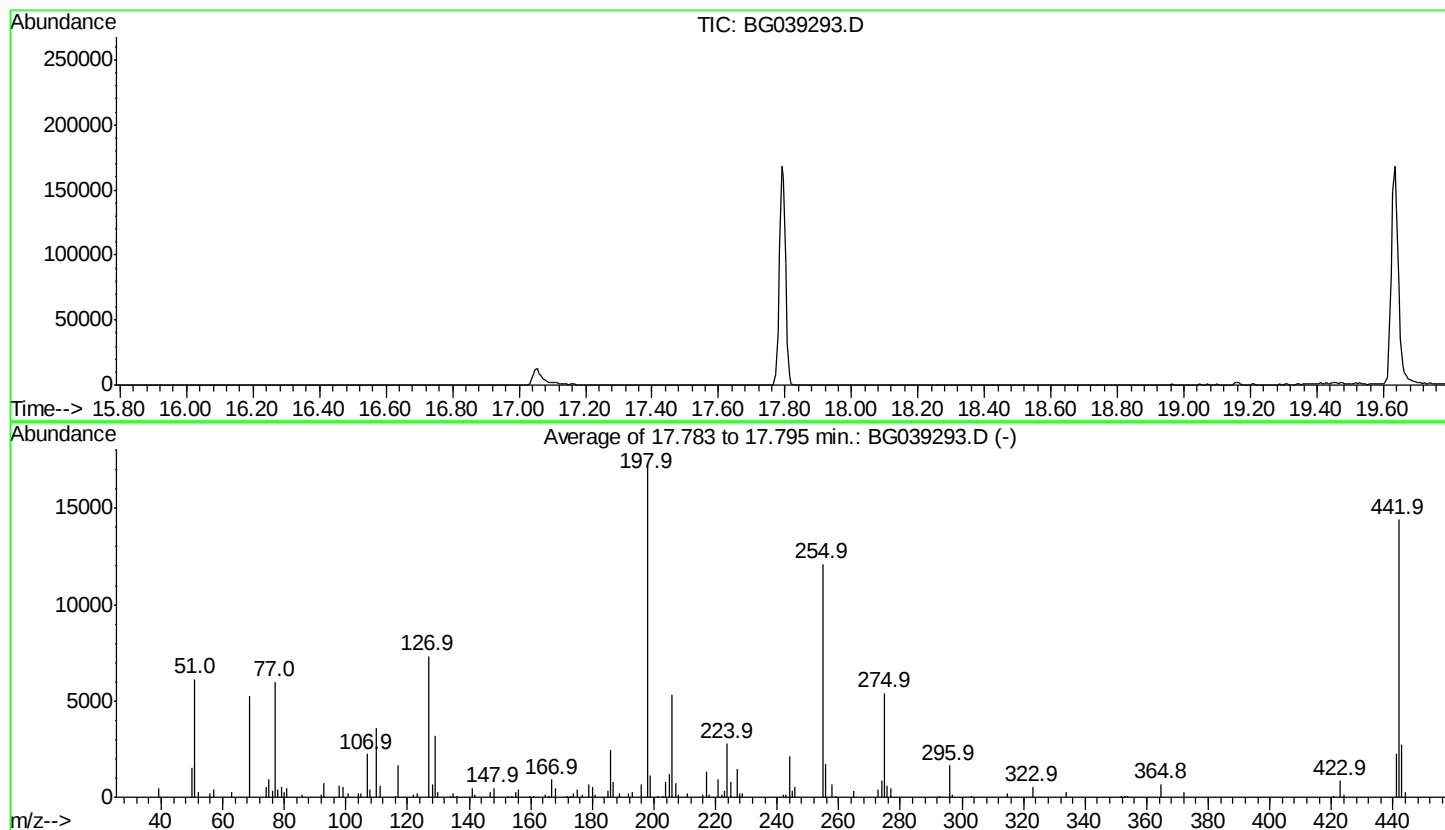

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	6119	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.7	5282	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	7338	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17217	PASS
199	198	5	9	6.7	1158	PASS
275	198	10	60	31.5	5416	PASS
365	198	1	100	4.0	689	PASS
441	198	0.01	100	13.1	2250	PASS
442	198	50	100	83.6	14397	PASS
443	442	15	24	18.7	2696	PASS