
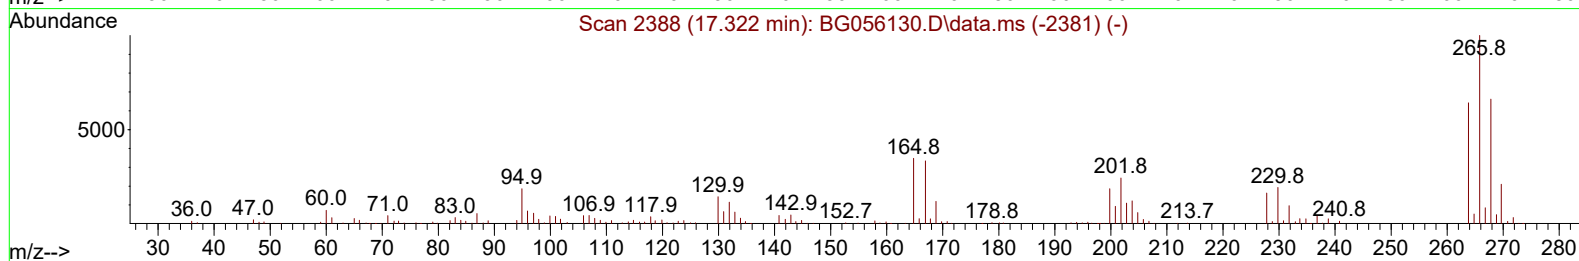
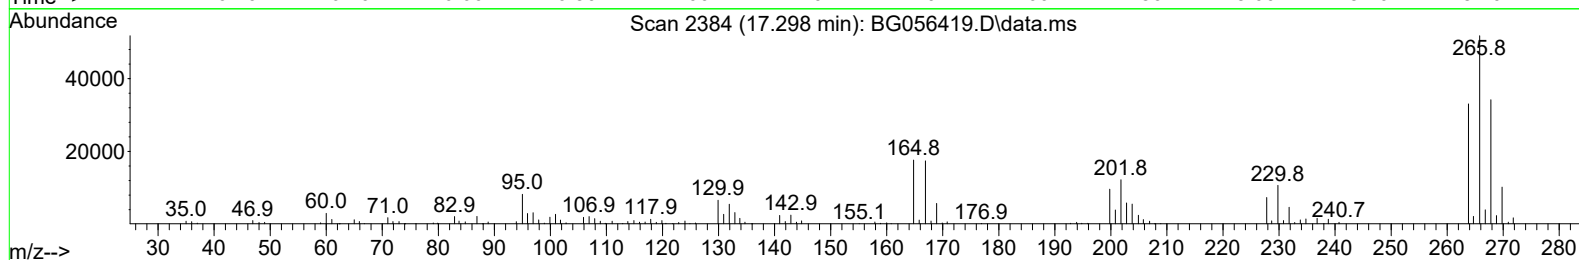


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012523\
Data File : BG056419.D
Acq On : 25 Jan 2023 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 03:35:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 04:54:56 2023
Response via : Initial Calibration

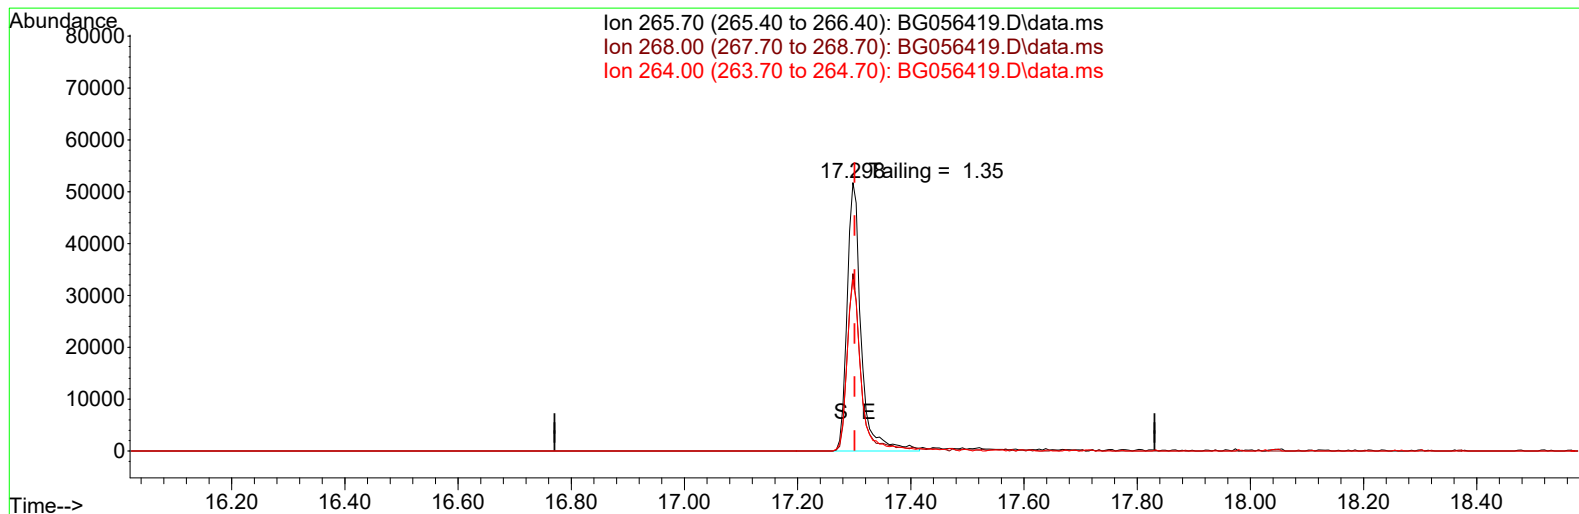

TIC: BG056419.D\data.ms

(70) Pentachlorophenol (C)




17.298min (-0.003) 17365.70 ng

response 88117

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.09
264.00	64.30	68.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012523\
Data File : BG056419.D
Acq On : 25 Jan 2023 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 03:35:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 04:54:56 2023
Response via : Initial Calibration

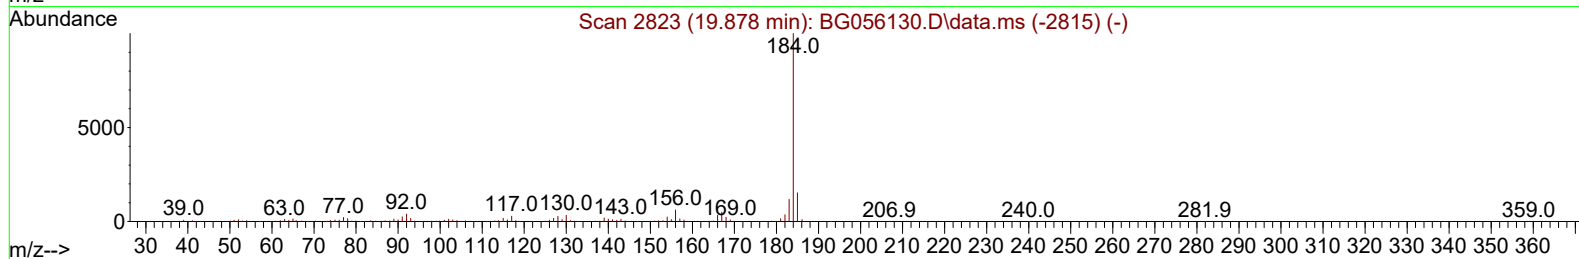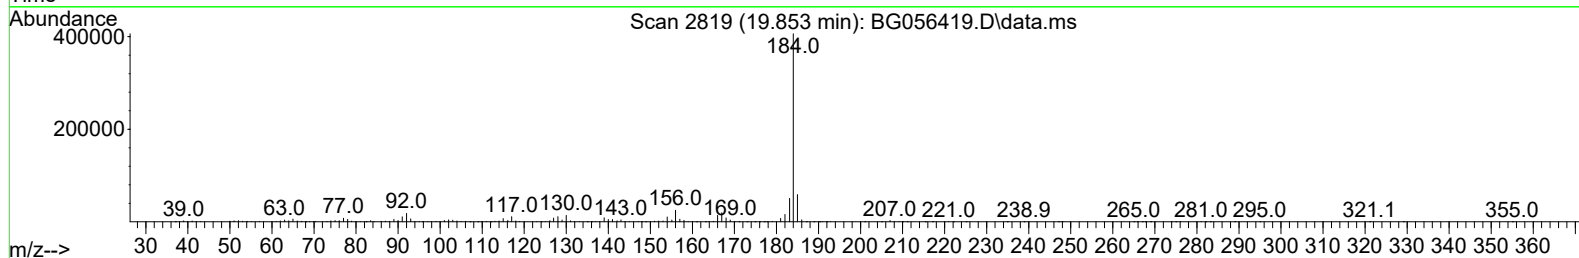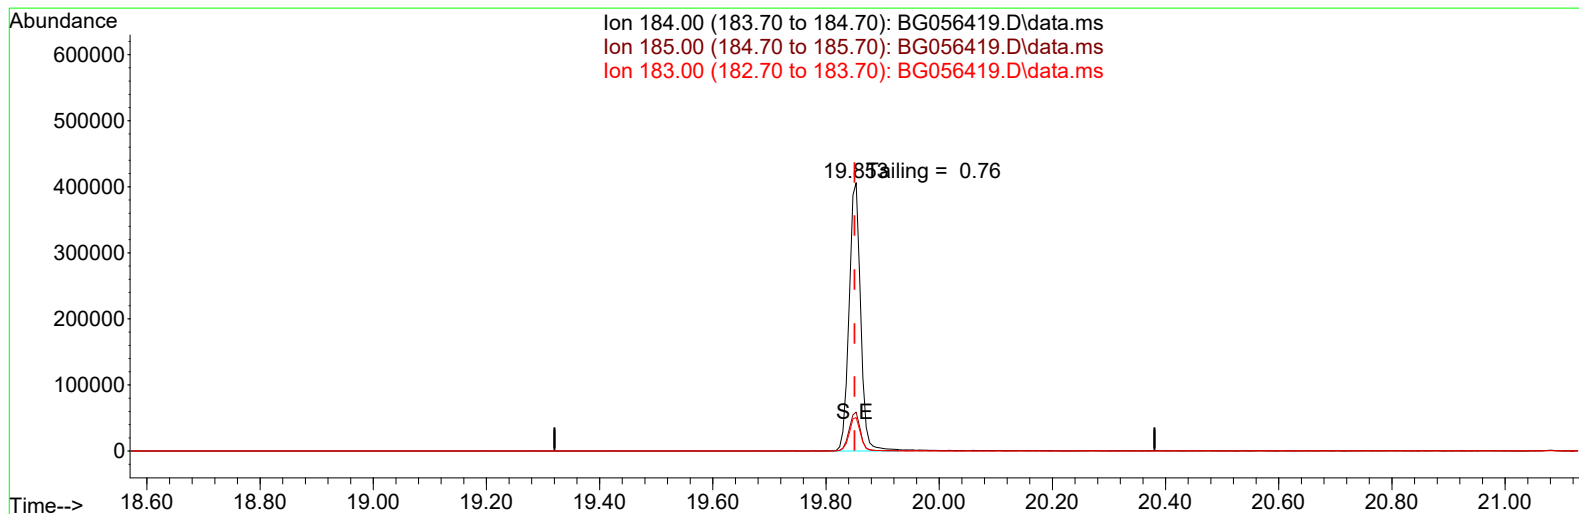

TIC: BG056419.D\data.ms

(77) Benzidine**19.853min (+ 0.003) 239550.16 ng****response 579246**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.48
183.00	11.70	12.46
0.00	0.00	0.00