

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012523\
 Data File : BG056421.D
 Acq On : 25 Jan 2023 11:49
 Operator : CG/JU
 Sample : PB150355BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB150355BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.329	340	347	356	rBB	115803	172944	5.09%	1.399%
2	5.816	423	430	442	rBV	477271	768366	22.62%	6.217%
3	7.438	698	706	720	rBV	484362	825302	24.30%	6.677%
4	8.290	845	851	859	rBB	111565	188918	5.56%	1.528%
5	9.471	1044	1052	1061	rBV	282157	509664	15.00%	4.124%
6	11.128	1326	1334	1344	rBB	156955	288728	8.50%	2.336%
7	13.537	1736	1744	1752	rBV	1278004	1890649	55.66%	15.297%
8	14.912	1970	1978	1986	rVB	334316	536413	15.79%	4.340%
9	16.392	2223	2230	2248	rBV	949161	1426930	42.01%	11.545%
10	17.650	2437	2444	2452	rVB	483169	748803	22.04%	6.058%
11	20.223	2876	2882	2888	rBV	2744090	3396835	100.00%	27.483%
12	21.939	3167	3174	3181	rVB2	458879	780058	22.96%	6.311%
13	25.370	3749	3758	3773	rVB2	257006	826168	24.32%	6.684%




Sum of corrected areas: 12359778

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012523\
Data File : BG056421.D
Acq On : 25 Jan 2023 11:49
Operator : CG/JU
Sample : PB150355BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150355BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

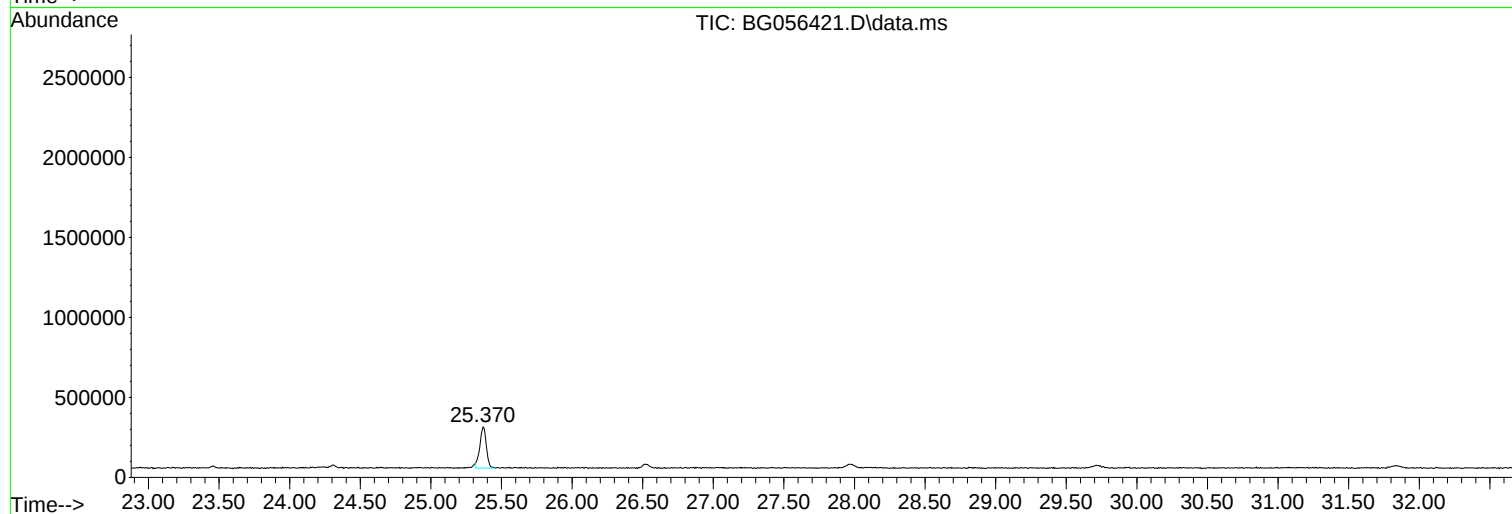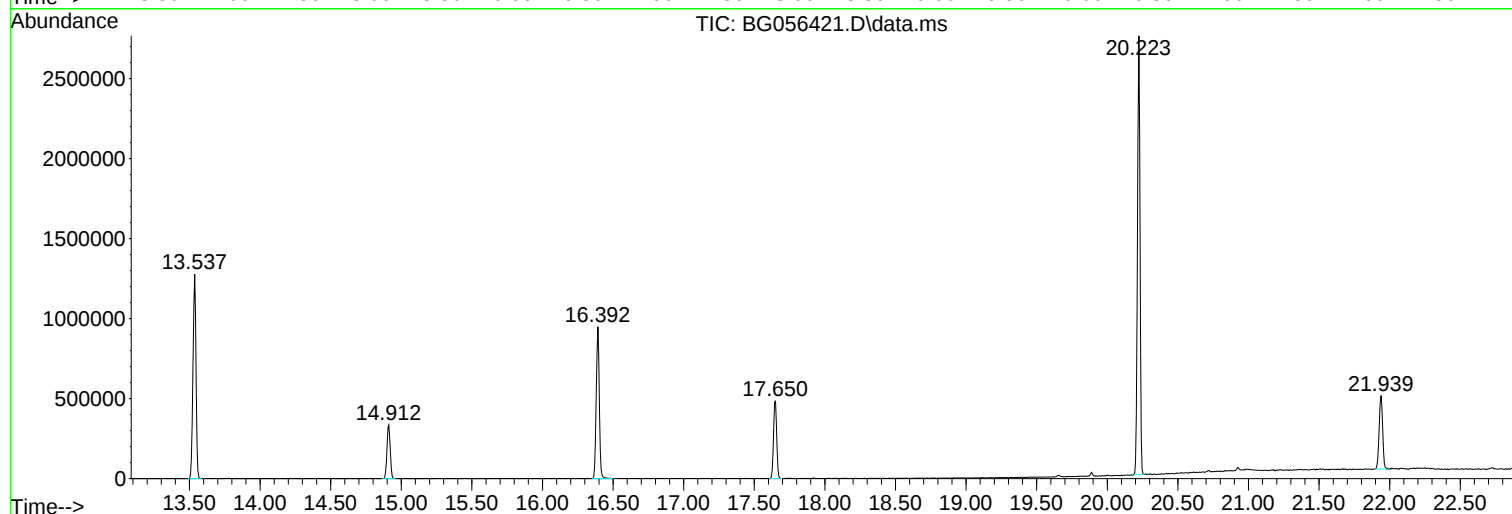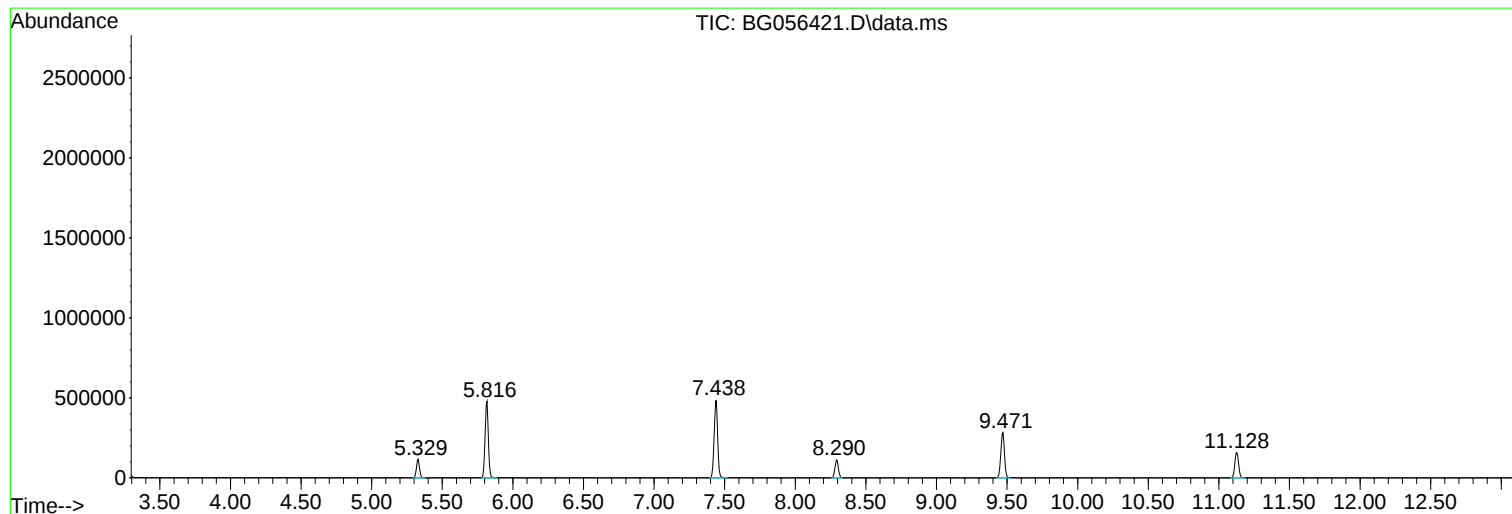

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012523\
Data File : BG056421.D
Acq On : 25 Jan 2023 11:49
Operator : CG/JU
Sample : PB150355BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
PB150355BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.329	18.31 ng	172944	1,4-Dichlorobenzene-d4			8.296
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	45
2	2-Pentanol, 2,4-dimethyl-		116	C7H16O	000625-06-9	42
3	Guanidine		59	CH5N3	000113-00-8	37
4	Propane, 1-ethoxy-2-methyl-		102	C6H14O	000627-02-1	35
5	Acetic acid, cyano-, 1,1-dimethy...		141	C7H11NO2	001116-98-9	35

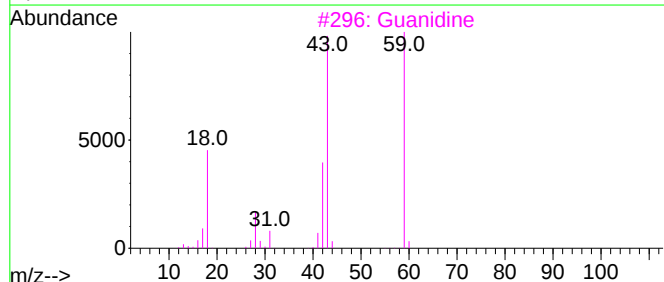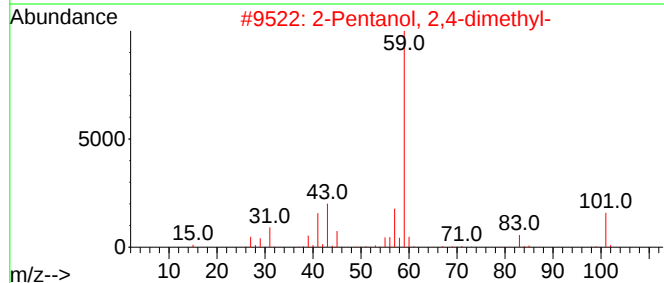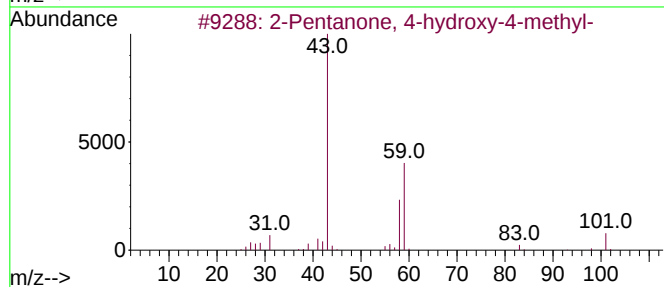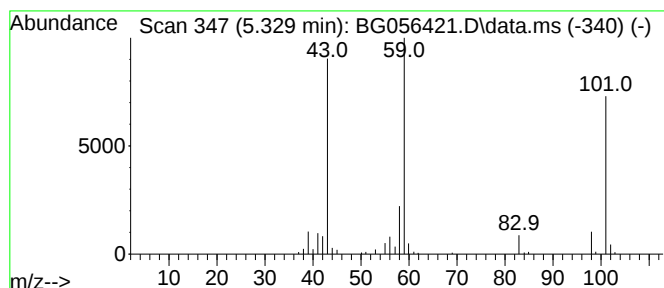

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012523\
Data File : BG056421.D
Acq On : 25 Jan 2023 11:49
Operator : CG/JU
Sample : PB150355BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150355BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.329	18.3	ng	172944	1	8.296	188918	20.0