


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012523\
Data File : BG056419.D
Acq On : 25 Jan 2023 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 25 04:54:56 2023

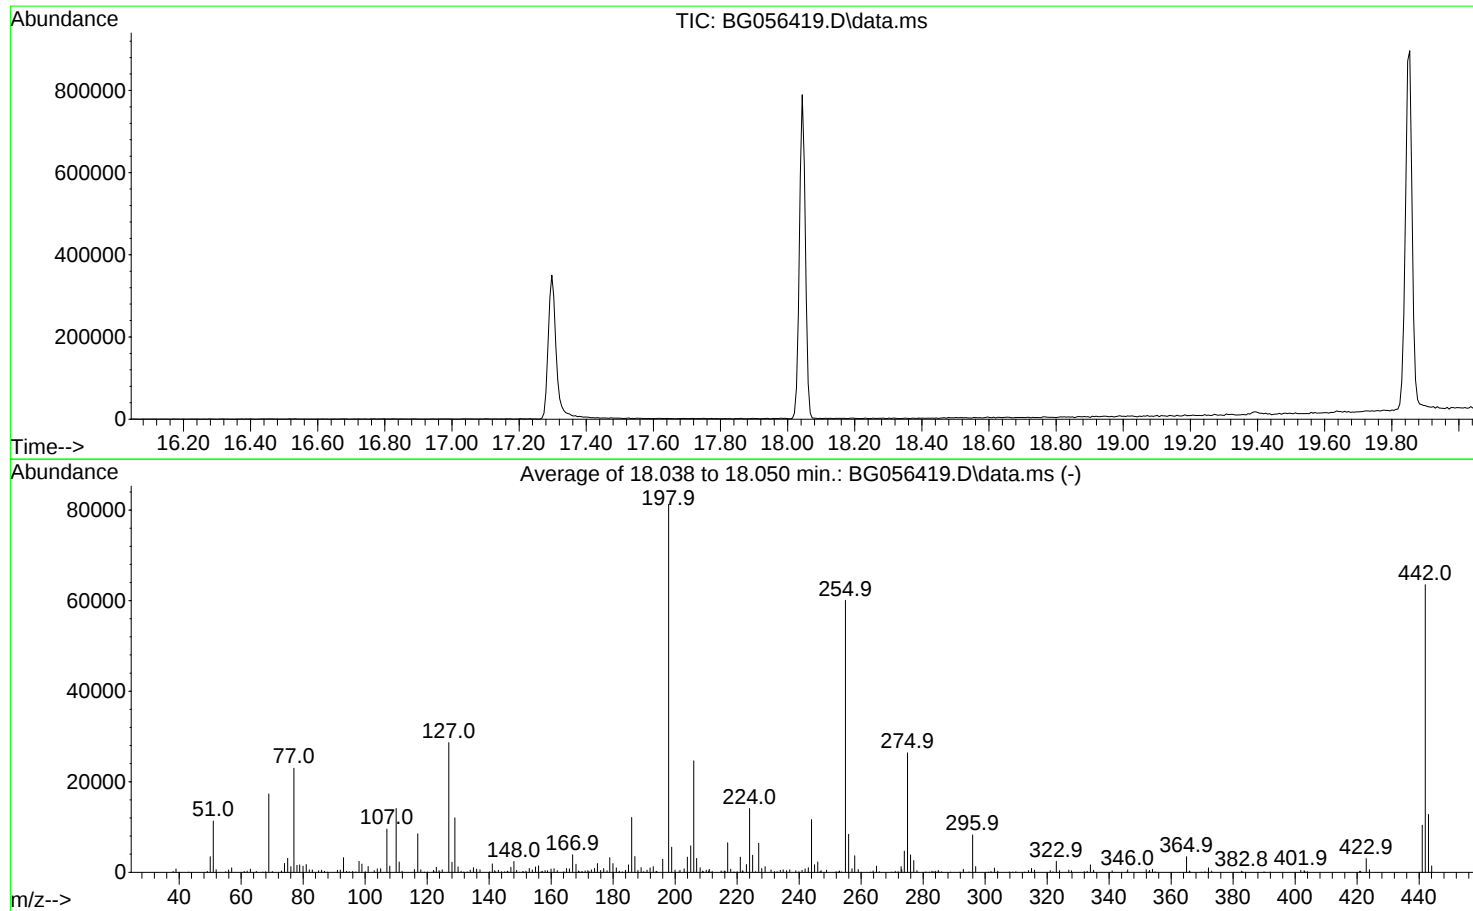




AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	13.9	11321	PASS
68	69	0.00	2	0.6	108	PASS
69	198	0.00	100	21.3	17286	PASS
70	69	0.00	2	0.6	110	PASS
127	198	10	80	35.3	28645	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81256	PASS
199	198	5	9	6.8	5527	PASS
275	198	10	60	32.5	26397	PASS
365	198	1	100	4.2	3433	PASS
441	198	0.01	100	12.8	10396	PASS
442	442	50	100	100.0	63523	PASS
443	442	15	24	20.1	12784	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012523\
Data File : BG056419.D
Acq On : 25 Jan 2023 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 26 03:35:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 04:54:56 2023
Response via : Initial Calibration

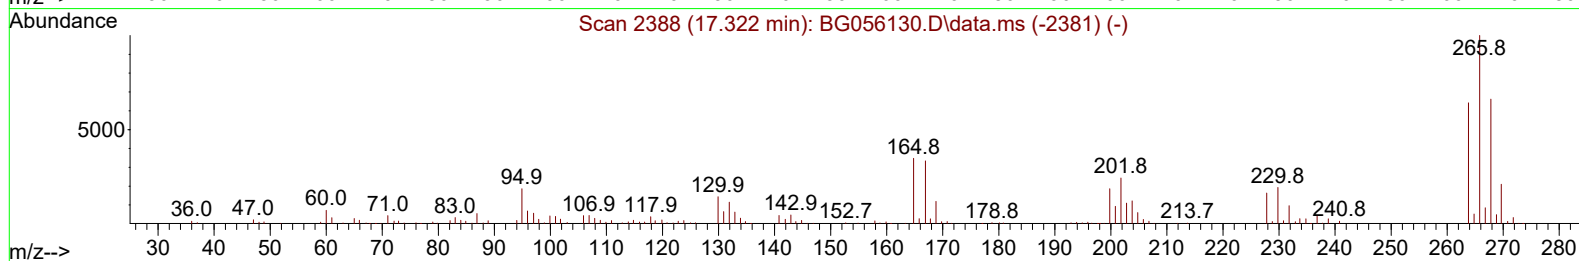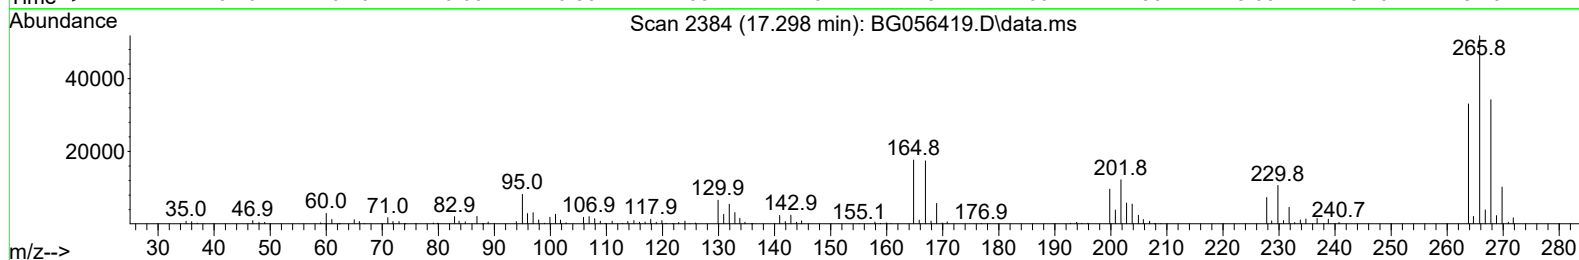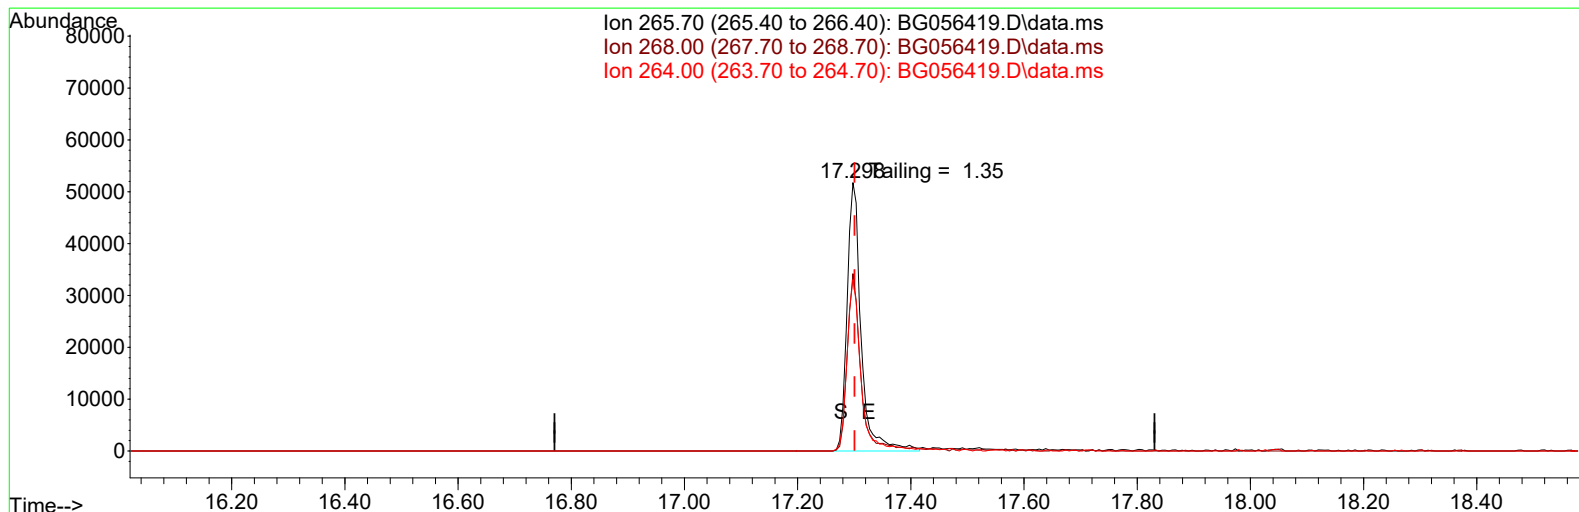

TIC: BG056419.D\data.ms

(70) Pentachlorophenol (C)

17.298min (-0.003) 17365.70 ng




response 88117

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.09
264.00	64.30	68.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012523\
 Data File : BG056419.D
 Acq On : 25 Jan 2023 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jan 26 03:35:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 04:54:56 2023
 Response via : Initial Calibration

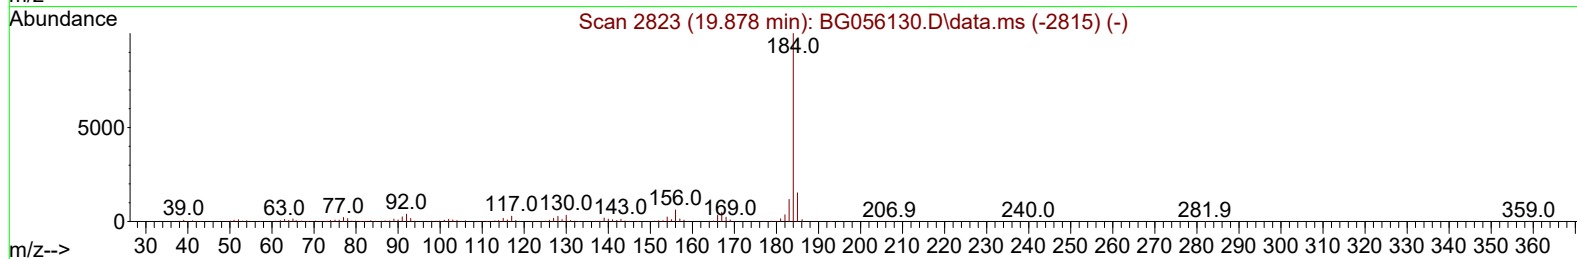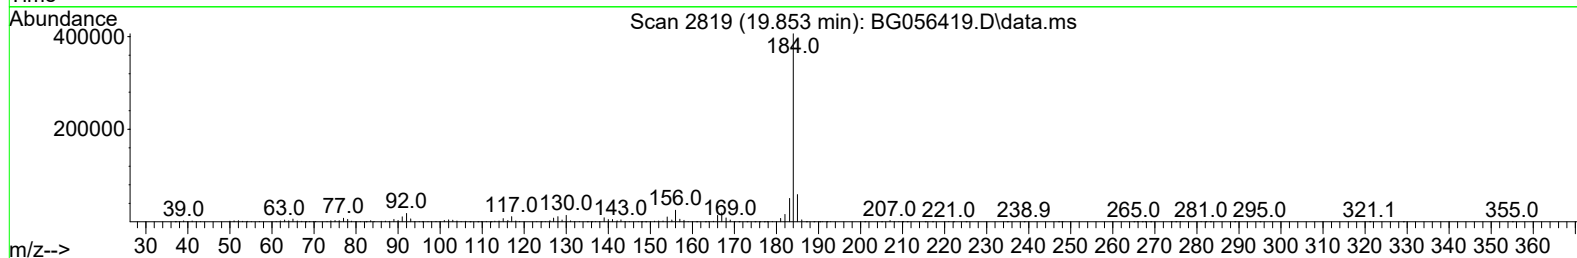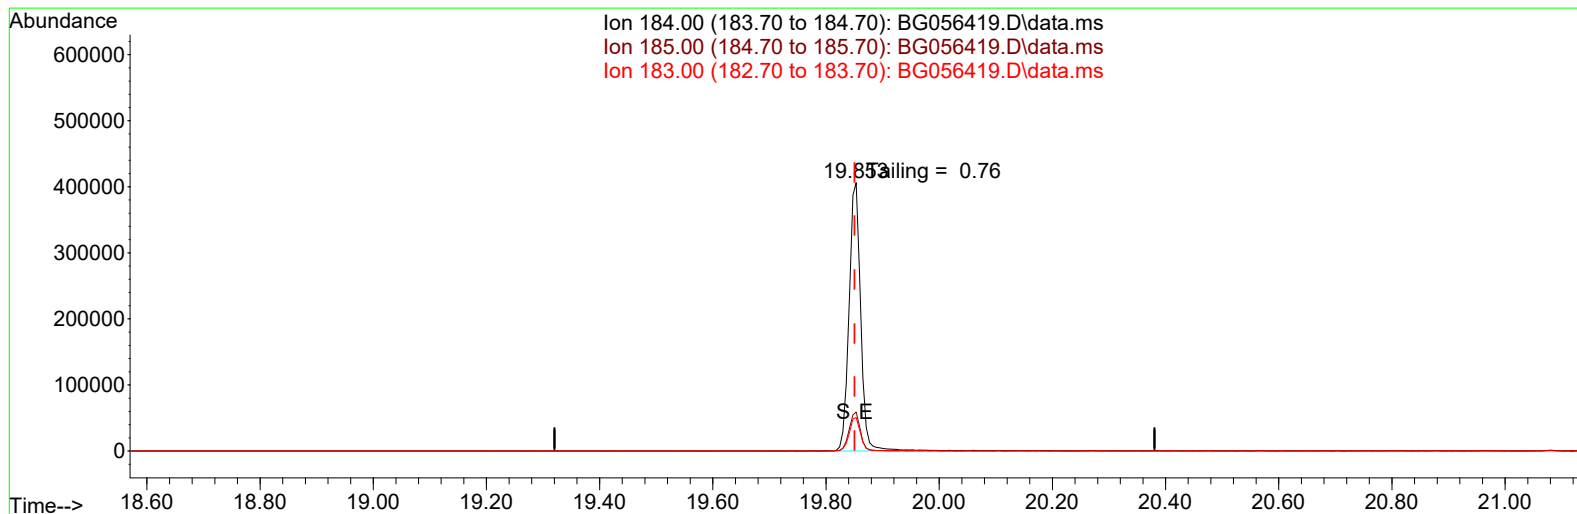

TIC: BG056419.D\data.ms

(77) Benzidine

19.853min (+ 0.003) 239550.16 ng

response 579246

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.48
183.00	11.70	12.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/25/2023	BNA_G	<u>BG056419.D</u>
Compound Name	Response	Retention Time
DDT	261424	21.081
DDD	13885	20.629
DDE	1617	20.124
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15502	276926	5.60

Instrument :
BNA_G
ClientSampleId :
DFTPP