




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052180.D
 Acq On : 27 Jan 2022 11:42
 Operator : CG/JU
 Sample : PB142296BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK296

Manual IntegrationsAPPROVED

Quant Time: Jan 27 23:58:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 26 23:58:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/28/2022
 Supervised By :Yogesh Patel 01/28/2022

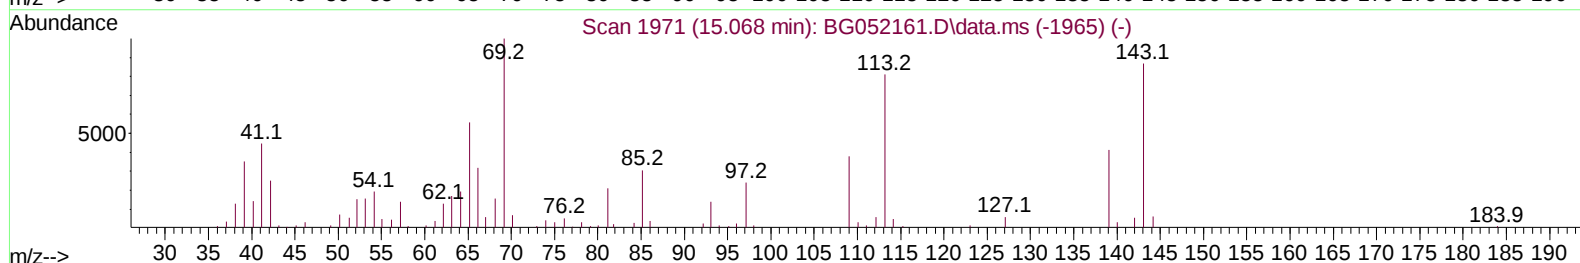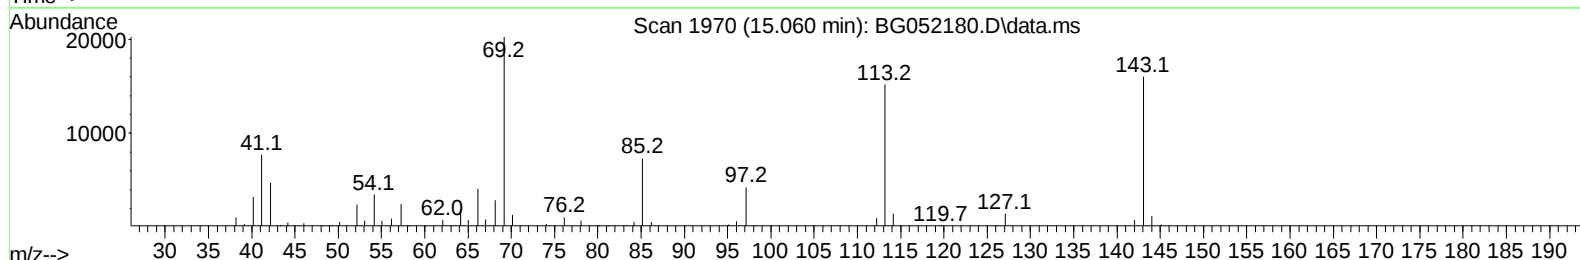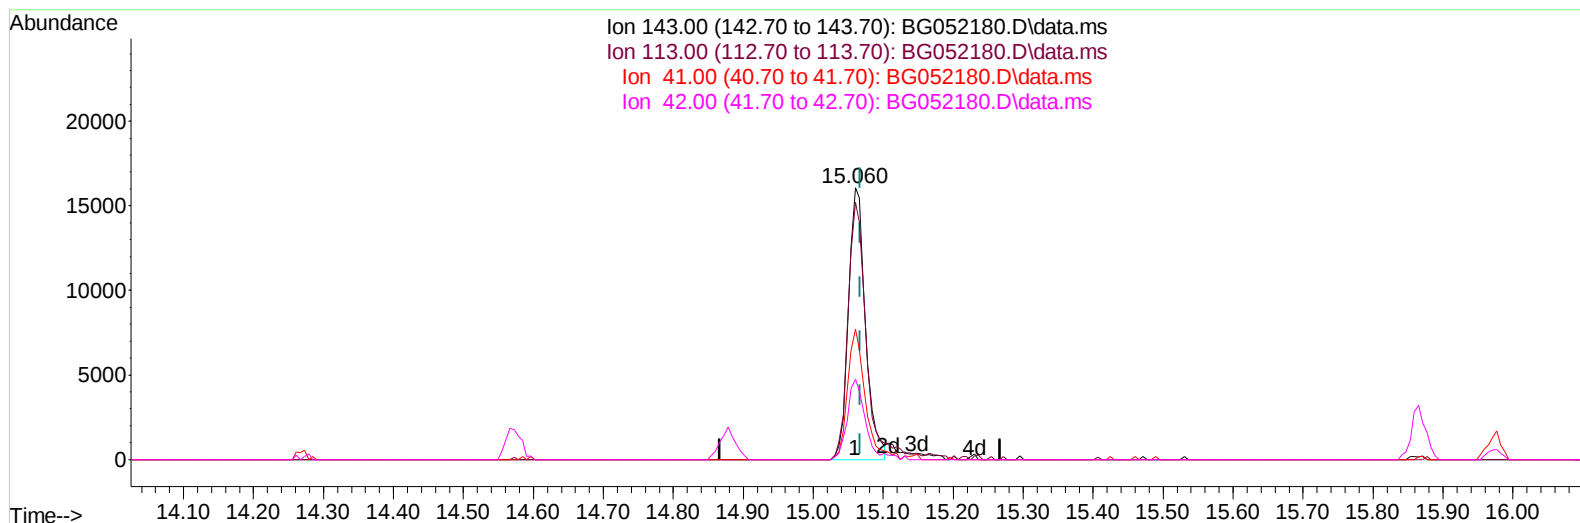

TIC: BG052180.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.060min (-0.007) 23.34 ng/u1

response 26996

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	94.66
41.00	44.40	47.89
42.00	29.70	29.61




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052180.D
Acq On : 27 Jan 2022 11:42
Operator : CG/JU
Sample : PB142296BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK296

Manual IntegrationsAPPROVED

Quant Time: Jan 27 23:58:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 26 23:58:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/28/2022
Supervised By :Yogesh Patel 01/28/2022

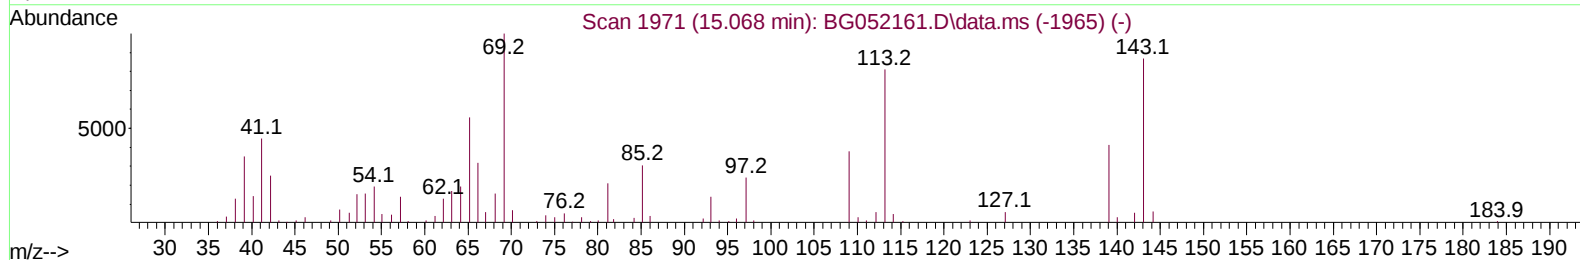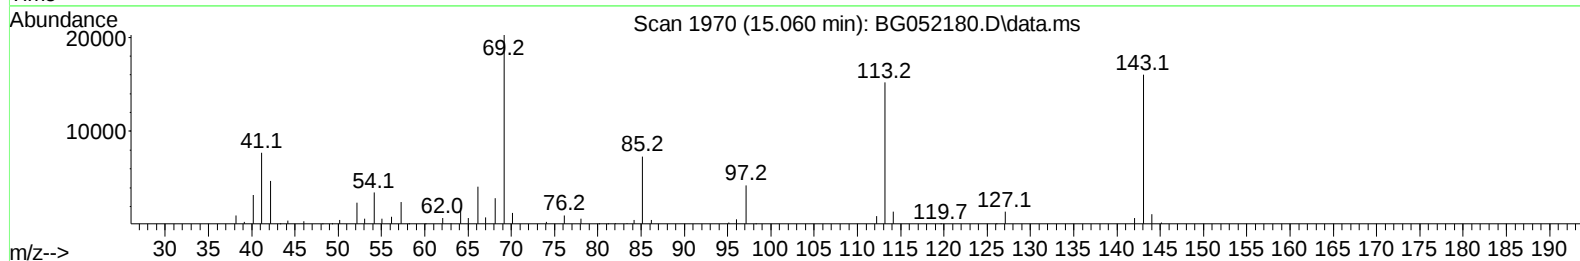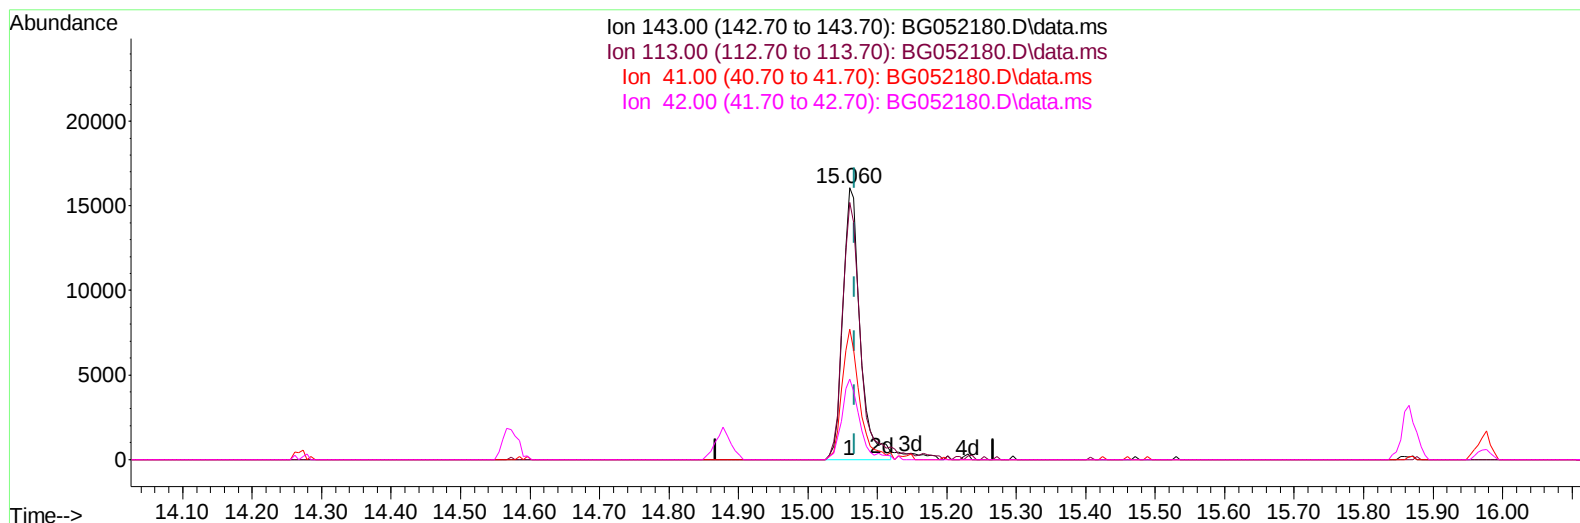

TIC: BG052180.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.060min (-0.007) 24.03 ng/ul m

response 27798

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	94.66
41.00	44.40	47.89
42.00	29.70	29.61

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052180.D
 Acq On : 27 Jan 2022 11:42
 Operator : CG/JU
 Sample : PB142296BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK296

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/28/2022
 Supervised By :Yogesh Patel 01/28/2022

Quant Time: Jan 27 23:58:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 26 23:58:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.240	152	25804	20.000	ng/ul	0.00
20) Naphthalene-d8	11.077	136	109520	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.878	164	83707	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.627	188	213619	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.945	240	219149	20.000	ng/ul	# 0.00
88) Perylene-d12	25.423	264	216563	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.564	96	4008	5.550	ng/uL	0.00
4) Pyridine-d5	3.987	84	55590	24.764	ng/ul	0.00
7) Phenol-d5	7.376	99	66503	26.332	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.541	67	40803	25.451	ng/ul	0.00
11) 2-Chlorophenol-d4	7.764	132	46442	27.775	ng/ul	0.00
15) 4-Methylphenol-d8	8.939	113	52833	26.911	ng/ul	0.00
21) Nitrobenzene-d5	9.409	128	25076	28.976	ng/ul	0.00
24) 2-Nitrophenol-d4	10.137	143	27891	29.141	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.690	165	54087	28.911	ng/ul	0.00
31) 4-Chloroaniline-d4	11.201	131	69769	26.779	ng/ul	0.00
46) Dimethylphthalate-d6	14.267	166	196416	28.388	ng/ul	0.00
49) Acenaphthylene-d8	14.573	160	236444	28.290	ng/ul	0.00
54) 4-Nitrophenol-d4	15.060	143	27798m	24.030	ng/ul	0.00
60) Fluorene-d10	15.865	176	168923	28.002	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.977	200	24121	17.899	ng/ul	0.00
73) Anthracene-d10	17.727	188	298254	29.432	ng/ul	0.00
81) Pyrene-d10	20.000	212	367612	29.147	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.182	264	347877	30.513	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052180.D
Acq On : 27 Jan 2022 11:42
Operator : CG/JU
Sample : PB142296BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK296

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/28/2022
Supervised By :Yogesh Patel 01/28/2022

Quant Time: Jan 27 23:58:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 26 23:58:52 2022
Response via : Initial Calibration

