




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052201.D
 Acq On : 28 Jan 2022 1:30
 Operator : CG/JU
 Sample : N1302-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F31

Manual IntegrationsAPPROVED

Quant Time: Jan 28 02:26:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 26 23:58:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/28/2022
 Supervised By :Yogesh Patel 01/28/2022

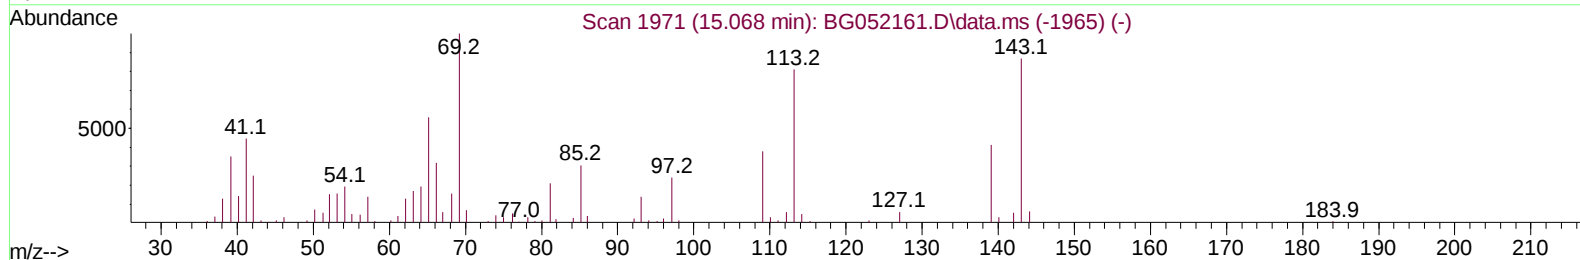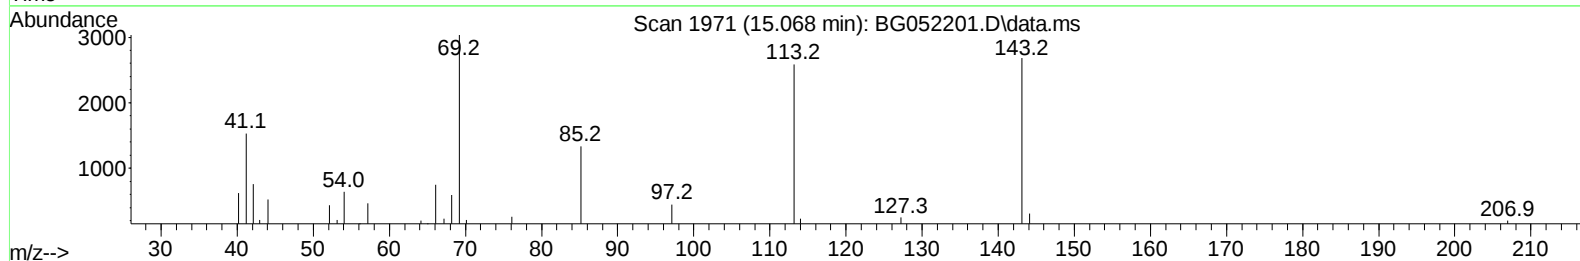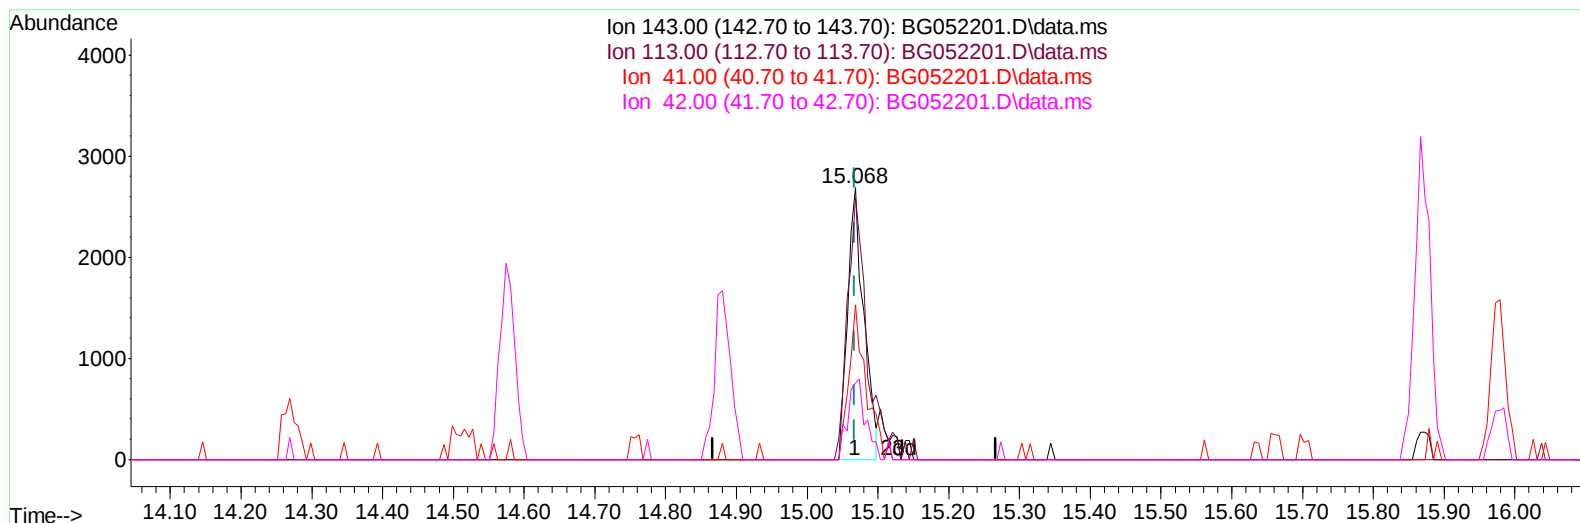

TIC: BG052201.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.068min (+ 0.001) 4.12 ng/u1

response 4278

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	96.35
41.00	44.40	57.04#
42.00	29.70	28.15




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052201.D
 Acq On : 28 Jan 2022 1:30
 Operator : CG/JU
 Sample : N1302-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F31

Manual IntegrationsAPPROVED

Quant Time: Jan 28 02:26:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 26 23:58:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/28/2022
 Supervised By :Yogesh Patel 01/28/2022

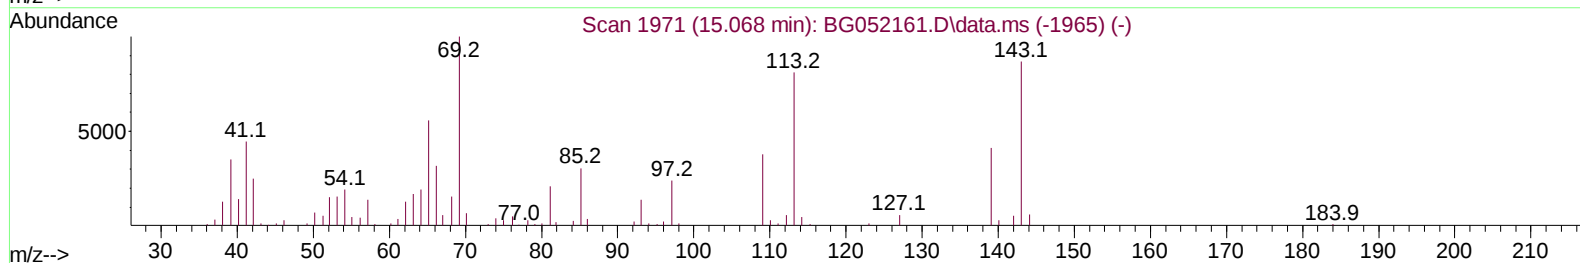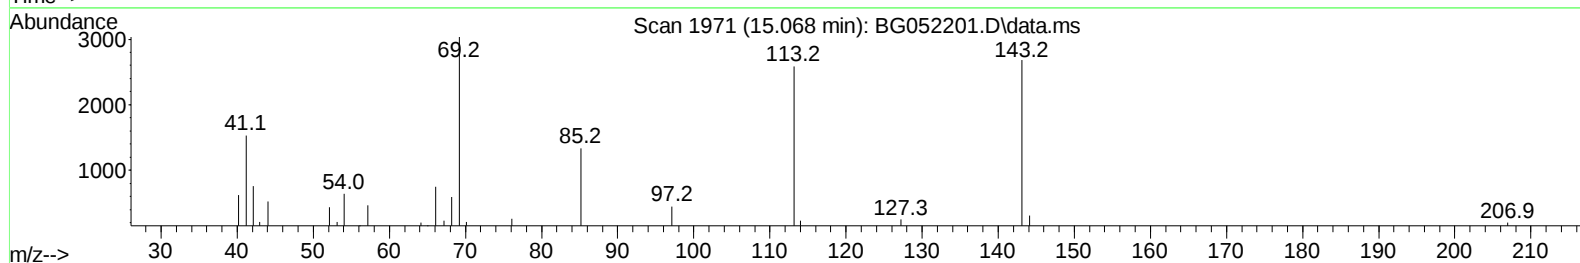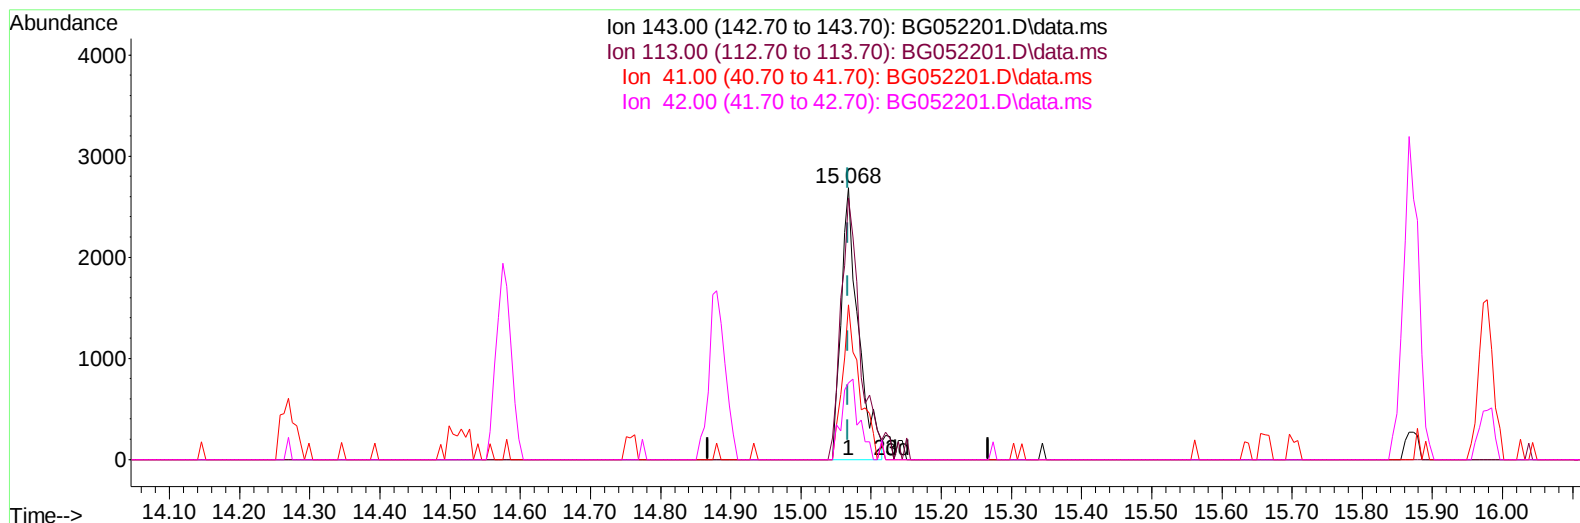

TIC: BG052201.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.068min (+ 0.001) 4.44 ng/ul m

response 4618

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	96.35
41.00	44.40	57.04#
42.00	29.70	28.15

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052201.D
 Acq On : 28 Jan 2022 1:30
 Operator : CG/JU
 Sample : N1302-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F31

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/28/2022
 Supervised By :Yogesh Patel 01/28/2022

Quant Time: Jan 28 02:26:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 26 23:58:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.236	152	23773	20.000	ng/ul	0.00
20) Naphthalene-d8	11.079	136	101238	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.886	164	75205	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.629	188	178471	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.947	240	180978	20.000	ng/ul	# 0.00
88) Perylene-d12	25.430	264	179955	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.572	96	2439	3.666	ng/uL	0.00
4) Pyridine-d5	4.001	84	22451	10.856	ng/ul	0.00
7) Phenol-d5	7.378	99	13278	5.707	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.543	67	43455	29.421	ng/ul	0.00
11) 2-Chlorophenol-d4	7.766	132	36767	23.867	ng/ul	0.00
15) 4-Methylphenol-d8	8.941	113	25493	14.094	ng/ul	0.00
21) Nitrobenzene-d5	9.405	128	27109	33.888	ng/ul	0.00
24) 2-Nitrophenol-d4	10.145	143	29276	33.090	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.692	165	50153	29.001	ng/ul	0.00
31) 4-Chloroaniline-d4	11.203	131	67908	28.197	ng/ul	0.00
46) Dimethylphthalate-d6	14.269	166	201883	32.477	ng/ul	0.00
49) Acenaphthylene-d8	14.575	160	250019	33.296	ng/ul	0.00
54) 4-Nitrophenol-d4	15.068	143	4618m	4.443	ng/ul	0.00
60) Fluorene-d10	15.873	176	183417	33.842	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.979	200	26260	23.324	ng/ul	0.00
73) Anthracene-d10	17.729	188	319616	37.752	ng/ul	0.00
81) Pyrene-d10	20.008	212	381264	36.605	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.190	264	363614	38.382	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052201.D
Acq On : 28 Jan 2022 1:30
Operator : CG/JU
Sample : N1302-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F31

Manual IntegrationsAPPROVED

Quant Time: Jan 28 02:26:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 26 23:58:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/28/2022
Supervised By :Yogesh Patel 01/28/2022

