

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052150.D
 Acq On : 26 Jan 2022 15:40
 Operator : CG/JU
 Sample : N1230-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q53

Quant Time: Jan 27 00:00:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 26 23:58:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.240	152	23203	20.000	ng/u1	0.00
20) Naphthalene-d8	11.078	136	102684	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.884	164	75575	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.628	188	192290	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.945	240	199251	20.000	ng/u1	# 0.00
88) Perylene-d12	25.429	264	199919	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.564	96	2823	4.347	ng/uL	0.00
4) Pyridine-d5	3.999	84	10100	5.004	ng/u1	0.00
7) Phenol-d5	7.383	99	19191	8.451	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.541	67	47229	32.761	ng/u1	0.00
11) 2-Chlorophenol-d4	7.764	132	42584	28.322	ng/u1	0.00
15) 4-Methylphenol-d8	8.945	113	33200	18.806	ng/u1	0.00
21) Nitrobenzene-d5	9.409	128	28577	35.220	ng/u1	0.00
24) 2-Nitrophenol-d4	10.144	143	30629	34.132	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.690	165	56696	32.323	ng/u1	0.00
31) 4-Chloroaniline-d4	11.201	131	51155	20.942	ng/u1	0.00
46) Dimethylphthalate-d6	14.273	166	231335	37.032	ng/u1	0.00
49) Acenaphthylene-d8	14.579	160	267093	35.396	ng/u1	0.00
54) 4-Nitrophenol-d4	15.066	143	9237	8.844	ng/u1	0.00
60) Fluorene-d10	15.871	176	201655	37.025	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.977	200	36649	30.212	ng/u1	0.00
73) Anthracene-d10	17.727	188	361853	39.669	ng/u1	0.00
81) Pyrene-d10	20.007	212	454251	39.613	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.188	264	433992	41.236	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	9.069	105	3590	1.288	ng/u1	99
59) Diethylphthalate	15.671	149	13225	2.081	ng/u1#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052150.D
Acq On : 26 Jan 2022 15:40
Operator : CG/JU
Sample : N1230-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q53

Quant Time: Jan 27 00:00:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 26 23:58:52 2022
Response via : Initial Calibration




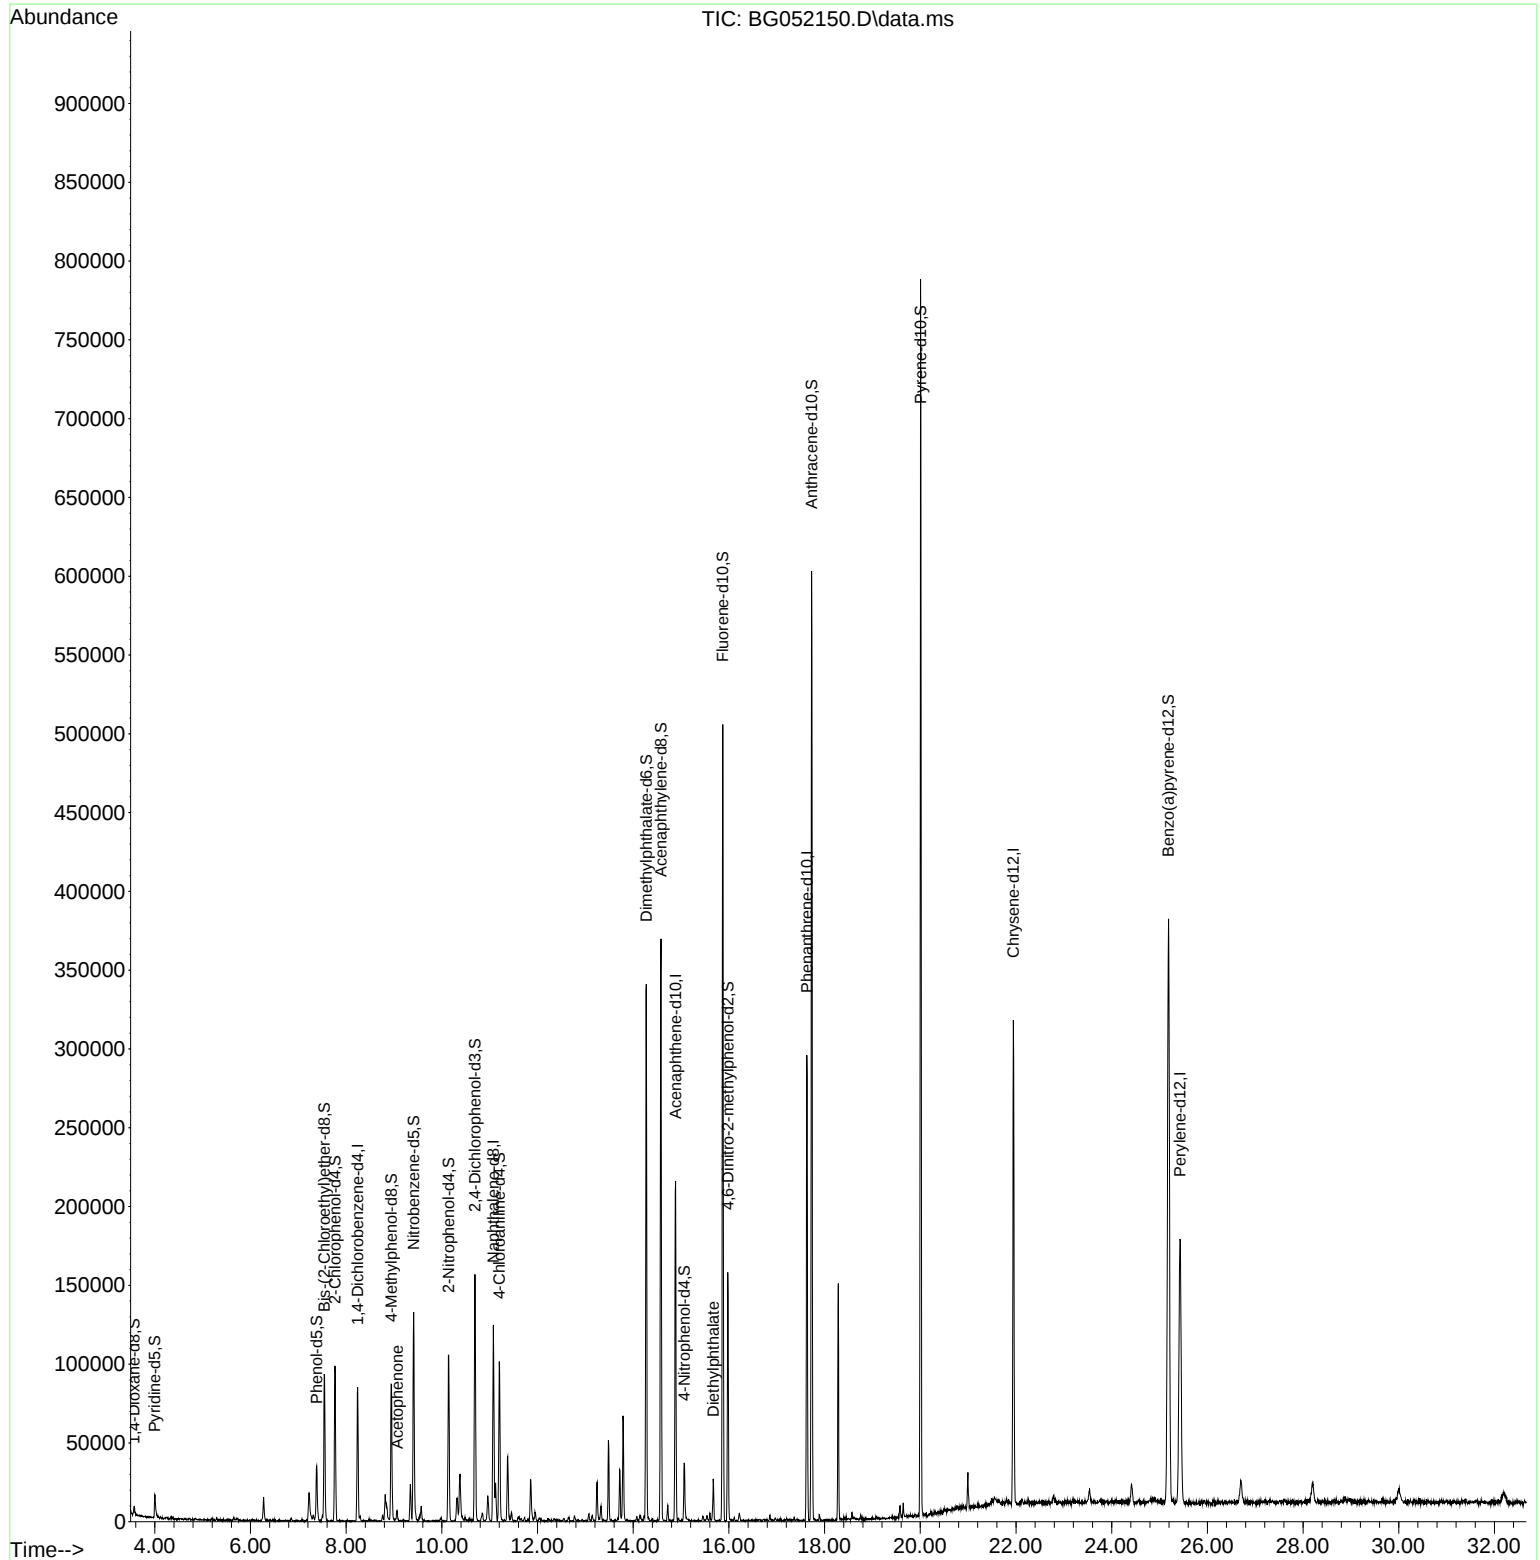


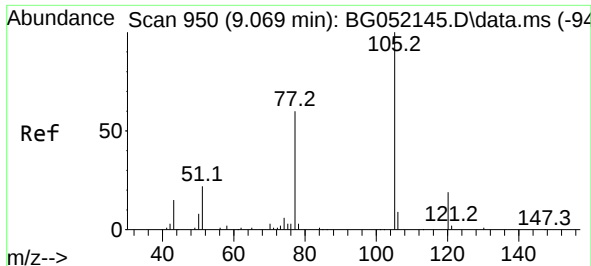

#16
Acetophenone
Concen: 1.288 ng/ul
RT: 9.069 min Scan# 91
Delta R.T. -0.001 min
Lab File: BG052150.D
Acq: 26 Jan 2022 15:40

Instrument :
BNA_G
ClientSampleId :
C0Q53

Tgt Ion:105 Resp: 3590
Ion Ratio Lower Upper
105 100
77 85.0 67.3 100.9
51 31.3 24.0 36.0

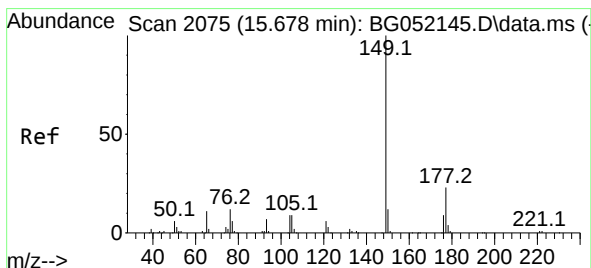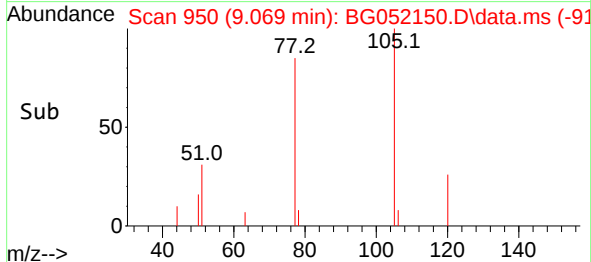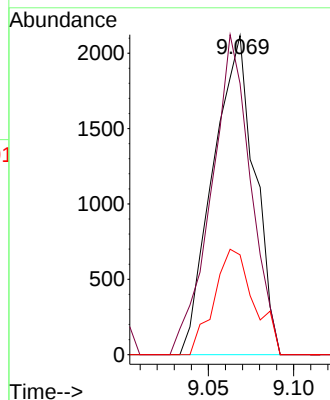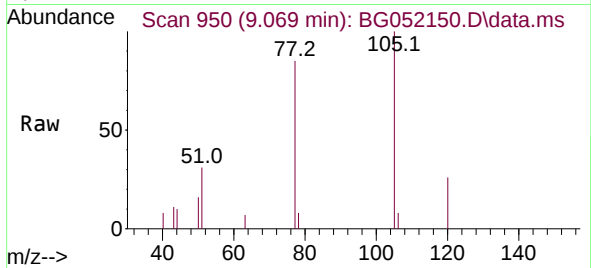

#59
Diethylphthalate
Concen: 2.081 ng/ul
RT: 15.671 min Scan# 2074
Delta R.T. -0.007 min
Lab File: BG052150.D
Acq: 26 Jan 2022 15:40

Tgt Ion:149 Resp: 13225
Ion Ratio Lower Upper
149 100
177 26.4 16.8 25.2#
150 13.2 10.1 15.1

