

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052200.D
 Acq On : 28 Jan 2022 00:52
 Operator : CG/JU
 Sample : N1273-10
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HK9

Quant Time: Jan 28 01:33:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 26 23:58:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.240	152	23679	20.000	ng/u1	0.00
20) Naphthalene-d8	11.077	136	101122	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.884	164	75117	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.627	188	176498	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.945	240	181610	20.000	ng/u1	# 0.00
88) Perylene-d12	25.428	264	180024	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.540	96	12018	18.136	ng/uL	-0.03
4) Pyridine-d5	3.998	84	12288	5.965	ng/u1	0.00
7) Phenol-d5	7.382	99	17133	7.393	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.541	67	47716	32.434	ng/u1	0.00
11) 2-Chlorophenol-d4	7.764	132	43733	28.502	ng/u1	0.00
15) 4-Methylphenol-d8	8.945	113	30761	17.075	ng/u1	0.00
21) Nitrobenzene-d5	9.409	128	30832	38.586	ng/u1	0.00
24) 2-Nitrophenol-d4	10.143	143	31955	36.160	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.689	165	56901	32.941	ng/u1	0.00
31) 4-Chloroaniline-d4	11.200	131	51236	21.299	ng/u1	0.00
46) Dimethylphthalate-d6	14.273	166	225770	36.362	ng/u1	0.00
49) Acenaphthylene-d8	14.578	160	270397	36.052	ng/u1	0.00
54) 4-Nitrophenol-d4	15.072	143	7063	6.804	ng/u1	0.00
60) Fluorene-d10	15.871	176	201576	37.236	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.976	200	33081	29.711	ng/u1	0.00
73) Anthracene-d10	17.727	188	345979	41.322	ng/u1	0.00
81) Pyrene-d10	20.006	212	420963	40.276	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.187	264	398267	42.023	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.605	88	22035	28.819	ng/uL#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052200.D
Acq On : 28 Jan 2022 00:52
Operator : CG/JU
Sample : N1273-10
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HK9


Quant Time: Jan 28 01:33:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 26 23:58:52 2022
Response via : Initial Calibration

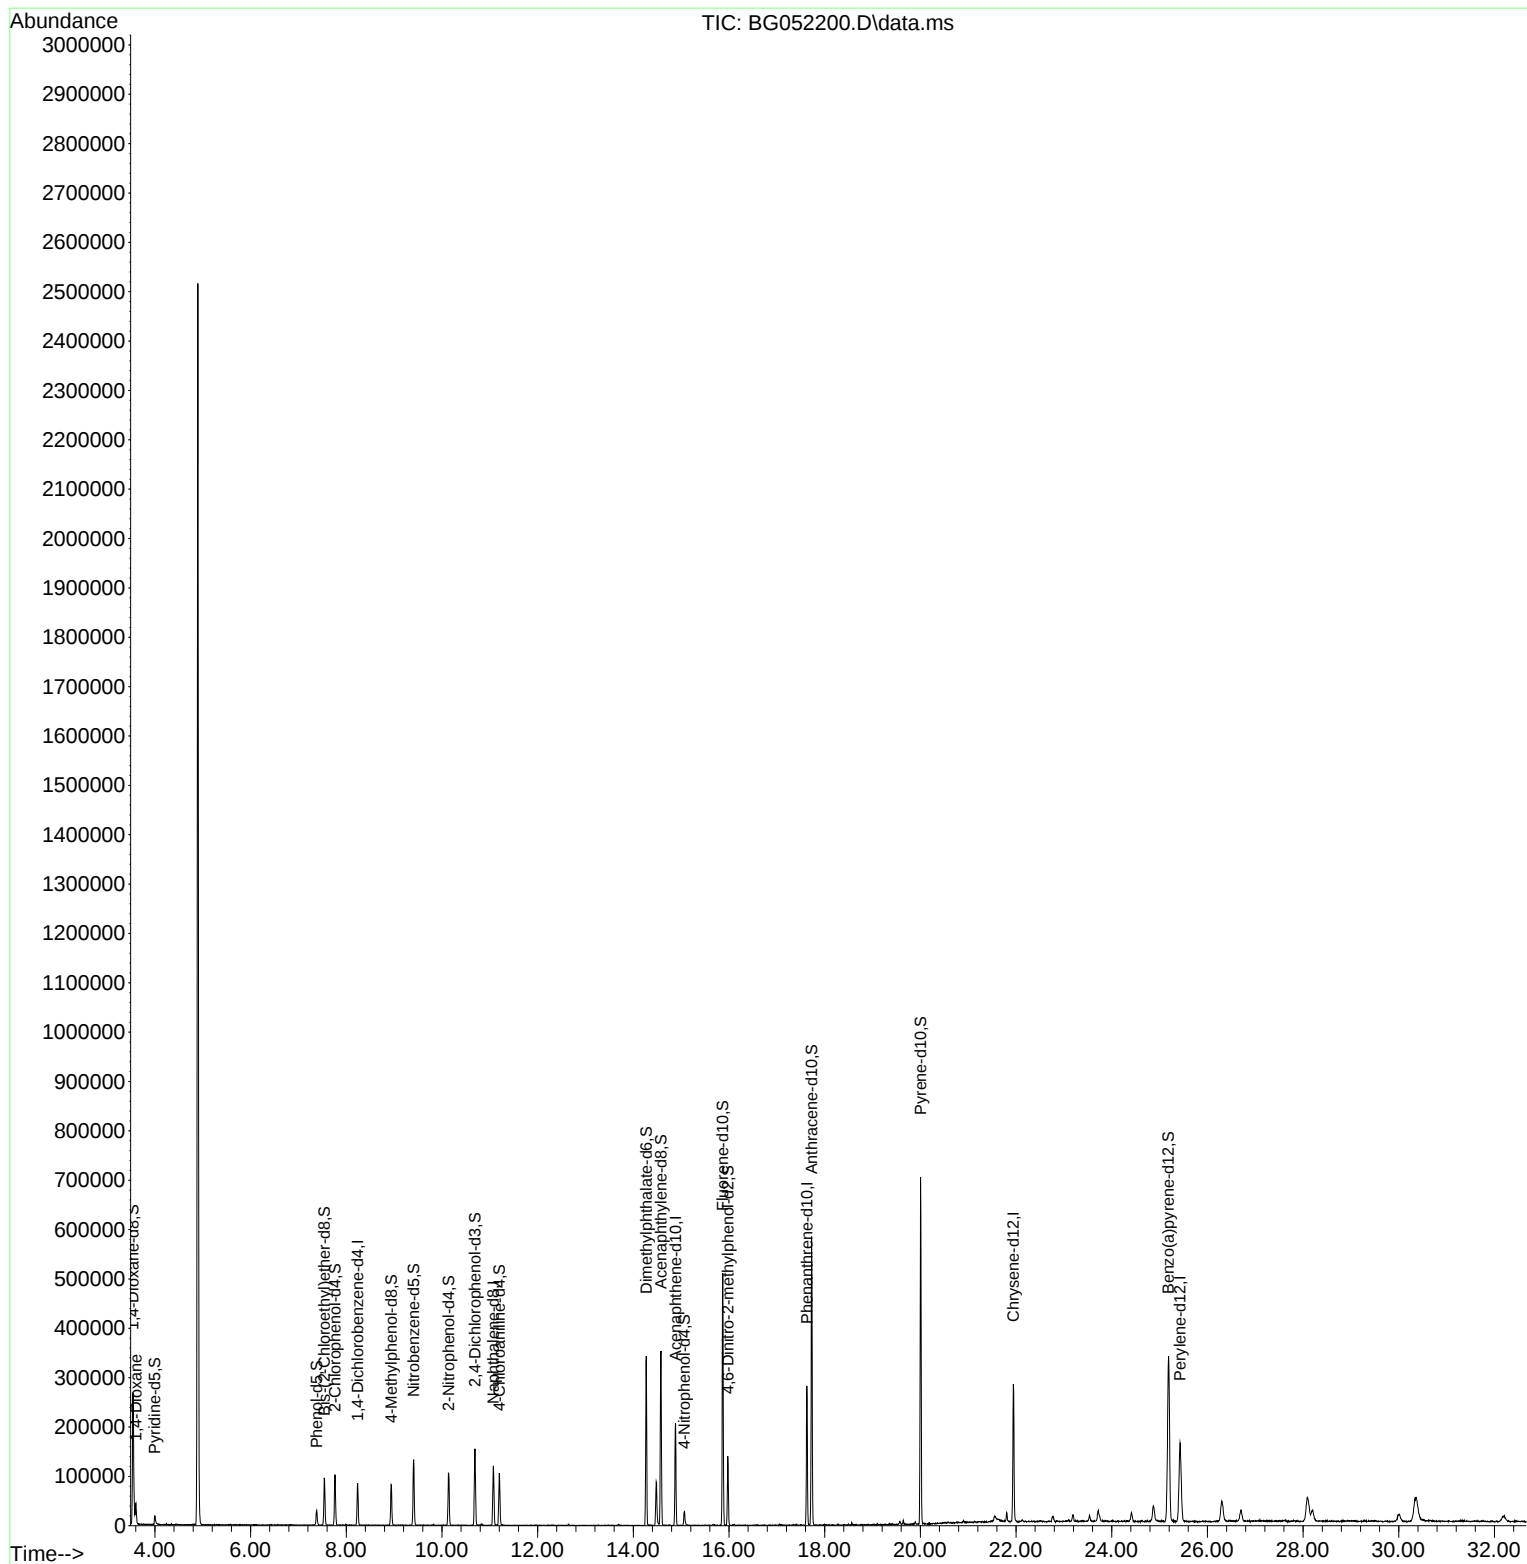

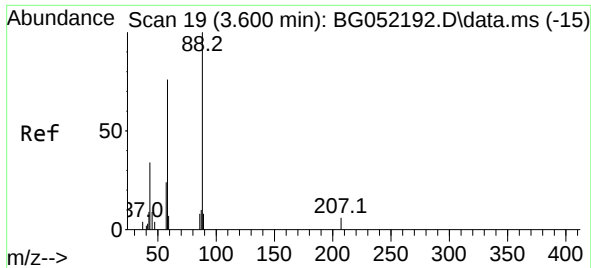

#2
 1,4-Dioxane
 Concen: 28.819 ng/uL
 RT: 3.605 min Scan# 20
 Delta R.T. -0.001 min
 Lab File: BG052200.D
 Acq: 28 Jan 2022 00:52

Instrument :
 BNA_G
 ClientSampleId :
 C0HK9

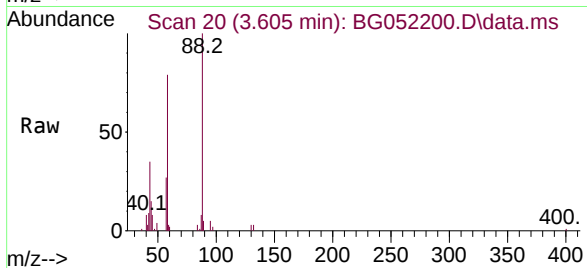

Tgt Ion: 88 Resp: 22035
 Ion Ratio Lower Upper
 88 100
 43 34.7 23.0 34.4#
 58 79.4 62.4 93.6

