

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052152.D
 Acq On : 26 Jan 2022 16:55
 Operator : CG/JU
 Sample : N1230-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.565	9	13	19	rVB2	5408	9251	0.89%	0.104%
2	3.999	83	87	95	rBV	31178	51670	4.96%	0.583%
3	4.352	142	147	149	rBV4	1735	3000	0.29%	0.034%
4	5.286	303	306	312	rVB3	1485	2661	0.26%	0.030%
5	7.383	657	663	673	rVB	27651	49441	4.75%	0.557%
6	7.542	683	690	698	rBV	89723	152041	14.61%	1.714%
7	7.765	720	728	735	rBV	91675	160882	15.46%	1.814%
8	8.241	802	809	816	rBV	84599	146458	14.07%	1.651%
9	8.940	921	928	936	rBV2	75493	129185	12.41%	1.456%
10	9.410	998	1008	1020	rBV	120377	219278	21.07%	2.472%
11	9.527	1024	1028	1035	rBV2	7338	12834	1.23%	0.145%
12	10.138	1125	1132	1140	rBV	101334	178604	17.16%	2.014%
13	10.690	1219	1226	1239	rVB	137129	242097	23.26%	2.729%
14	11.078	1285	1292	1301	rVB	117858	210891	20.26%	2.378%
15	11.201	1306	1313	1325	rVB	134126	242030	23.25%	2.729%
16	12.652	1554	1560	1564	rBV2	2433	3946	0.38%	0.044%
17	12.770	1576	1580	1585	rBV	1427	2565	0.25%	0.029%
18	13.692	1734	1737	1741	rVB3	3026	3661	0.35%	0.041%
19	14.274	1829	1836	1842	rBV	310765	449451	43.18%	5.067%
20	14.579	1881	1888	1895	rVV	331474	521186	50.07%	5.876%
21	14.761	1914	1919	1926	rVB4	1908	2992	0.29%	0.034%
22	14.885	1932	1940	1947	rBV	200715	317606	30.51%	3.581%
23	15.067	1965	1971	1984	rBV2	25319	48530	4.66%	0.547%
24	15.701	2076	2079	2083	rVB3	2295	2711	0.26%	0.031%
25	15.872	2101	2108	2114	rBV	452758	678153	65.15%	7.646%
26	15.977	2120	2126	2135	rBV	148647	211767	20.34%	2.388%
27	16.112	2143	2149	2152	rBV2	2215	3181	0.31%	0.036%
28	16.565	2223	2226	2229	rVV2	1582	2231	0.21%	0.025%
29	17.352	2358	2360	2365	rBV3	1801	2426	0.23%	0.027%
30	17.516	2383	2388	2390	rBV2	1927	2544	0.24%	0.029%
31	17.628	2401	2407	2413	rBV	288789	427360	41.06%	4.818%
32	17.728	2416	2424	2436	rVV2	552904	819939	78.77%	9.244%
33	17.881	2448	2450	2454	rBV4	1370	2029	0.19%	0.023%
34	18.268	2513	2516	2517	rBV3	2362	2317	0.22%	0.026%
35	18.492	2551	2554	2558	rBV3	3581	4588	0.44%	0.052%
36	18.574	2562	2568	2570	rBV4	2090	3189	0.31%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052152.D
 Acq On : 26 Jan 2022 16:55
 Operator : CG/JU
 Sample : N1230-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	19.009	2639	2642	2645	rBV4	2398	3596	0.35%	0.041%
38	19.349	2698	2700	2707	rVB5	3423	4227	0.41%	0.048%
39	19.414	2707	2711	2712	rBV3	1960	2899	0.28%	0.033%
40	19.473	2719	2721	2725	rBV4	1912	2912	0.28%	0.033%
41	19.572	2733	2738	2742	rBV5	8021	11717	1.13%	0.132%
42	19.643	2745	2750	2756	rVV3	7602	11755	1.13%	0.133%
43	19.884	2789	2791	2793	rVV3	3491	3192	0.31%	0.036%
44	19.901	2793	2794	2797	rVV3	3114	2167	0.21%	0.024%
45	20.007	2805	2812	2820	rVV	751125	1040898	100.00%	11.735%
46	20.207	2845	2846	2850	rBV4	2434	2486	0.24%	0.028%
47	20.330	2865	2867	2871	rVB4	3232	4453	0.43%	0.050%
48	20.371	2871	2874	2875	rBV3	2781	3014	0.29%	0.034%
49	20.430	2882	2884	2887	rVB3	3335	2655	0.26%	0.030%
50	20.477	2887	2892	2895	rBV5	3805	7621	0.73%	0.086%
51	20.577	2905	2909	2910	rBV3	3652	4670	0.45%	0.053%
52	20.941	2969	2971	2973	rBV3	2320	2108	0.20%	0.024%
53	21.388	3044	3047	3050	rBV5	3456	4831	0.46%	0.054%
54	21.499	3064	3066	3068	rBV3	2860	1906	0.18%	0.021%
55	21.546	3068	3074	3083	rBV8	25608	64028	6.15%	0.722%
56	21.799	3114	3117	3118	rBV3	3338	3636	0.35%	0.041%
57	21.946	3135	3142	3149	rVB	289334	495483	47.60%	5.586%
58	22.051	3158	3160	3162	rBV3	3082	2667	0.26%	0.030%
59	22.498	3235	3236	3238	rBV2	3319	2649	0.25%	0.030%
60	22.751	3277	3279	3282	rBV5	2825	3143	0.30%	0.035%
61	22.786	3282	3285	3286	rBV2	4791	4716	0.45%	0.053%
62	22.997	3319	3321	3325	rBV4	2414	3169	0.30%	0.036%
63	23.514	3401	3409	3413	rBV9	9076	27983	2.69%	0.315%
64	23.743	3440	3448	3455	rVB2	78173	159287	15.30%	1.796%
65	24.184	3521	3523	3526	rBV4	2475	3227	0.31%	0.036%
66	24.413	3555	3562	3568	rBV10	9741	20438	1.96%	0.230%
67	24.671	3604	3606	3607	rVB2	3513	1877	0.18%	0.021%
68	24.854	3635	3637	3639	rBV3	4761	4322	0.42%	0.049%
69	25.188	3681	3694	3707	rBV2	351374	1021490	98.14%	11.517%
70	25.347	3719	3721	3723	rVB2	2833	2254	0.22%	0.025%
71	25.423	3723	3734	3747	rBV2	168132	529520	50.87%	5.970%
72	25.723	3783	3785	3787	rBV3	2038	1998	0.19%	0.023%
73	25.776	3792	3794	3797	rBV4	2366	2319	0.22%	0.026%
74	25.799	3797	3798	3801	rVB3	2924	2234	0.21%	0.025%
75	27.233	4041	4042	4044	rBV2	2250	1885	0.18%	0.021%
76	27.286	4049	4051	4052	rBV2	3212	2125	0.20%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052152.D
 Acq On : 26 Jan 2022 16:55
 Operator : CG/JU
 Sample : N1230-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	27.626	4107	4109	4111	rBV3	2622	2407	0.23%	0.027%
78	27.673	4114	4117	4119	rBV4	3204	4125	0.40%	0.047%
79	28.032	4174	4178	4179	rBV4	2637	3710	0.36%	0.042%
80	28.331	4227	4229	4234	rBV5	2265	3322	0.32%	0.037%
81	28.590	4271	4273	4275	rBV2	2596	2626	0.25%	0.030%
82	28.907	4325	4327	4329	rVB3	2943	2143	0.21%	0.024%
83	28.930	4329	4331	4333	rBV3	2381	1902	0.18%	0.021%
84	29.218	4378	4380	4385	rBV5	2171	3358	0.32%	0.038%
85	29.259	4385	4387	4389	rBV3	2888	2033	0.20%	0.023%
86	29.377	4404	4407	4409	rBV4	3750	3780	0.36%	0.043%
87	29.412	4411	4413	4415	rBV3	3003	3245	0.31%	0.037%
88	29.430	4415	4416	4419	rBV3	3511	3186	0.31%	0.036%
89	29.847	4485	4487	4490	rVB4	2838	2488	0.24%	0.028%
90	29.929	4499	4501	4502	rBV2	3067	2389	0.23%	0.027%
91	30.475	4592	4594	4596	rVB3	3058	2636	0.25%	0.030%
92	31.086	4696	4698	4699	rVB2	3141	2112	0.20%	0.024%
93	31.104	4699	4701	4704	rBV4	4362	5548	0.53%	0.063%
94	31.145	4706	4708	4709	rVB2	2655	1888	0.18%	0.021%
95	31.409	4751	4753	4756	rBV3	3119	3670	0.35%	0.041%
96	31.691	4799	4801	4807	rBV6	2435	3299	0.32%	0.037%
97	31.815	4820	4822	4823	rBV2	3382	3188	0.31%	0.036%
98	32.026	4857	4858	4860	rBV2	3869	2135	0.21%	0.024%
99	32.114	4871	4873	4874	rBV2	3054	1899	0.18%	0.021%
100	32.308	4904	4906	4908	rBV3	2205	2334	0.22%	0.026%




Sum of corrected areas: 8869675

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052152.D
Acq On : 26 Jan 2022 16:55
Operator : CG/JU
Sample : N1230-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

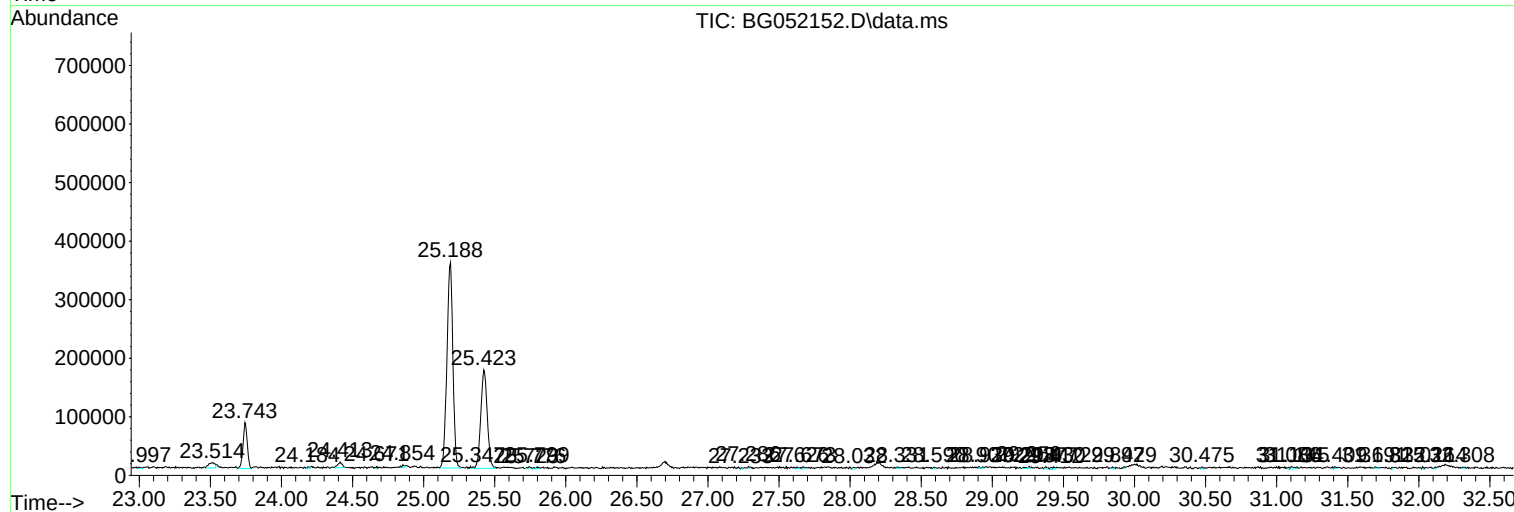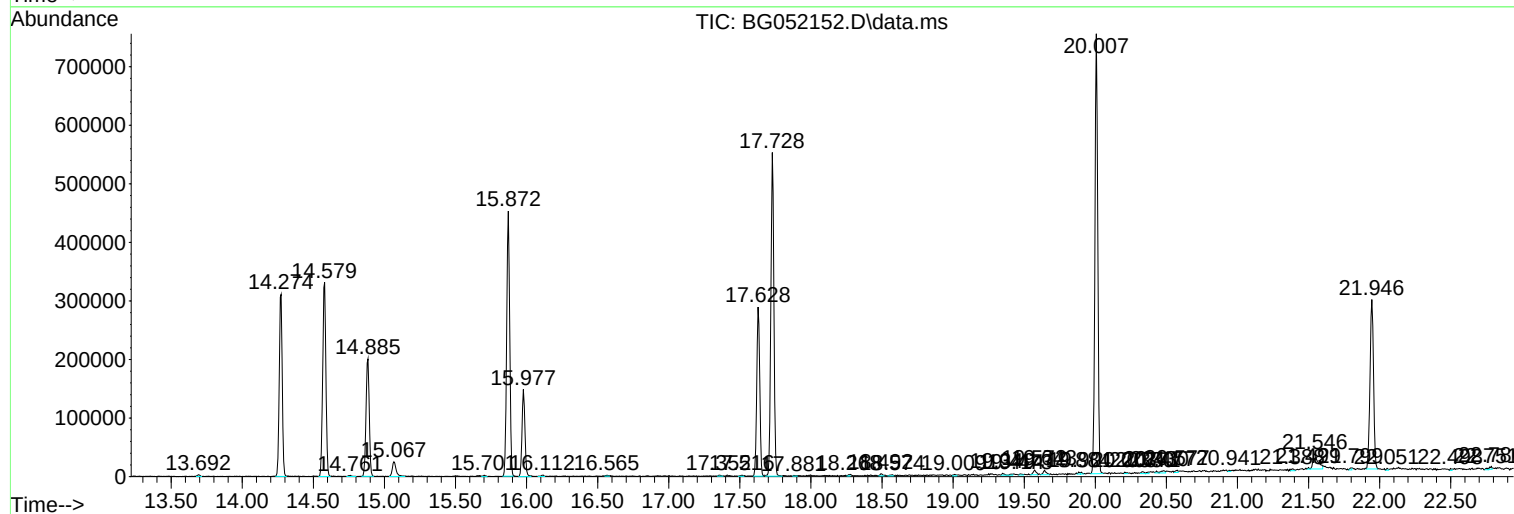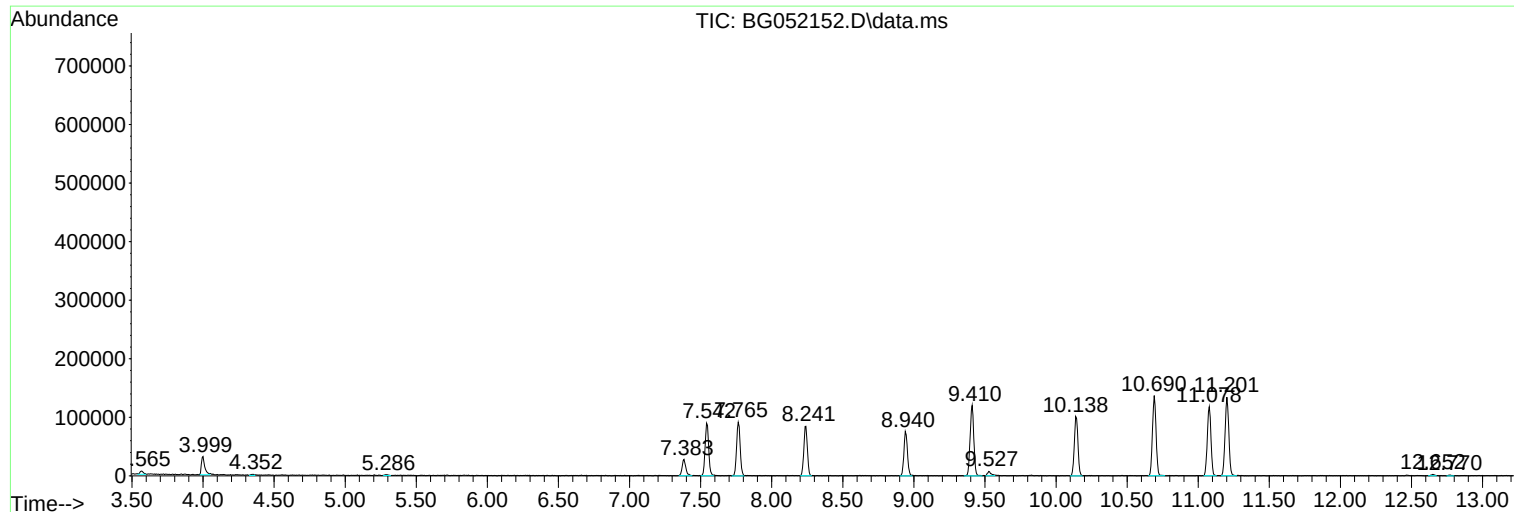

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052152.D
Acq On : 26 Jan 2022 16:55
Operator : CG/JU
Sample : N1230-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q03










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2- Chloropropionic acid, oc... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.546	2.58 ng/ul	64028	Chrysene-d12	21.946

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-	Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	90	
2	Dichloroacetic acid, tridecyl ester	310	C15H28Cl2O2	1000280-48-3	87		
3	Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	86		
4	Pentadecafluorooctanoic acid, tr...	596	C21H27F15O2	1000406-04-3	83		
5	n-Pentadecanol	228	C15H32O	000629-76-5	76		

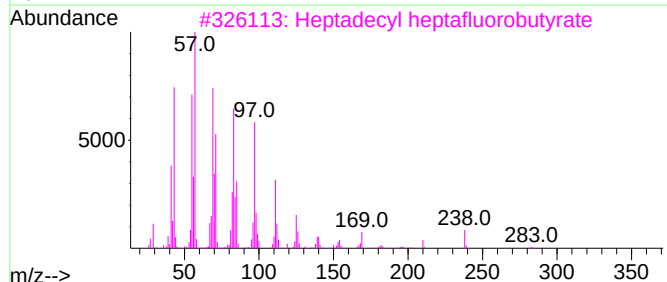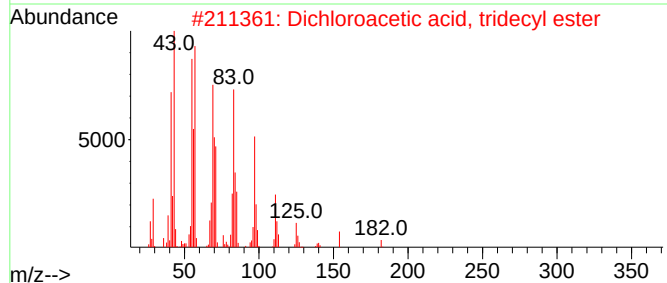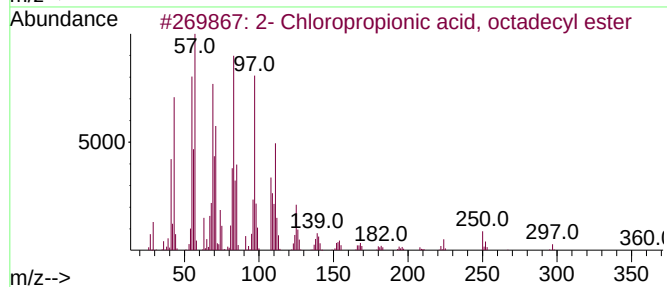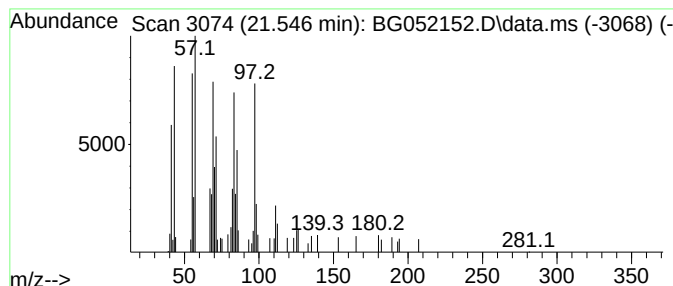

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052152.D
Acq On : 26 Jan 2022 16:55
Operator : CG/JU
Sample : N1230-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q03










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 7,11-Dimethyldodeca-2,6,10-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
23.743	6.02 ng/ul	159287	Perylene-d12	25.423

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,11-Dimethyldodeca-2,6,10-trien...	208	C14H24O	125529-10-4	83		
2	4,8,12-Tetradecatrienal, 5,9,13-...	248	C17H28O	066408-55-7	72		
3	2,3,5-Trimethyl-2,3,5-hexanetric...	203	C12H17N3	003974-79-6	72		
4	3,7,11-Trimethyl-2,6,10-dodecatr...	217	C15H23N	029789-67-1	64		
5	Trideca-1,3,7,11-tetraene-1,1-di...	268	C18H24N2	1000159-88-9	59		

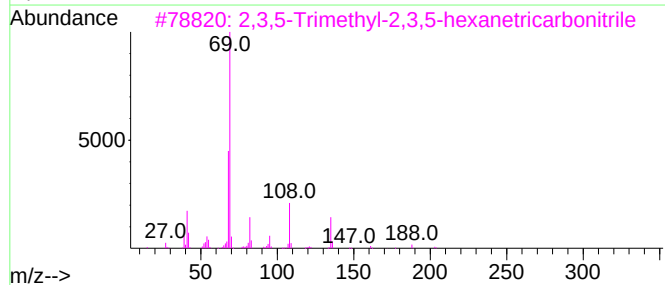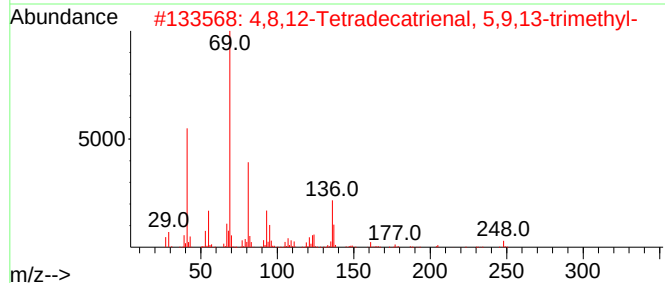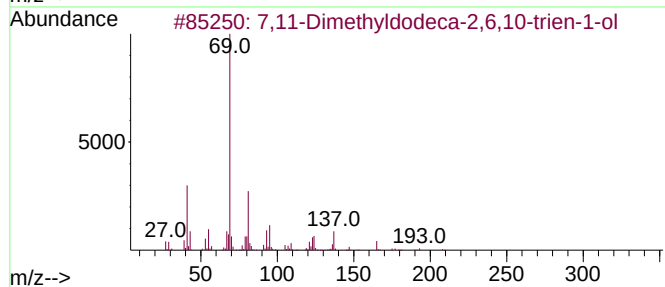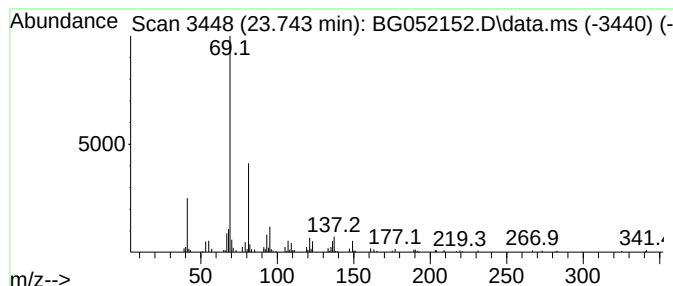

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052152.D
Acq On : 26 Jan 2022 16:55
Operator : CG/JU
Sample : N1230-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2- Chloropropio...	21.546	2.6	ng/ul	64028	5	21.946	495483	20.0
7,11-Dimethyldo...	23.743	6.0	ng/ul	159287	6	25.423	529520	20.0