

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052155.D
 Acq On : 26 Jan 2022 18:48
 Operator : CG/JU
 Sample : N1230-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.567	9	13	21	rVB2	5584	8462	0.82%	0.094%
2	4.002	83	87	97	rBV	19300	33275	3.22%	0.370%
3	4.108	101	105	107	rBV3	1481	1709	0.17%	0.019%
4	4.343	135	145	151	rBV3	2247	4993	0.48%	0.056%
5	4.595	186	188	193	rVV4	1431	1567	0.15%	0.017%
6	4.666	195	200	206	rBV3	2360	4148	0.40%	0.046%
7	7.380	652	662	671	rBV2	31489	57771	5.60%	0.643%
8	7.544	683	690	698	rVB	91465	153552	14.88%	1.709%
9	7.762	720	727	735	rVB	96339	169106	16.38%	1.883%
10	7.838	735	740	743	rBV	816	1372	0.13%	0.015%
11	8.238	799	808	815	rBV	92576	155847	15.10%	1.735%
12	8.942	921	928	935	rBV	86962	151081	14.64%	1.682%
13	9.407	1000	1007	1015	rBV	127396	225173	21.82%	2.507%
14	9.530	1023	1028	1034	rBV4	5741	12490	1.21%	0.139%
15	9.830	1074	1079	1081	rVB	2023	2633	0.26%	0.029%
16	10.141	1125	1132	1139	rBV	103161	190096	18.42%	2.116%
17	10.687	1217	1225	1233	rBV	151760	278825	27.01%	3.104%
18	10.822	1244	1248	1256	rBV3	4999	8703	0.84%	0.097%
19	11.075	1284	1291	1299	rBV	132369	227860	22.08%	2.537%
20	11.198	1303	1312	1322	rBV	127907	236463	22.91%	2.632%
21	11.850	1419	1423	1426	rVB	1400	1815	0.18%	0.020%
22	12.649	1550	1559	1563	rBV3	2560	5038	0.49%	0.056%
23	13.601	1718	1721	1726	rVB2	910	1333	0.13%	0.015%
24	13.695	1734	1737	1741	rVB3	1563	1911	0.19%	0.021%
25	14.271	1828	1835	1841	rBV	362491	510673	49.48%	5.685%
26	14.576	1880	1887	1895	rBV	378021	585043	56.68%	6.513%
27	14.811	1923	1927	1929	rBV2	1145	1453	0.14%	0.016%
28	14.881	1931	1939	1948	rVB	230678	354659	34.36%	3.948%
29	15.064	1965	1970	1977	rBV2	34452	58887	5.71%	0.656%
30	15.651	2064	2070	2072	rBV	974	1626	0.16%	0.018%
31	15.868	2100	2107	2116	rVB	487445	753727	73.03%	8.391%
32	15.974	2120	2125	2136	rBV	159055	244243	23.66%	2.719%
33	16.056	2136	2139	2144	rVB	1299	1627	0.16%	0.018%
34	16.109	2144	2148	2152	rBV4	2839	4149	0.40%	0.046%
35	16.562	2222	2225	2227	rVB2	1231	1324	0.13%	0.015%
36	16.808	2263	2267	2269	rBV	1141	1373	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052155.D
 Acq On : 26 Jan 2022 18:48
 Operator : CG/JU
 Sample : N1230-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	17.073	2308	2312	2315	rBV3	1012	1509	0.15%	0.017%
38	17.278	2342	2347	2354	rBV2	14509	22957	2.22%	0.256%
39	17.407	2365	2369	2370	rBV	1216	1744	0.17%	0.019%
40	17.631	2400	2407	2414	rVB	298817	464358	44.99%	5.169%
41	17.725	2417	2423	2436	rVB	570648	875783	84.85%	9.749%
42	17.819	2436	2439	2442	rBV3	1035	1339	0.13%	0.015%
43	17.889	2448	2451	2455	rBV4	1713	2426	0.24%	0.027%
44	18.271	2512	2516	2519	rBV2	6008	6934	0.67%	0.077%
45	18.494	2551	2554	2558	rVB5	2238	2931	0.28%	0.033%
46	18.623	2574	2576	2583	rBV3	1578	2761	0.27%	0.031%
47	18.747	2591	2597	2600	rBV2	965	1889	0.18%	0.021%
48	18.929	2626	2628	2631	rVB3	1522	1389	0.13%	0.015%
49	19.046	2646	2648	2651	rVB2	1878	1678	0.16%	0.019%
50	19.082	2651	2654	2656	rBV3	1604	1807	0.18%	0.020%
51	19.434	2711	2714	2718	rVB4	3766	4247	0.41%	0.047%
52	19.569	2733	2737	2744	rBV4	9985	15791	1.53%	0.176%
53	19.640	2744	2749	2756	rBV2	7743	14621	1.42%	0.163%
54	19.763	2766	2770	2773	rVB4	2020	2310	0.22%	0.026%
55	20.004	2805	2811	2817	rVB2	684196	1032118	100.00%	11.490%
56	20.204	2843	2845	2846	rBV	3494	2662	0.26%	0.030%
57	20.245	2851	2852	2855	rVB3	2956	1786	0.17%	0.020%
58	20.315	2862	2864	2869	rBV5	2071	2702	0.26%	0.030%
59	21.543	3069	3073	3084	rBV6	21592	52546	5.09%	0.585%
60	21.943	3135	3141	3149	rVB	283918	493334	47.80%	5.492%
61	25.185	3682	3693	3704	rVB	335957	990259	95.94%	11.024%
62	25.426	3723	3734	3749	rVB2	162442	524906	50.86%	5.843%
63	28.692	4288	4290	4291	rBV2	4372	2236	0.22%	0.025%




Sum of corrected areas: 8983030

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052155.D
Acq On : 26 Jan 2022 18:48
Operator : CG/JU
Sample : N1230-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

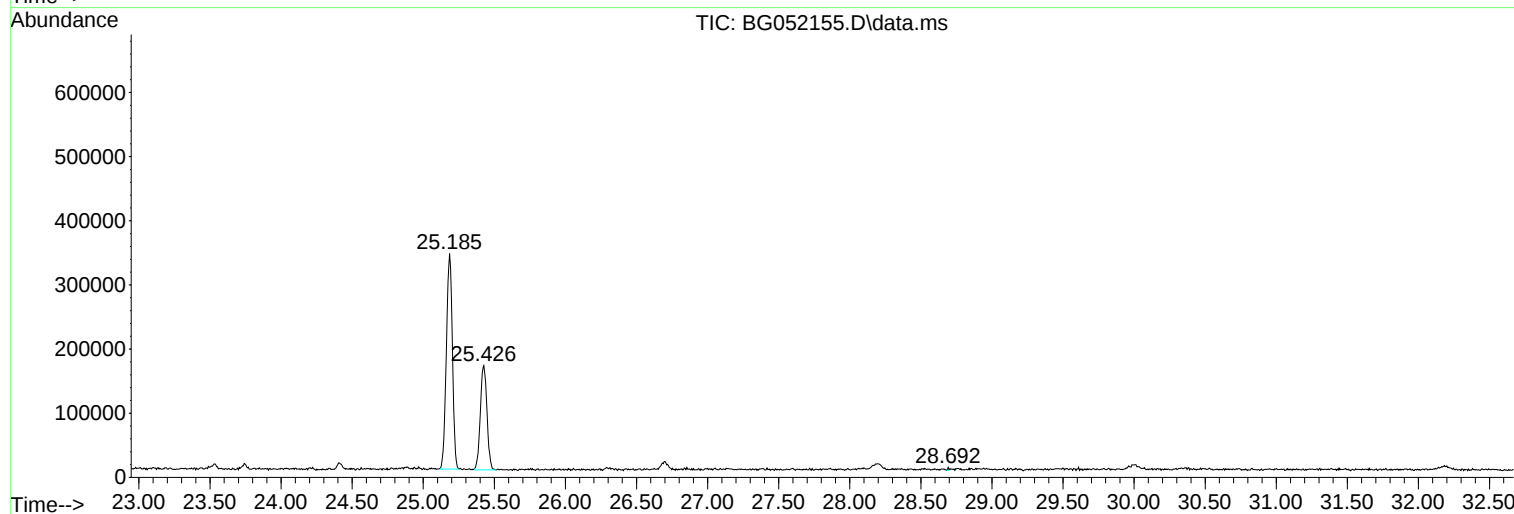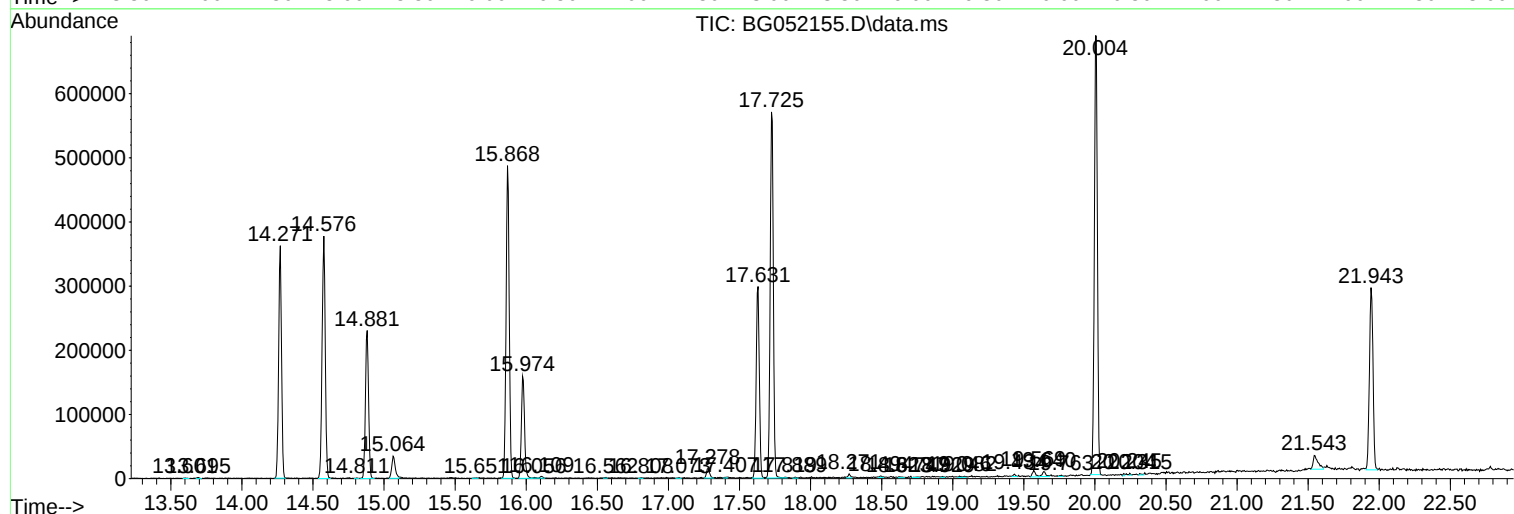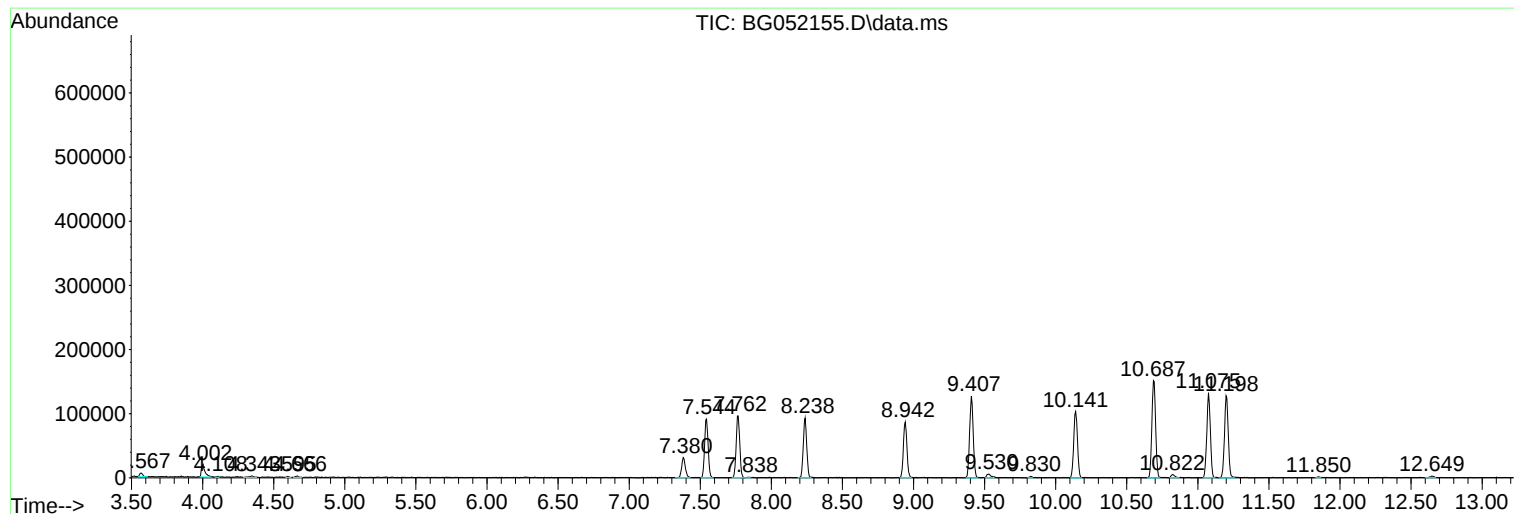

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052155.D
Acq On : 26 Jan 2022 18:48
Operator : CG/JU
Sample : N1230-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q20










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.543 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.543	2.13 ng/ul	52546	Chrysene-d12	21.942

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentadecane	210	C15H30	000295-48-7	96
2			1-Pentadecene	210	C15H30	013360-61-7	89
3			Bromoacetic acid, hexadecyl ester	362	C18H35BrO2	005454-48-8	76
4			Behenic alcohol	326	C22H46O	000661-19-8	68
5			Trichloroacetic acid, undecyl ester	316	C13H23Cl3O2	074339-49-4	68

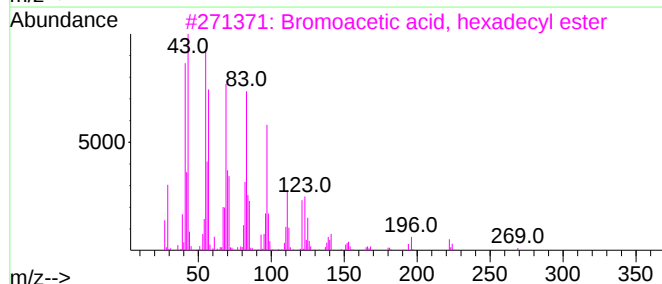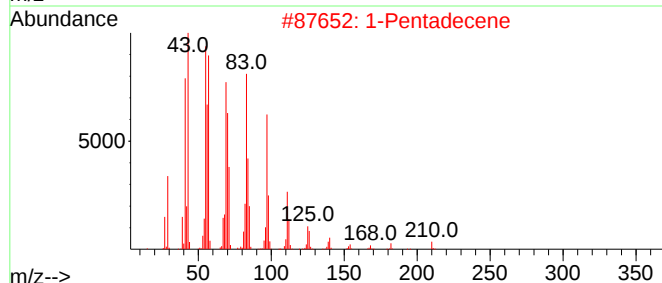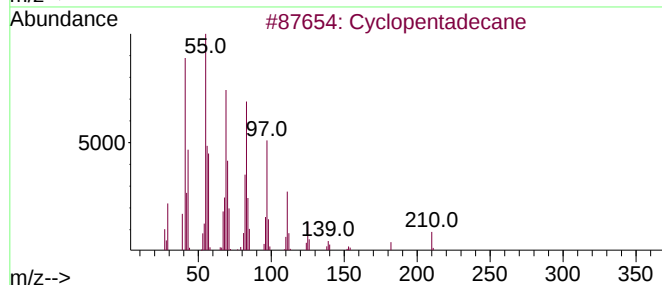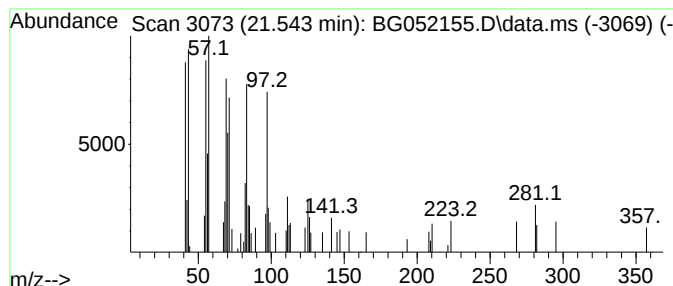

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052155.D
Acq On : 26 Jan 2022 18:48
Operator : CG/JU
Sample : N1230-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.543	2.1	ng/u1	52546	5	21.942	493334	20.0