

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052165.D
 Acq On : 27 Jan 2022 1:42
 Operator : CG/JU
 Sample : N1229-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.670	28	31	34	rBV3	982	1429	0.26%	0.061%
2	3.999	85	87	89	rBV2	820	1011	0.19%	0.043%
3	4.022	89	91	94	rVB	905	932	0.17%	0.040%
4	4.181	117	118	120	rVB	1124	690	0.13%	0.029%
5	4.228	125	126	128	rVB	1445	896	0.17%	0.038%
6	4.257	128	131	133	rBV2	1202	1580	0.29%	0.067%
7	4.345	143	146	149	rBV3	1714	1969	0.36%	0.084%
8	4.398	153	155	156	rBV3	814	827	0.15%	0.035%
9	4.439	158	162	164	rBV	553	759	0.14%	0.032%
10	4.463	164	166	170	rVB2	984	1331	0.25%	0.057%
11	4.492	170	171	174	rBV2	1054	1142	0.21%	0.049%
12	4.833	227	229	234	rVB2	1235	1896	0.35%	0.081%
13	4.880	234	237	238	rBV2	928	835	0.15%	0.035%
14	4.915	241	243	246	rVB	923	1144	0.21%	0.049%
15	4.992	255	256	259	rBV	622	754	0.14%	0.032%
16	5.385	320	323	325	rBV2	913	771	0.14%	0.033%
17	5.620	362	363	366	rVB2	1091	698	0.13%	0.030%
18	5.943	417	418	422	rBV	594	768	0.14%	0.033%
19	6.231	464	467	470	rBV	851	992	0.18%	0.042%
20	6.836	566	570	573	rBV2	428	725	0.13%	0.031%
21	6.889	576	579	582	rBV2	715	701	0.13%	0.030%
22	7.065	606	609	613	rBV	452	725	0.13%	0.031%
23	7.171	624	627	630	rBV	658	817	0.15%	0.035%
24	7.300	645	649	651	rVB	645	823	0.15%	0.035%
25	7.670	707	712	714	rBV	678	1043	0.19%	0.044%
26	7.929	753	756	760	rBB	672	808	0.15%	0.034%
27	7.999	763	768	772	rVV2	672	1535	0.28%	0.065%
28	8.064	776	779	782	rVB2	570	687	0.13%	0.029%
29	8.170	794	797	801	rVB	615	884	0.16%	0.038%
30	8.240	801	809	816	rBV	90859	152246	28.07%	6.470%
31	8.757	895	897	900	rBV	652	656	0.12%	0.028%
32	9.491	1018	1022	1025	rBV	416	851	0.16%	0.036%
33	9.574	1032	1036	1037	rVB	499	645	0.12%	0.027%
34	9.591	1038	1039	1042	rBV2	828	675	0.12%	0.029%
35	9.897	1086	1091	1095	rBV	418	717	0.13%	0.030%
36	10.102	1122	1126	1129	rBV	601	994	0.18%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052165.D
 Acq On : 27 Jan 2022 1:42
 Operator : CG/JU
 Sample : N1229-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	10.420	1177	1180	1183	rBV	555	834	0.15%	0.035%
38	10.637	1214	1217	1219	rBV	534	659	0.12%	0.028%
39	10.948	1268	1270	1273	rBV	488	632	0.12%	0.027%
40	11.077	1283	1292	1300	rBV	121114	216964	40.00%	9.220%

41	11.171	1305	1308	1310	rVB	623	677	0.12%	0.029%
42	12.270	1492	1495	1498	rBB	572	811	0.15%	0.034%
43	12.716	1567	1571	1572	rBV	524	647	0.12%	0.027%
44	14.391	1855	1856	1862	rVB2	719	916	0.17%	0.039%
45	14.444	1862	1865	1867	rBV2	751	1029	0.19%	0.044%

46	14.608	1888	1893	1896	rBV	429	820	0.15%	0.035%
47	14.737	1913	1915	1918	rBV	476	678	0.12%	0.029%
48	14.802	1924	1926	1930	rVB	591	754	0.14%	0.032%
49	14.878	1932	1939	1948	rBV	219663	352433	64.97%	14.976%
50	15.448	2034	2036	2039	rVB2	609	652	0.12%	0.028%

51	15.871	2106	2108	2111	rBV2	720	831	0.15%	0.035%
52	16.159	2153	2157	2160	rVB	621	907	0.17%	0.039%
53	16.200	2160	2164	2167	rBV3	733	922	0.17%	0.039%
54	16.523	2217	2219	2221	rBV3	765	705	0.13%	0.030%
55	16.564	2223	2226	2228	rBV2	632	680	0.13%	0.029%

56	16.635	2235	2238	2241	rVB2	534	683	0.13%	0.029%
57	17.052	2306	2309	2311	rBV2	840	681	0.13%	0.029%
58	17.310	2351	2353	2356	rVB	971	1021	0.19%	0.043%
59	17.351	2356	2360	2361	rBV	675	680	0.13%	0.029%
60	17.410	2368	2370	2372	rBV	1462	1509	0.28%	0.064%

61	17.627	2400	2407	2418	rBV	304083	471804	86.98%	20.049%
62	17.845	2442	2444	2446	rBV	917	795	0.15%	0.034%
63	17.974	2465	2466	2470	rBV2	862	800	0.15%	0.034%
64	18.520	2556	2559	2561	rBV	801	703	0.13%	0.030%
65	18.573	2566	2568	2570	rVB3	691	633	0.12%	0.027%

66	18.603	2570	2573	2574	rBV	609	777	0.14%	0.033%
67	18.685	2584	2587	2589	rVB2	945	874	0.16%	0.037%
68	18.896	2621	2623	2624	rBV	919	634	0.12%	0.027%
69	18.979	2636	2637	2640	rVB	846	698	0.13%	0.030%
70	19.172	2668	2670	2674	rVB2	666	699	0.13%	0.030%

71	19.202	2674	2675	2679	rVB2	1152	1344	0.25%	0.057%
72	19.237	2679	2681	2684	rBV2	794	1036	0.19%	0.044%
73	19.272	2684	2687	2688	rBV	888	761	0.14%	0.032%
74	19.319	2691	2695	2697	rBV3	796	1353	0.25%	0.057%
75	19.396	2706	2708	2711	rBV2	967	1129	0.21%	0.048%

76	19.525	2728	2730	2733	rVB2	832	797	0.15%	0.034%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052165.D
 Acq On : 27 Jan 2022 1:42
 Operator : CG/JU
 Sample : N1229-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	19.742	2766	2767	2770	rBV2	1118	827	0.15%	0.035%
78	19.877	2788	2790	2791	rBV	980	834	0.15%	0.035%
79	19.918	2795	2797	2798	rBV2	1055	845	0.16%	0.036%
80	19.989	2807	2809	2813	rVB4	1147	749	0.14%	0.032%
81	20.095	2825	2827	2828	rBV	1299	734	0.14%	0.031%
82	20.183	2840	2842	2844	rBV2	1376	1141	0.21%	0.048%
83	20.247	2852	2853	2856	rVB4	2006	1365	0.25%	0.058%
84	20.359	2870	2872	2873	rBV2	1965	1650	0.30%	0.070%
85	20.435	2883	2885	2886	rVB	1850	1262	0.23%	0.054%
86	20.453	2886	2888	2890	rBV2	1286	1090	0.20%	0.046%
87	20.482	2890	2893	2895	rVV3	1822	2152	0.40%	0.091%
88	21.945	3135	3142	3151	rBV	321611	534805	98.60%	22.726%
89	25.423	3724	3734	3746	rVB2	178955	542415	100.00%	23.049%
90	28.348	4230	4232	4235	rBV4	3041	3473	0.64%	0.148%
91	30.669	4626	4627	4629	rBV2	3780	2019	0.37%	0.086%




Sum of corrected areas: 2353279

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052165.D
Acq On : 27 Jan 2022 1:42
Operator : CG/JU
Sample : N1229-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

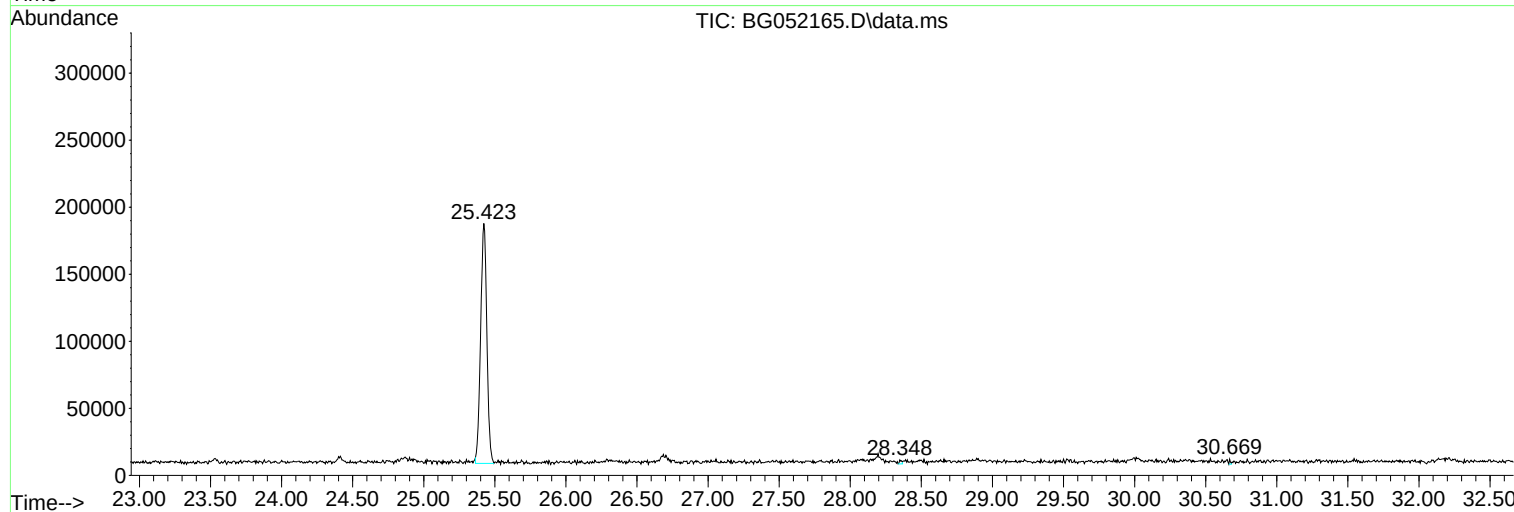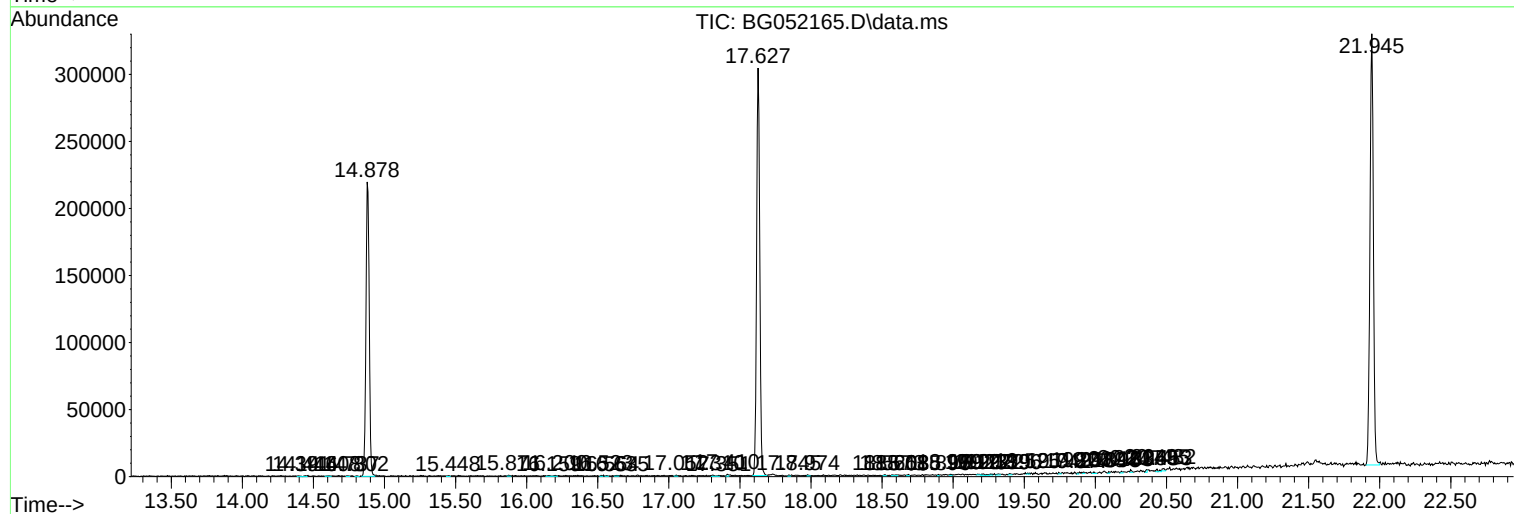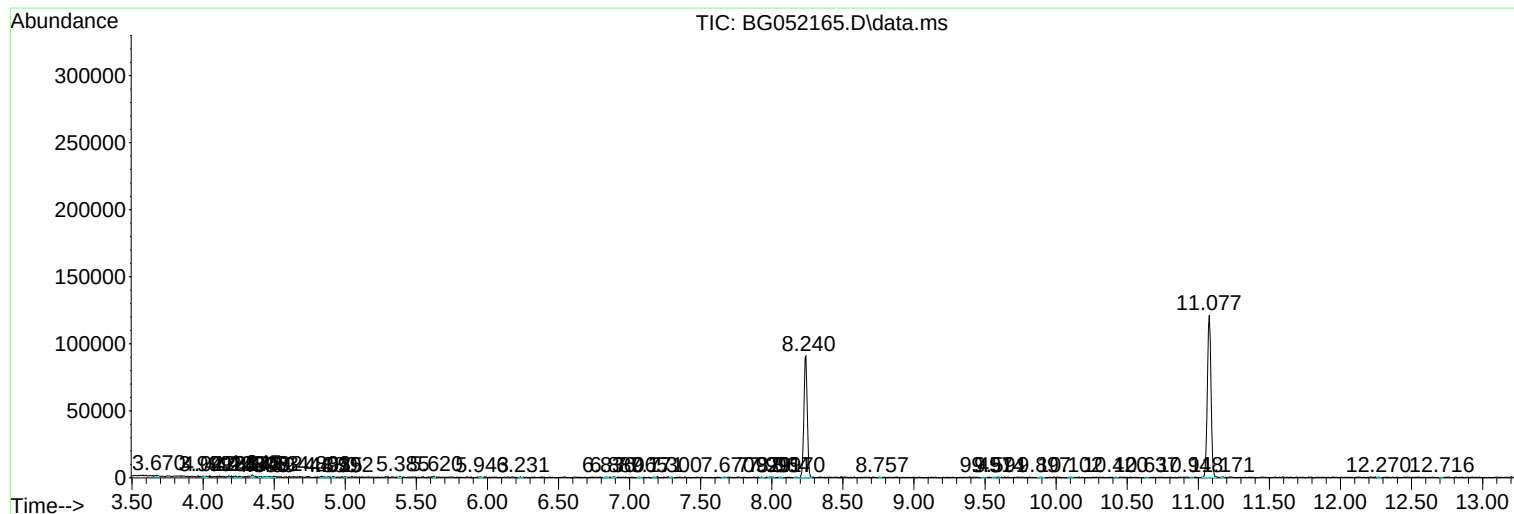

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052165.D
Acq On : 27 Jan 2022 1:42
Operator : CG/JU
Sample : N1229-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052165.D
Acq On : 27 Jan 2022 1:42
Operator : CG/JU
Sample : N1229-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc