

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052167.D
 Acq On : 27 Jan 2022 2:57
 Operator : CG/JU
 Sample : PB142285BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK285

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.564	9	13	21	rVB2	9296	13238	1.36%	0.139%
2	3.992	81	86	100	rBV	96902	169908	17.48%	1.780%
3	4.351	141	147	150	rBV3	1697	3093	0.32%	0.032%
4	4.838	225	230	232	rVB3	1069	1632	0.17%	0.017%
5	7.382	654	663	671	rBV	126224	219149	22.55%	2.296%
6	7.541	684	690	699	rBV	91419	152391	15.68%	1.596%
7	7.764	721	728	737	rVB	118591	203382	20.93%	2.130%
8	8.234	802	808	815	rVB	88510	150663	15.50%	1.578%
9	8.939	922	928	937	rBV2	148725	262448	27.01%	2.749%
10	9.409	999	1008	1016	rBV	118044	216708	22.30%	2.270%
11	10.143	1125	1133	1140	rBV	105373	183057	18.84%	1.918%
12	10.689	1219	1226	1237	rBV	156935	277909	28.60%	2.911%
13	11.077	1283	1292	1301	rBV	130403	228342	23.50%	2.392%
14	11.200	1305	1313	1323	rVV	145096	275650	28.36%	2.887%
15	12.657	1555	1561	1565	rVB3	2408	3920	0.40%	0.041%
16	14.273	1828	1836	1842	rBV	321720	473483	48.72%	4.960%
17	14.578	1881	1888	1896	rBV	352578	546223	56.21%	5.722%
18	14.884	1933	1940	1949	rVB	225072	362154	37.27%	3.794%
19	15.060	1965	1970	1982	rBV	129588	225684	23.22%	2.364%
20	15.870	2101	2108	2118	rVB	457858	691139	71.12%	7.240%
21	15.976	2121	2126	2136	rVV	120465	174150	17.92%	1.824%
22	16.111	2145	2149	2153	rVB	2422	2921	0.30%	0.031%
23	17.415	2366	2371	2374	rVV3	1472	1888	0.19%	0.020%
24	17.627	2401	2407	2417	rBV	309998	482359	49.63%	5.053%
25	17.727	2417	2424	2432	rBV	526442	811218	83.47%	8.498%
26	18.908	2622	2625	2628	rBV2	1057	1461	0.15%	0.015%
27	19.266	2683	2686	2690	rBV2	952	1626	0.17%	0.017%
28	19.571	2731	2738	2744	rBV4	6668	11934	1.23%	0.125%
29	19.642	2747	2750	2755	rVB2	7291	8623	0.89%	0.090%
30	19.877	2787	2790	2794	rVB3	1415	2146	0.22%	0.022%
31	19.918	2794	2797	2800	rBV2	1515	2125	0.22%	0.022%
32	20.006	2805	2812	2819	rBV	695520	971813	100.00%	10.180%
33	20.423	2881	2883	2888	rBV4	1140	1916	0.20%	0.020%
34	20.552	2902	2905	2908	rBV4	1411	1901	0.20%	0.020%
35	20.582	2908	2910	2912	rVB2	1579	1503	0.15%	0.016%
36	20.617	2912	2916	2917	rBV3	1295	1586	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052167.D
 Acq On : 27 Jan 2022 2:57
 Operator : CG/JU
 Sample : PB142285BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK285

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	20.676	2924	2926	2929	rVB4	1563	1471	0.15%	0.015%
38	20.799	2945	2947	2950	rBV4	2514	3191	0.33%	0.033%
39	20.828	2950	2952	2955	rVB3	1626	1500	0.15%	0.016%
40	21.293	3029	3031	3034	rVB3	1892	1596	0.16%	0.017%
41	21.557	3074	3076	3081	rVB6	3149	3149	0.32%	0.033%
42	21.633	3086	3089	3091	rBV3	2380	2195	0.23%	0.023%
43	21.804	3116	3118	3120	rBV2	2295	1771	0.18%	0.019%
44	21.945	3135	3142	3150	rVB2	311785	532292	54.77%	5.576%
45	22.086	3164	3166	3168	rVV2	1815	1545	0.16%	0.016%
46	22.133	3170	3174	3183	rVB7	4062	8658	0.89%	0.091%
47	22.415	3220	3222	3225	rBV4	1673	1523	0.16%	0.016%
48	22.650	3261	3262	3265	rBV3	1793	1638	0.17%	0.017%
49	22.761	3279	3281	3282	rBV2	2577	1452	0.15%	0.015%
50	22.820	3289	3291	3294	rVB4	1829	1483	0.15%	0.016%
51	23.055	3329	3331	3334	rBV2	2352	2202	0.23%	0.023%
52	23.537	3408	3413	3417	rVV5	8245	13263	1.36%	0.139%
53	23.613	3422	3426	3427	rBV3	2767	3535	0.36%	0.037%
54	23.719	3438	3444	3450	rVB8	6275	13019	1.34%	0.136%
55	24.147	3513	3517	3520	rBV6	1823	2521	0.26%	0.026%
56	24.206	3525	3527	3530	rVB3	3373	3261	0.34%	0.034%
57	24.412	3559	3562	3568	rVB6	8570	16129	1.66%	0.169%
58	24.682	3606	3608	3611	rBV4	1924	2725	0.28%	0.029%
59	24.876	3632	3641	3649	rBV7	11190	31328	3.22%	0.328%
60	25.040	3666	3669	3671	rBV3	2254	2964	0.30%	0.031%
61	25.181	3682	3693	3708	rVB2	321838	935757	96.29%	9.802%
62	25.281	3708	3710	3711	rBV	1970	1506	0.15%	0.016%
63	25.428	3720	3735	3751	rBV2	180129	569220	58.57%	5.963%
64	26.221	3865	3870	3872	rBV5	2400	4879	0.50%	0.051%
65	26.303	3875	3884	3893	rVB9	14803	48307	4.97%	0.506%
66	26.591	3931	3933	3934	rVB	3205	1967	0.20%	0.021%
67	26.609	3934	3936	3939	rBV3	1945	3208	0.33%	0.034%
68	26.644	3941	3942	3943	rVV	3983	2400	0.25%	0.025%
69	26.697	3946	3951	3956	rVV6	10491	29480	3.03%	0.309%
70	26.762	3960	3962	3964	rVB3	2997	1894	0.19%	0.020%
71	26.779	3964	3965	3968	rBV2	2366	2117	0.22%	0.022%
72	27.590	4101	4103	4106	rVB4	2307	1783	0.18%	0.019%
73	27.813	4139	4141	4146	rBV4	1930	2430	0.25%	0.025%
74	28.095	4179	4189	4197	rBV9	14446	49979	5.14%	0.524%
75	28.559	4266	4268	4272	rBV4	1824	2744	0.28%	0.029%
76	28.806	4307	4310	4311	rBV2	1812	1830	0.19%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052167.D
 Acq On : 27 Jan 2022 2:57
 Operator : CG/JU
 Sample : PB142285BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK285

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	29.141	4364	4367	4368	rBV3	1677	1591	0.16%	0.017%
78	29.158	4368	4370	4372	rBV2	1545	1463	0.15%	0.015%
79	29.217	4378	4380	4381	rBV2	2201	1714	0.18%	0.018%
80	29.340	4399	4401	4403	rBV3	2314	1740	0.18%	0.018%
81	29.523	4430	4432	4436	rBV5	2003	2135	0.22%	0.022%
82	29.622	4447	4449	4450	rBV	2317	2180	0.22%	0.023%
83	29.658	4453	4455	4457	rBV2	1915	1439	0.15%	0.015%
84	29.993	4504	4512	4515	rBV9	6553	17449	1.80%	0.183%
85	30.139	4536	4537	4540	rVB3	2340	1798	0.19%	0.019%
86	30.286	4559	4562	4563	rBV2	4760	4075	0.42%	0.043%
87	30.339	4563	4571	4572	rBV5	15272	28427	2.93%	0.298%
88	30.486	4594	4596	4598	rBV2	2286	1447	0.15%	0.015%
89	30.598	4614	4615	4617	rBV2	2066	1645	0.17%	0.017%
90	30.921	4668	4670	4672	rBV3	1857	1417	0.15%	0.015%
91	31.373	4744	4747	4751	rVB6	1675	2453	0.25%	0.026%
92	31.655	4793	4795	4797	rBV3	1400	1456	0.15%	0.015%
93	31.690	4800	4801	4804	rVB3	2490	2413	0.25%	0.025%
94	31.725	4804	4807	4808	rBV2	1706	1751	0.18%	0.018%
95	32.137	4871	4877	4878	rBV4	3324	6851	0.70%	0.072%
96	32.166	4881	4882	4883	rBV	2424	1409	0.14%	0.015%
97	32.289	4901	4903	4905	rBB3	1753	1573	0.16%	0.016%
98	32.336	4909	4911	4913	rBV3	2390	1871	0.19%	0.020%
99	32.360	4913	4915	4918	rBV4	2069	2500	0.26%	0.026%
100	32.618	4956	4959	4961	rBV3	1954	2403	0.25%	0.025%




Sum of corrected areas: 9546455

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052167.D
Acq On : 27 Jan 2022 2:57
Operator : CG/JU
Sample : PB142285BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

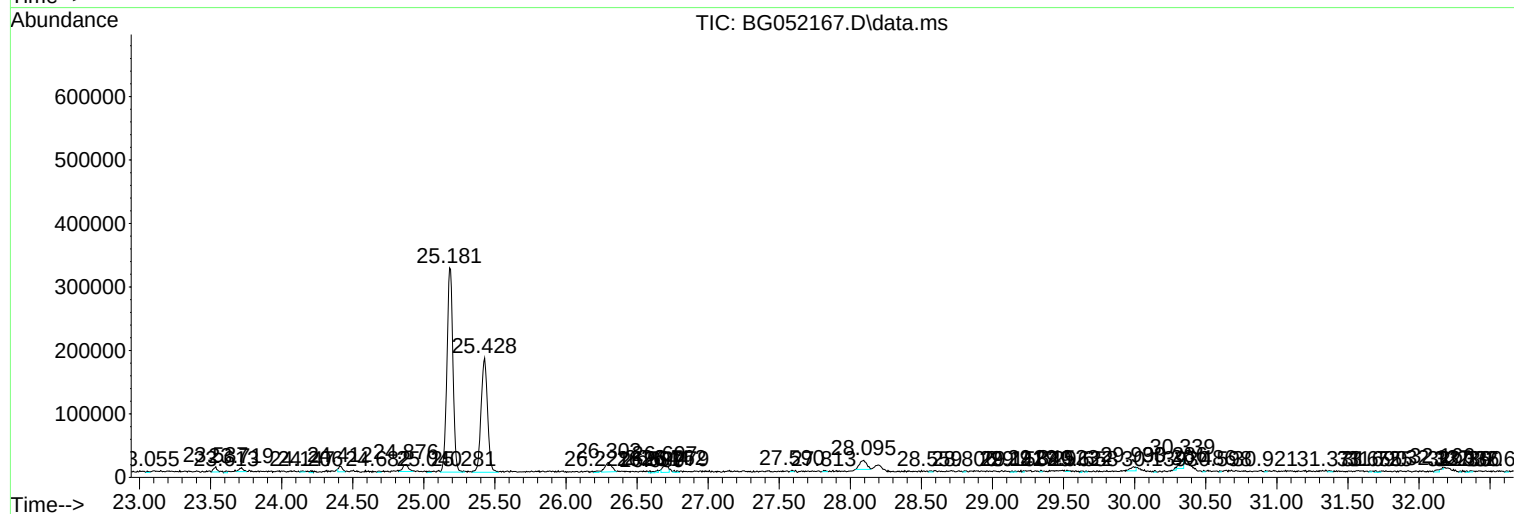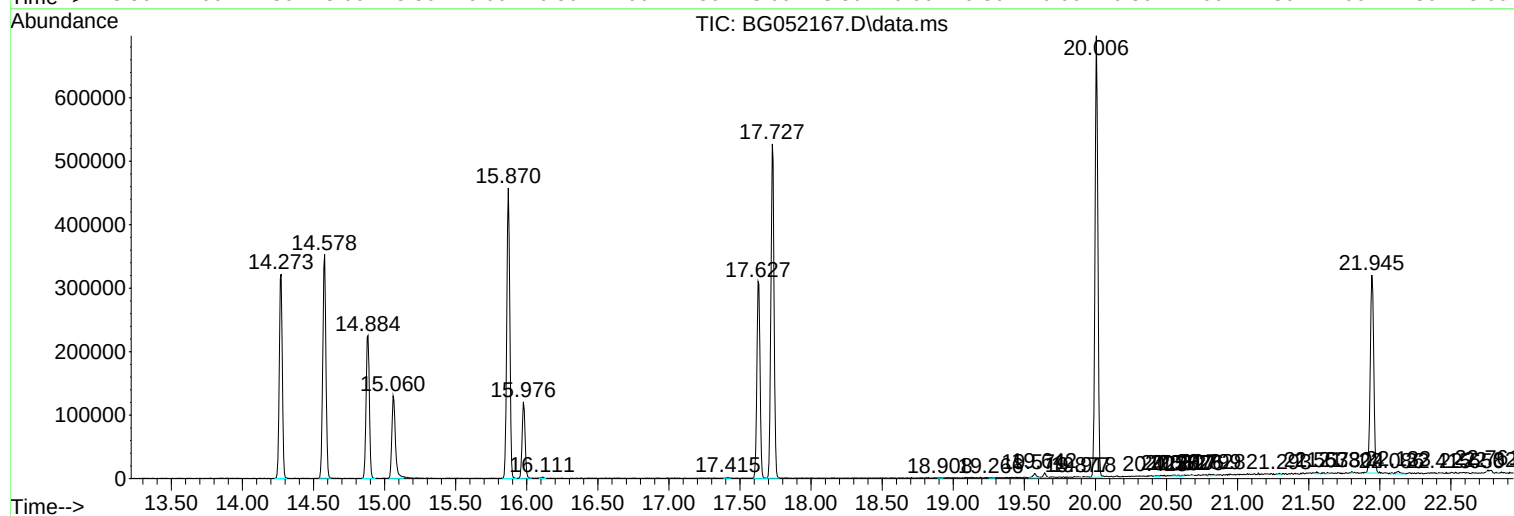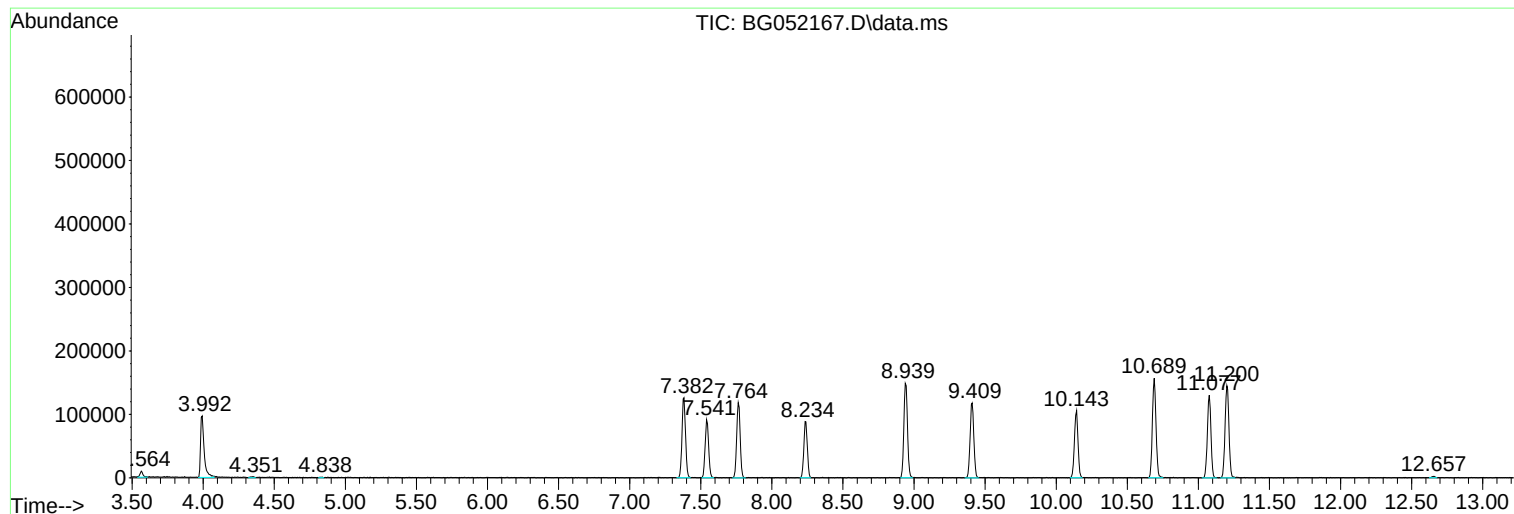

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052167.D
Acq On : 27 Jan 2022 2:57
Operator : CG/JU
Sample : PB142285BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052167.D
Acq On : 27 Jan 2022 2:57
Operator : CG/JU
Sample : PB142285BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc