

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052181.D
 Acq On : 27 Jan 2022 12:19
 Operator : CG/JU
 Sample : N1279-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COVD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.565	9	13	20	rVB4	5943	10325	1.07%	0.132%
2	4.012	86	89	92	rBV	3510	3713	0.38%	0.047%
3	4.347	143	146	149	rBV3	1444	2027	0.21%	0.026%
4	4.517	173	175	178	rBV3	1332	1497	0.15%	0.019%
5	4.858	230	233	235	rVB2	1568	1567	0.16%	0.020%
6	4.875	235	236	239	rBV2	1315	1283	0.13%	0.016%
7	4.981	251	254	257	rBV2	1056	1554	0.16%	0.020%
8	5.281	303	305	309	rVB2	1457	1375	0.14%	0.018%
9	6.561	520	523	529	rBV2	602	1401	0.14%	0.018%
10	7.213	632	634	639	rVB3	1772	2012	0.21%	0.026%
11	7.378	652	662	669	rBV3	24191	44547	4.60%	0.568%
12	7.542	682	690	700	rBV	88844	147949	15.26%	1.888%
13	7.766	721	728	736	rVB	87214	147630	15.23%	1.884%
14	8.236	801	808	816	rVB	81426	133151	13.74%	1.699%
15	8.941	921	928	936	rVB	69529	115944	11.96%	1.480%
16	9.405	1000	1007	1017	rVB	115205	206203	21.27%	2.631%
17	9.822	1072	1078	1083	rVB	10693	16755	1.73%	0.214%
18	10.139	1124	1132	1140	rVB	93429	166229	17.15%	2.121%
19	10.691	1219	1226	1234	rBV	130869	238429	24.60%	3.043%
20	11.073	1284	1291	1300	rBV	112660	199823	20.61%	2.550%
21	11.202	1305	1313	1322	rVV	62150	116350	12.00%	1.485%
22	12.324	1498	1504	1508	rBV3	4317	5340	0.55%	0.068%
23	12.653	1555	1560	1565	rVB4	2676	4305	0.44%	0.055%
24	14.269	1828	1835	1843	rBV	295609	436033	44.98%	5.564%
25	14.574	1879	1887	1898	rBV	324848	509021	52.51%	6.496%
26	14.880	1928	1939	1946	rBV	206185	315219	32.52%	4.022%
27	15.068	1964	1971	1985	rBV3	16975	35782	3.69%	0.457%
28	15.866	2101	2107	2120	rVB	444286	663742	68.47%	8.470%
29	15.972	2120	2125	2132	rBV	108033	161675	16.68%	2.063%
30	16.107	2144	2148	2151	rVB2	1954	2100	0.22%	0.027%
31	17.411	2367	2370	2375	rBV2	1268	1974	0.20%	0.025%
32	17.629	2400	2407	2414	rBV	279565	423221	43.66%	5.401%
33	17.729	2417	2424	2431	rVV	522714	794126	81.92%	10.134%
34	18.281	2515	2518	2523	rVB	1273	1594	0.16%	0.020%
35	18.945	2626	2631	2634	rBV2	1247	2115	0.22%	0.027%
36	18.974	2634	2636	2641	rBV2	1270	1365	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052181.D
 Acq On : 27 Jan 2022 12:19
 Operator : CG/JU
 Sample : N1279-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0VD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	19.115	2657	2660	2663	rBV2	1398	1433	0.15%	0.018%
38	19.174	2667	2670	2673	rBV2	1065	1507	0.16%	0.019%
39	19.274	2684	2687	2692	rBV2	1055	1717	0.18%	0.022%
40	19.567	2730	2737	2741	rBV3	7294	10909	1.13%	0.139%
41	19.644	2746	2750	2754	rVV3	5934	8311	0.86%	0.106%
42	19.932	2797	2799	2802	rBV2	1526	1897	0.20%	0.024%
43	20.008	2805	2812	2820	rVB	668853	969371	100.00%	12.370%
44	20.284	2855	2859	2860	rBV2	1479	2080	0.21%	0.027%
45	20.407	2878	2880	2883	rBV3	1527	1788	0.18%	0.023%
46	20.989	2978	2979	2982	rBV3	1890	2138	0.22%	0.027%
47	21.042	2987	2988	2991	rVB2	2370	1610	0.17%	0.021%
48	21.946	3135	3142	3152	rVB2	274249	473797	48.88%	6.046%
49	24.402	3557	3560	3561	rBV3	6079	6089	0.63%	0.078%
50	25.183	3681	3693	3706	rVB3	303619	931480	96.09%	11.887%
51	25.424	3723	3734	3751	rVB3	156168	500710	51.65%	6.390%
52	28.156	4197	4199	4201	rBV3	4529	4184	0.43%	0.053%




Sum of corrected areas: 7836397

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052181.D
Acq On : 27 Jan 2022 12:19
Operator : CG/JU
Sample : N1279-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0VD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

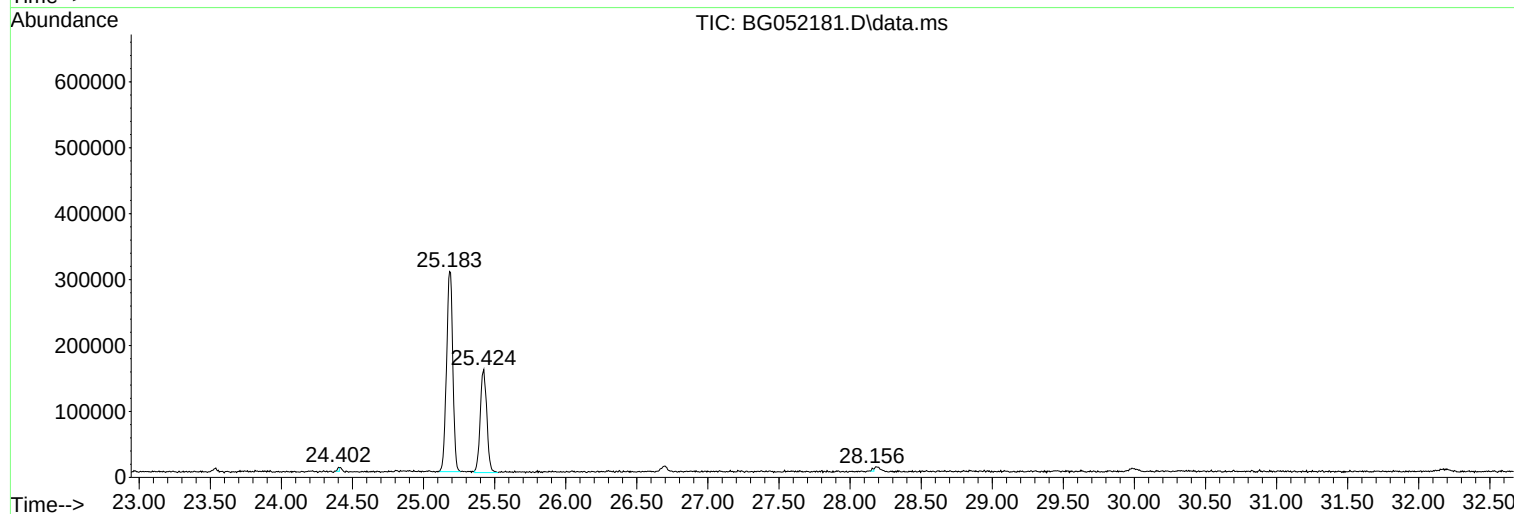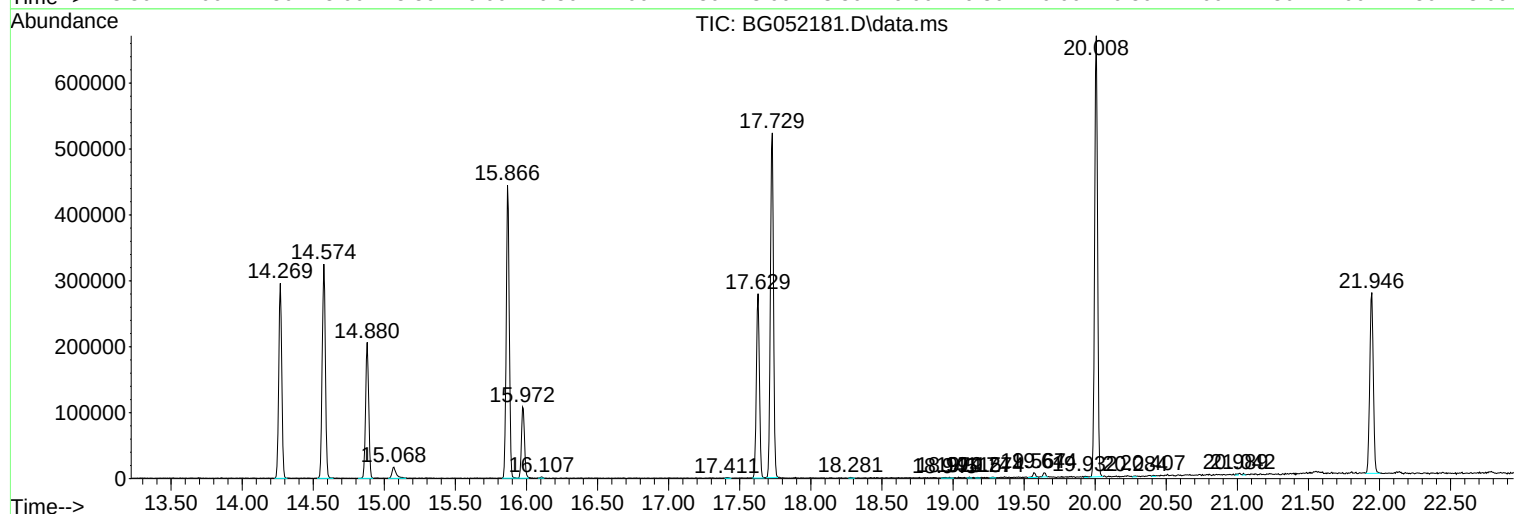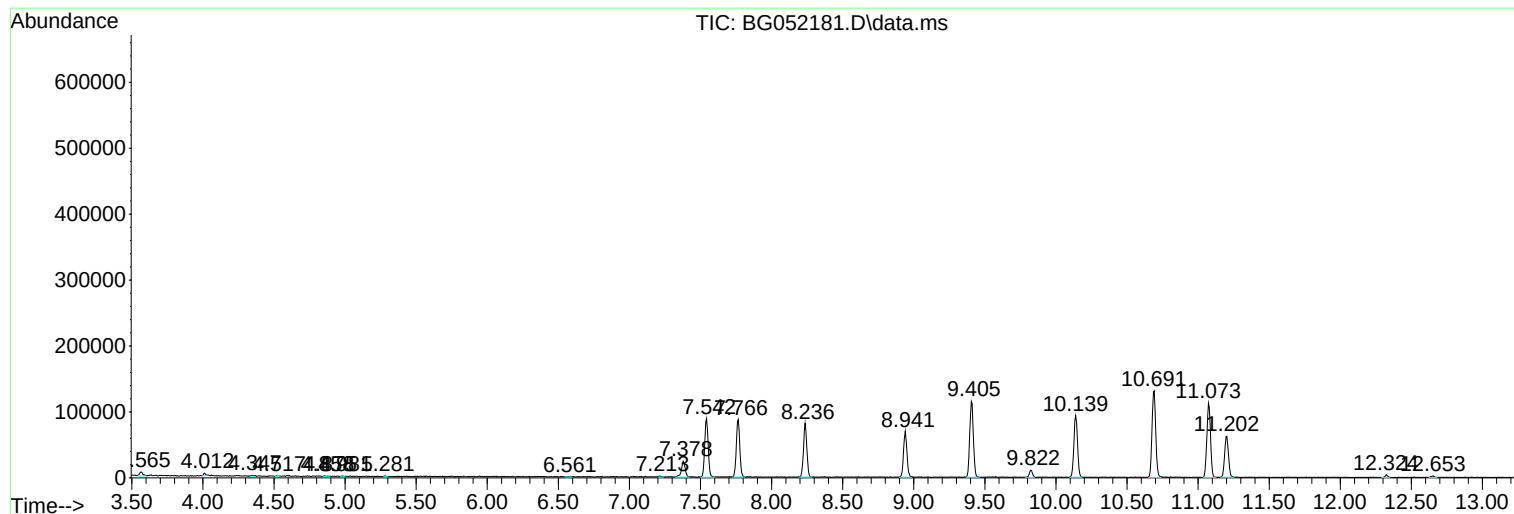

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052181.D
Acq On : 27 Jan 2022 12:19
Operator : CG/JU
Sample : N1279-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0VD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052181.D
Acq On : 27 Jan 2022 12:19
Operator : CG/JU
Sample : N1279-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0VD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc