

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052185.D
 Acq On : 27 Jan 2022 14:50
 Operator : CG/JU
 Sample : N1279-05
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COVID3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.567	9	13	17	rVB4	4634	6759	0.70%	0.088%
2	3.996	83	86	93	rBV	15921	27379	2.84%	0.355%
3	4.348	142	146	148	rVB3	1531	1728	0.18%	0.022%
4	7.379	657	662	670	rVB2	23821	38438	3.99%	0.499%
5	7.544	681	690	698	rBV	76913	134589	13.97%	1.746%
6	7.761	721	727	735	rBV	79916	134430	13.95%	1.744%
7	8.237	801	808	815	rBV2	80875	138443	14.37%	1.796%
8	8.942	921	928	935	rBV	65637	107618	11.17%	1.396%
9	9.406	1000	1007	1014	rBV	105277	188971	19.61%	2.452%
10	9.823	1074	1078	1082	rBV3	3180	4566	0.47%	0.059%
11	10.140	1124	1132	1140	rBV2	87284	153560	15.93%	1.992%
12	10.687	1217	1225	1233	rBV	116602	212892	22.09%	2.762%
13	11.074	1284	1291	1299	rBV	111398	200042	20.76%	2.595%
14	11.198	1305	1312	1320	rBV	106968	192869	20.01%	2.502%
15	12.326	1499	1504	1508	rVB2	4455	6431	0.67%	0.083%
16	12.649	1555	1559	1560	rBV2	1757	1940	0.20%	0.025%
17	13.694	1732	1737	1742	rBV2	1657	1928	0.20%	0.025%
18	14.270	1828	1835	1841	rBV	277600	395637	41.05%	5.133%
19	14.576	1879	1887	1894	rBV	297910	467033	48.46%	6.059%
20	14.881	1932	1939	1947	rVB	201167	313456	32.53%	4.067%
21	15.069	1966	1971	1985	rBV3	16147	32299	3.35%	0.419%
22	15.868	2098	2107	2116	rBV	405403	633707	65.76%	8.221%
23	15.980	2120	2126	2136	rVB	103640	158344	16.43%	2.054%
24	16.115	2145	2149	2152	rBV2	1816	2677	0.28%	0.035%
25	17.419	2366	2371	2375	rBV3	1686	2516	0.26%	0.033%
26	17.630	2400	2407	2414	rBV	278965	415744	43.14%	5.394%
27	17.730	2417	2424	2433	rVB	538744	799351	82.95%	10.370%
28	18.864	2614	2617	2618	rBV2	1138	1270	0.13%	0.016%
29	18.905	2622	2624	2628	rVV3	1059	1493	0.15%	0.019%
30	19.252	2679	2683	2685	rBV3	1048	1431	0.15%	0.019%
31	19.469	2718	2720	2723	rBV2	1258	1601	0.17%	0.021%
32	19.575	2734	2738	2743	rBV4	6638	9484	0.98%	0.123%
33	19.645	2746	2750	2757	rVB2	7291	9829	1.02%	0.128%
34	19.716	2757	2762	2763	rBV2	972	1500	0.16%	0.019%
35	19.804	2776	2777	2781	rBV	1522	1708	0.18%	0.022%
36	20.009	2805	2812	2825	rVB	647804	963711	100.00%	12.503%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052185.D
 Acq On : 27 Jan 2022 14:50
 Operator : CG/JU
 Sample : N1279-05
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0VD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	21.637	3088	3089	3092	rBV2	2777	1843	0.19%	0.024%
38	21.948	3135	3142	3150	rVB	276255	475754	49.37%	6.172%
39	23.164	3347	3349	3351	rBV3	2565	1390	0.14%	0.018%
40	23.534	3407	3412	3416	rBV5	9074	15204	1.58%	0.197%
41	23.857	3465	3467	3468	rBV2	3013	2481	0.26%	0.032%
42	24.415	3556	3562	3570	rVB7	12110	27218	2.82%	0.353%
43	25.185	3682	3693	3705	rBV2	302920	915362	94.98%	11.875%
44	25.426	3724	3734	3747	rVB2	157600	501166	52.00%	6.502%
45	31.200	4715	4717	4719	rBV3	2790	2239	0.23%	0.029%




Sum of corrected areas: 7708031

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052185.D
Acq On : 27 Jan 2022 14:50
Operator : CG/JU
Sample : N1279-05
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0VD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

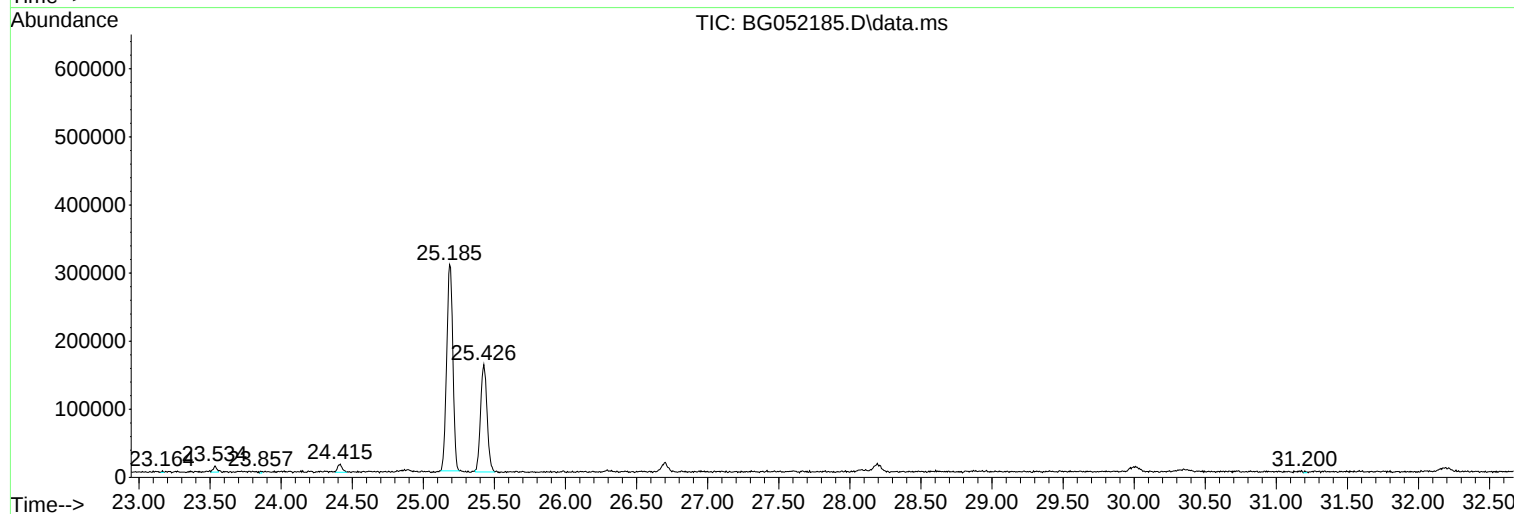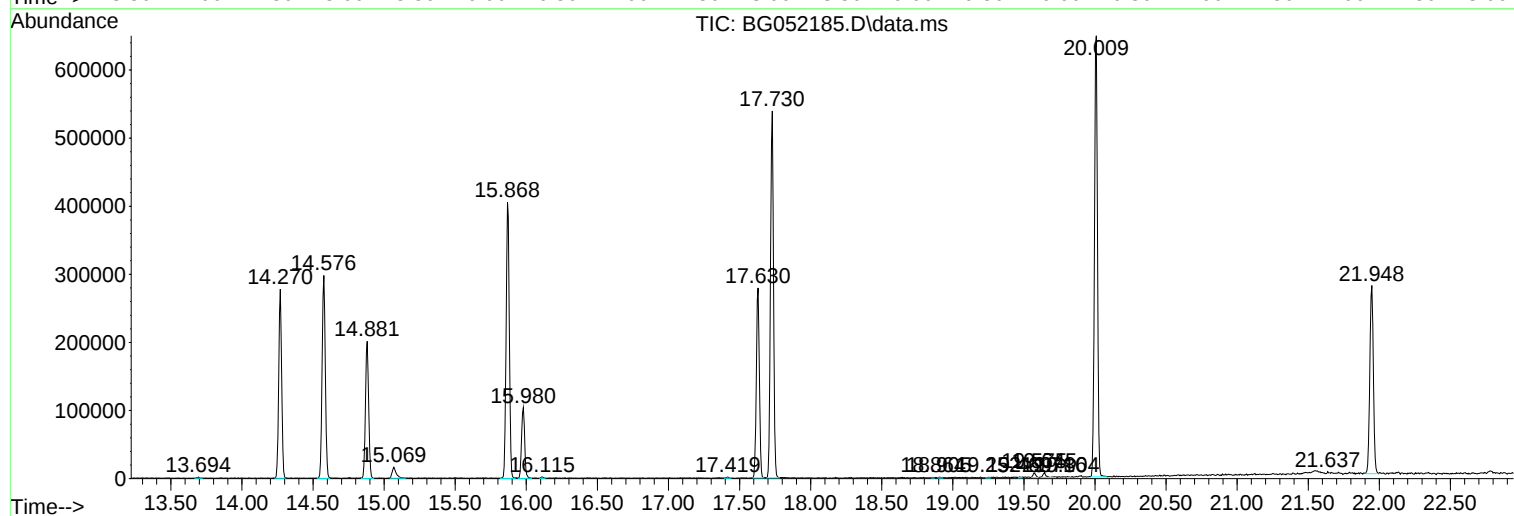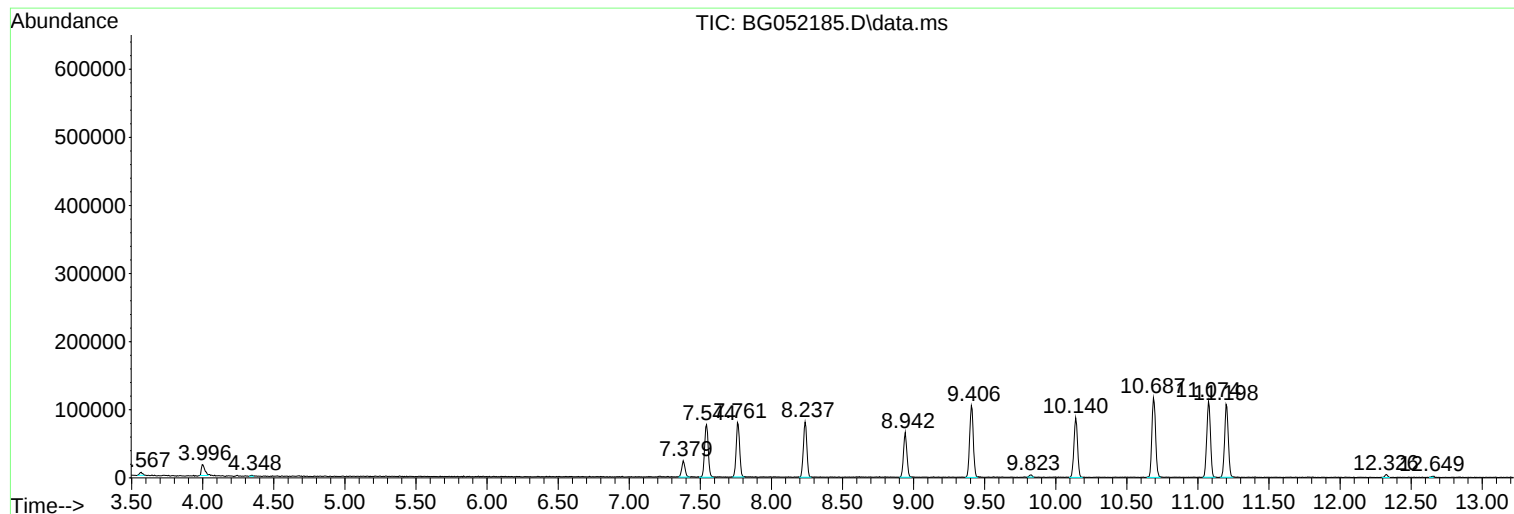

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052185.D
Acq On : 27 Jan 2022 14:50
Operator : CG/JU
Sample : N1279-05
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0VD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052185.D
Acq On : 27 Jan 2022 14:50
Operator : CG/JU
Sample : N1279-05
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0VD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc