

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052193.D
 Acq On : 27 Jan 2022 20:29
 Operator : CG/JU
 Sample : PB142310BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK310

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.567	9	13	17	rBV3	8262	11206	1.24%	0.129%
2	3.990	81	85	106	rBV	100203	174753	19.28%	2.008%
3	4.172	114	116	119	rBV3	1318	1669	0.18%	0.019%
4	4.895	236	239	242	rVB2	968	1179	0.13%	0.014%
5	5.400	322	325	327	rBV2	1115	1394	0.15%	0.016%
6	7.380	655	662	672	rBV	130248	221716	24.47%	2.547%
7	7.544	683	690	698	rBV	89047	154613	17.06%	1.776%
8	7.762	721	727	738	rVB	116447	205756	22.71%	2.364%
9	8.237	801	808	815	rVB	89050	147129	16.24%	1.690%
10	8.942	920	928	939	rVB	153484	266667	29.43%	3.064%
11	9.406	1000	1007	1016	rVB2	118243	215924	23.83%	2.481%
12	10.141	1124	1132	1140	rBV2	103751	186889	20.62%	2.147%
13	10.687	1218	1225	1236	rBV	157359	275032	30.35%	3.160%
14	11.075	1283	1291	1299	rBV	127152	219677	24.24%	2.524%
15	11.198	1305	1312	1326	rVB	148130	270459	29.85%	3.107%
16	12.103	1460	1466	1470	rVB	616	1518	0.17%	0.017%
17	12.655	1554	1560	1565	rBV3	1734	3621	0.40%	0.042%
18	14.270	1828	1835	1842	rBV	316902	449372	49.59%	5.163%
19	14.576	1879	1887	1895	rBV	347319	538675	59.45%	6.188%
20	14.881	1932	1939	1946	rVB	216975	336001	37.08%	3.860%
21	14.981	1955	1956	1962	rVB2	918	1409	0.16%	0.016%
22	15.063	1962	1970	1984	rBV	114467	206613	22.80%	2.374%
23	15.269	2001	2005	2009	rVB3	836	1286	0.14%	0.015%
24	15.868	2101	2107	2116	rBV	452208	670525	74.00%	7.703%
25	15.974	2120	2125	2134	rVB	102512	154412	17.04%	1.774%
26	16.109	2144	2148	2153	rVB4	2081	3449	0.38%	0.040%
27	17.631	2399	2407	2417	rBV	276399	432731	47.75%	4.971%
28	17.725	2417	2423	2430	rBV2	500313	752721	83.07%	8.648%
29	19.575	2734	2738	2742	rBV4	7658	9304	1.03%	0.107%
30	19.640	2746	2749	2754	rVB3	6358	8610	0.95%	0.099%
31	19.769	2769	2771	2775	rVB3	1222	1620	0.18%	0.019%
32	19.869	2786	2788	2791	rBV3	1141	1323	0.15%	0.015%
33	20.004	2805	2811	2818	rBV	604938	906169	100.00%	10.410%
34	20.098	2826	2827	2829	rBV	1526	1163	0.13%	0.013%
35	20.826	2949	2951	2954	rBV2	1940	2083	0.23%	0.024%
36	21.942	3135	3141	3151	rVB2	284499	486909	53.73%	5.594%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052193.D
Acq On : 27 Jan 2022 20:29
Operator : CG/JU
Sample : PB142310BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK310

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

37	25.185	3682	3693	3709	rVB3	296808	875763	96.64%	10.061%
38	25.426	3723	3734	3748	rVB2	157253	500250	55.20%	5.747%
39	26.107	3848	3850	3851	rBV2	2362	1383	0.15%	0.016%
40	27.623	4106	4108	4112	rBV4	3457	3497	0.39%	0.040%




Sum of corrected areas: 8704470

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052193.D
Acq On : 27 Jan 2022 20:29
Operator : CG/JU
Sample : PB142310BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK310

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

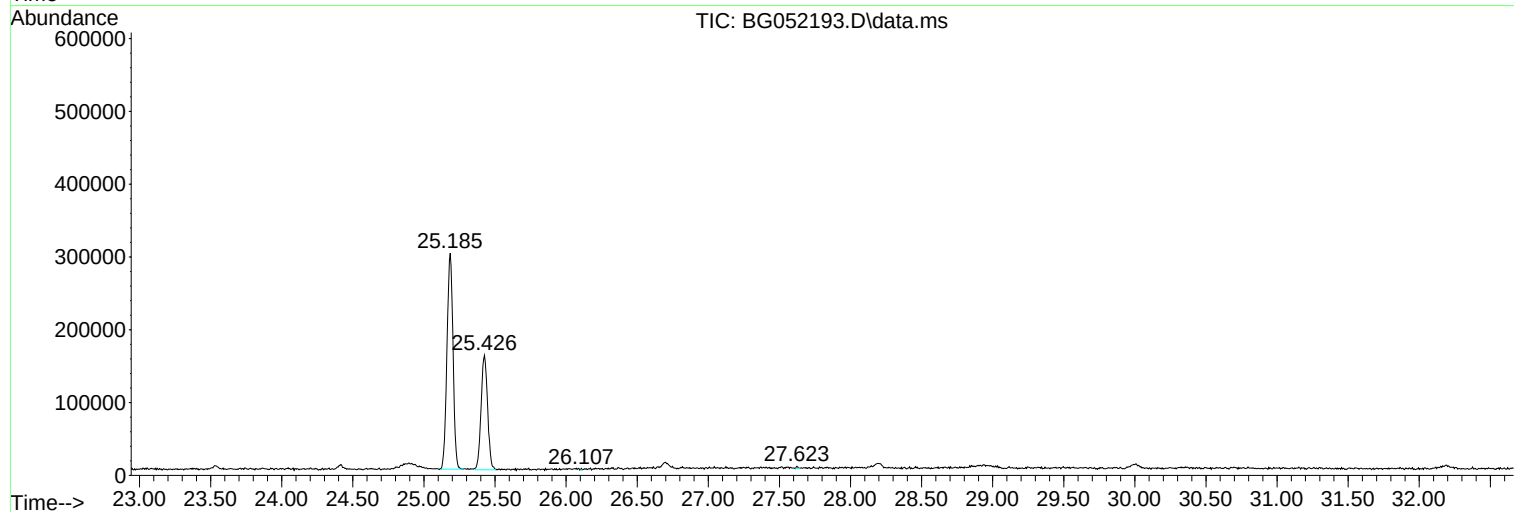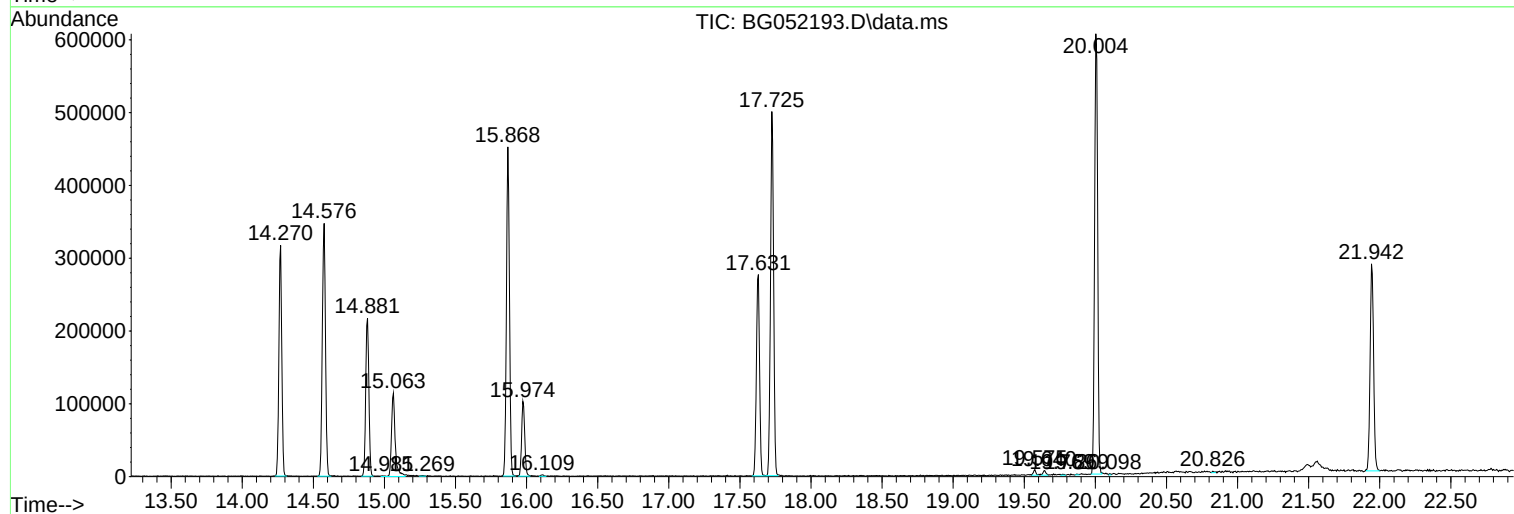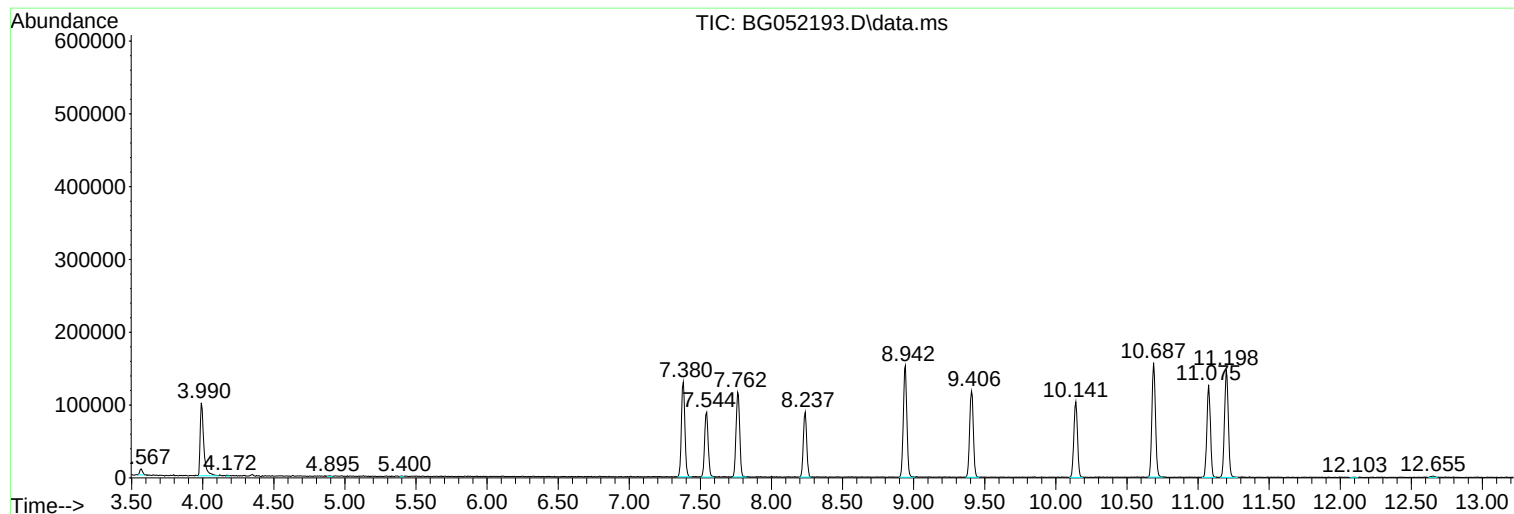

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052193.D
Acq On : 27 Jan 2022 20:29
Operator : CG/JU
Sample : PB142310BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK310

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052193.D
Acq On : 27 Jan 2022 20:29
Operator : CG/JU
Sample : PB142310BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK310

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc