

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052194.D
 Acq On : 27 Jan 2022 21:06
 Operator : CG/JU
 Sample : PB142333BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK333

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.567	8	13	19	rBV2	8103	12009	1.34%	0.142%
2	3.990	80	85	97	rBV	96112	163977	18.26%	1.932%
3	4.225	122	125	127	rVB2	1082	1255	0.14%	0.015%
4	4.343	143	145	149	rVB4	1637	2118	0.24%	0.025%
5	4.624	190	193	194	rBV	972	1205	0.13%	0.014%
6	7.380	654	662	674	rVB	127934	214778	23.92%	2.531%
7	7.544	683	690	703	rVB	89084	147889	16.47%	1.743%
8	7.761	720	727	738	rVB	118242	202279	22.53%	2.383%
9	8.237	801	808	817	rVB	83630	141775	15.79%	1.671%
10	8.942	921	928	936	rVB	149292	254300	28.32%	2.996%
11	9.406	1000	1007	1015	rVB	116829	210689	23.46%	2.483%
12	10.141	1125	1132	1140	rBV	101394	178171	19.84%	2.099%
13	10.687	1218	1225	1234	rBV	145687	262464	29.23%	3.093%
14	10.746	1234	1235	1241	rVB2	1125	1272	0.14%	0.015%
15	11.075	1284	1291	1300	rBV	116519	211011	23.50%	2.486%
16	11.198	1305	1312	1321	rBV	141524	261298	29.10%	3.079%
17	12.655	1555	1560	1561	rBV4	2441	2869	0.32%	0.034%
18	14.270	1829	1835	1842	rVB	296946	430756	47.97%	5.076%
19	14.576	1880	1887	1894	rBV	329208	517121	57.59%	6.093%
20	14.881	1932	1939	1946	rVB	208272	325157	36.21%	3.831%
21	15.063	1961	1970	1983	rBV	116141	204248	22.75%	2.407%
22	15.868	2101	2107	2115	rBV	425428	646589	72.01%	7.619%
23	15.980	2120	2126	2138	rVB	102624	150692	16.78%	1.776%
24	16.109	2143	2148	2153	rBV2	2349	2748	0.31%	0.032%
25	17.407	2367	2369	2374	rBV3	821	1292	0.14%	0.015%
26	17.630	2400	2407	2413	rBV	287400	426344	47.48%	5.024%
27	17.730	2417	2424	2432	rVV2	476770	747035	83.20%	8.802%
28	18.535	2557	2561	2563	rVB2	1178	1521	0.17%	0.018%
29	18.564	2563	2566	2568	rBV2	1533	1634	0.18%	0.019%
30	19.193	2669	2673	2675	rBV2	1046	1469	0.16%	0.017%
31	19.381	2700	2705	2706	rBV2	1089	1336	0.15%	0.016%
32	19.451	2713	2717	2720	rVB3	789	1322	0.15%	0.016%
33	19.569	2734	2737	2743	rBV3	6060	8838	0.98%	0.104%
34	19.639	2747	2749	2756	rVB	5684	8051	0.90%	0.095%
35	20.004	2805	2811	2820	rVB	615532	897931	100.00%	10.580%
36	20.121	2829	2831	2834	rBV3	1372	2129	0.24%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052194.D
 Acq On : 27 Jan 2022 21:06
 Operator : CG/JU
 Sample : PB142333BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK333

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	21.948	3135	3142	3149	rBV	277483	478079	53.24%	5.633%
38	22.395	3216	3218	3221	rBV2	3222	2515	0.28%	0.030%
39	23.199	3353	3355	3359	rBV3	3960	4444	0.49%	0.052%
40	24.885	3640	3642	3643	rBV2	3207	2265	0.25%	0.027%
41	25.191	3683	3694	3705	rVB2	294652	862977	96.11%	10.168%
42	25.426	3723	3734	3746	rVB2	161114	481339	53.61%	5.672%
43	27.488	4083	4085	4089	rBV4	2885	3363	0.37%	0.040%
44	27.523	4089	4091	4092	rVB2	3071	1408	0.16%	0.017%
45	27.758	4130	4131	4133	rBV2	2625	1724	0.19%	0.020%
46	30.431	4584	4586	4587	rVB2	2902	1282	0.14%	0.015%
47	30.954	4673	4675	4677	rVB2	2863	1868	0.21%	0.022%




Sum of corrected areas: 8486836

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052194.D
Acq On : 27 Jan 2022 21:06
Operator : CG/JU
Sample : PB142333BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

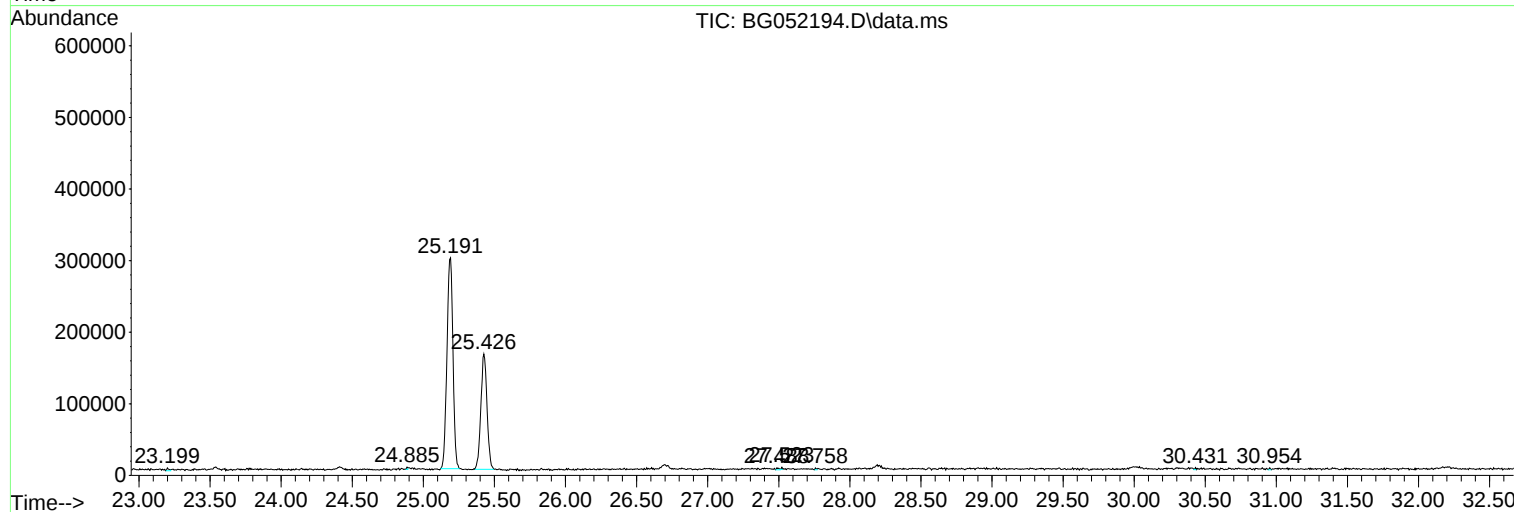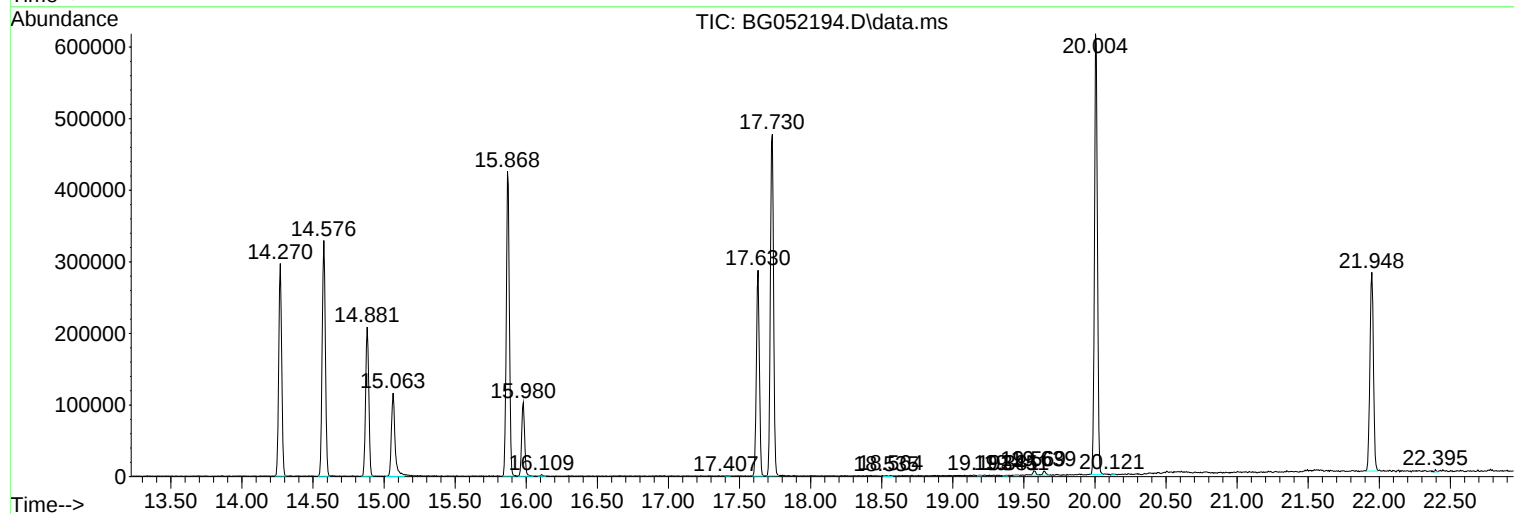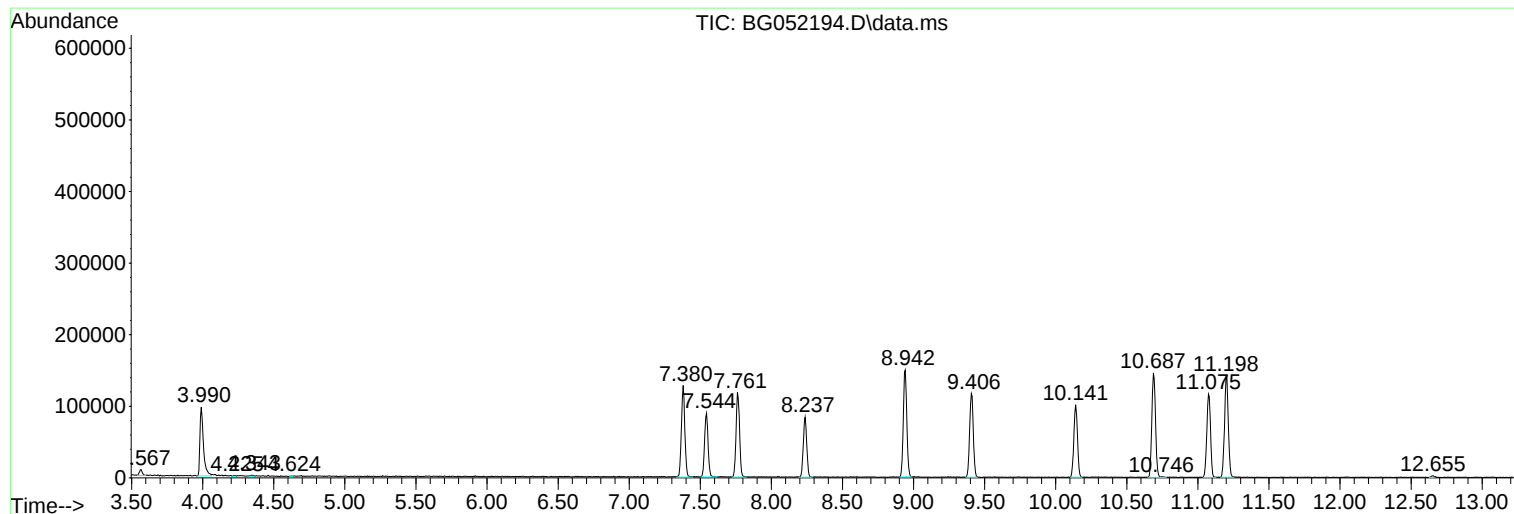

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052194.D
Acq On : 27 Jan 2022 21:06
Operator : CG/JU
Sample : PB142333BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052194.D
Acq On : 27 Jan 2022 21:06
Operator : CG/JU
Sample : PB142333BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc