

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052201.D
 Acq On : 28 Jan 2022 1:30
 Operator : CG/JU
 Sample : N1302-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.566	10	13	18	rVB4	4933	6787	0.73%	0.083%
2	3.995	82	86	95	rBV	35332	61906	6.64%	0.756%
3	4.247	126	129	132	rBV2	1198	1699	0.18%	0.021%
4	4.347	144	146	149	rVB4	1521	1517	0.16%	0.019%
5	5.281	303	305	315	rVB3	2083	3860	0.41%	0.047%
6	5.593	354	358	361	rBV2	1160	1564	0.17%	0.019%
7	6.462	505	506	513	rVB2	1183	1681	0.18%	0.021%
8	7.220	632	635	640	rBV2	1043	1972	0.21%	0.024%
9	7.378	658	662	671	rVB4	22744	41698	4.47%	0.509%
10	7.543	681	690	698	rBV	89770	151639	16.27%	1.851%
11	7.766	721	728	736	rBV	87506	148530	15.94%	1.813%
12	8.236	801	808	816	rBV2	85884	147755	15.86%	1.804%
13	8.941	921	928	937	rBV	70372	117857	12.65%	1.439%
14	9.405	1000	1007	1016	rBV	117851	212734	22.83%	2.597%
15	9.828	1074	1079	1084	rVB	14963	21240	2.28%	0.259%
16	10.139	1125	1132	1139	rVB2	98209	175925	18.88%	2.148%
17	10.692	1219	1226	1234	rBV	136101	242280	26.00%	2.958%
18	10.827	1245	1249	1252	rBV2	2234	2637	0.28%	0.032%
19	11.079	1284	1292	1298	rBV	119277	216418	23.23%	2.642%
20	11.203	1305	1313	1320	rBV	134806	245603	26.36%	2.998%
21	12.325	1497	1504	1510	rVB3	6938	9728	1.04%	0.119%
22	12.466	1525	1528	1531	rBV3	2004	2361	0.25%	0.029%
23	12.654	1553	1560	1565	rBV3	2327	4210	0.45%	0.051%
24	13.488	1696	1702	1707	rBV3	1103	1808	0.19%	0.022%
25	13.693	1733	1737	1743	rBV4	4478	7024	0.75%	0.086%
26	13.776	1746	1751	1754	rVB2	885	1316	0.14%	0.016%
27	14.269	1829	1835	1842	rBV	310594	450646	48.36%	5.502%
28	14.498	1870	1874	1875	rBV2	1640	1256	0.13%	0.015%
29	14.575	1880	1887	1894	rVB	335968	532490	57.14%	6.501%
30	14.757	1913	1918	1921	rBV3	2339	3295	0.35%	0.040%
31	14.880	1933	1939	1947	rBV2	206346	332944	35.73%	4.065%
32	15.068	1965	1971	1978	rBV2	18436	31929	3.43%	0.390%
33	15.503	2041	2045	2050	rVB3	2100	2714	0.29%	0.033%
34	15.573	2050	2057	2061	rBV3	726	1519	0.16%	0.019%
35	15.661	2065	2072	2075	rBV3	2580	5231	0.56%	0.064%
36	15.702	2076	2079	2083	rVB2	2408	2662	0.29%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052201.D
 Acq On : 28 Jan 2022 1:30
 Operator : CG/JU
 Sample : N1302-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0F31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	15.873	2101	2108	2120	rVB	439645	680806	73.06%	8.312%
38	15.979	2120	2126	2134	rBV2	119689	168731	18.11%	2.060%
39	16.114	2144	2149	2151	rBV	2975	3332	0.36%	0.041%
40	16.537	2219	2221	2222	rBV2	1621	1309	0.14%	0.016%
41	16.566	2222	2226	2228	rVB3	1412	1765	0.19%	0.022%
42	16.642	2238	2239	2243	rVB	1144	1290	0.14%	0.016%
43	16.907	2280	2284	2287	rBV2	1478	1902	0.20%	0.023%
44	17.083	2313	2314	2319	rVB	1468	1508	0.16%	0.018%
45	17.359	2358	2361	2366	rVB5	2741	3899	0.42%	0.048%
46	17.418	2366	2371	2375	rBV2	2573	3896	0.42%	0.048%
47	17.518	2384	2388	2391	rBV4	4696	5820	0.62%	0.071%
48	17.629	2401	2407	2414	rBV	278805	420862	45.17%	5.138%
49	17.729	2417	2424	2434	rVV	516803	802145	86.08%	9.793%
50	17.805	2434	2437	2440	rVB3	1678	2353	0.25%	0.029%
51	17.841	2440	2443	2445	rBV	1248	1263	0.14%	0.015%
52	18.023	2471	2474	2480	rVB3	1941	2336	0.25%	0.029%
53	18.105	2484	2488	2491	rBV3	1362	2068	0.22%	0.025%
54	18.228	2506	2509	2512	rVV	1173	1402	0.15%	0.017%
55	18.270	2512	2516	2523	rVB4	3261	4855	0.52%	0.059%
56	18.499	2551	2555	2558	rVB3	1492	2441	0.26%	0.030%
57	18.687	2586	2587	2592	rVB4	1511	1809	0.19%	0.022%
58	18.787	2602	2604	2608	rBV3	2567	2881	0.31%	0.035%
59	18.916	2623	2626	2630	rVB3	6340	7125	0.76%	0.087%
60	19.021	2638	2644	2646	rBV6	1859	2981	0.32%	0.036%
61	19.145	2663	2665	2668	rVB3	1873	1914	0.21%	0.023%
62	19.245	2678	2682	2683	rBV2	1255	1413	0.15%	0.017%
63	19.350	2698	2700	2704	rBV3	3545	4167	0.45%	0.051%
64	19.409	2708	2710	2711	rBV2	1860	1355	0.15%	0.017%
65	19.486	2721	2723	2724	rBV2	3411	2301	0.25%	0.028%
66	19.574	2736	2738	2741	rVB2	8420	7025	0.75%	0.086%
67	20.008	2806	2812	2819	rVB	655128	931832	100.00%	11.376%
68	20.173	2838	2840	2842	rBV2	1713	1531	0.16%	0.019%
69	20.666	2921	2924	2927	rBV5	2296	4265	0.46%	0.052%
70	20.948	2970	2972	2976	rVB5	2686	2266	0.24%	0.028%
71	21.553	3071	3075	3084	rBV7	9362	23729	2.55%	0.290%
72	21.947	3135	3142	3150	rVB	264208	459226	49.28%	5.606%
73	24.408	3559	3561	3567	rVB7	7587	12691	1.36%	0.155%
74	25.190	3683	3694	3706	rBV2	309378	900103	96.59%	10.989%
75	25.430	3724	3735	3747	rBV2	157187	472107	50.66%	5.764%
76	26.699	3944	3951	3960	rVB7	8967	28366	3.04%	0.346%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052201.D
Acq On : 28 Jan 2022 1:30
Operator : CG/JU
Sample : N1302-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F31

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

77	27.134	4024	4025	4027	rVB2	3454	1490	0.16%	0.018%
78	28.497	4255	4257	4258	rBV	4493	3280	0.35%	0.040%
79	31.411	4751	4753	4754	rVB	3370	2065	0.22%	0.025%
80	31.428	4754	4756	4758	rBV3	2785	2178	0.23%	0.027%
81	32.403	4920	4922	4925	rVB4	3479	2574	0.28%	0.031%




Sum of corrected areas: 8191092

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052201.D
Acq On : 28 Jan 2022 1:30
Operator : CG/JU
Sample : N1302-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F31

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

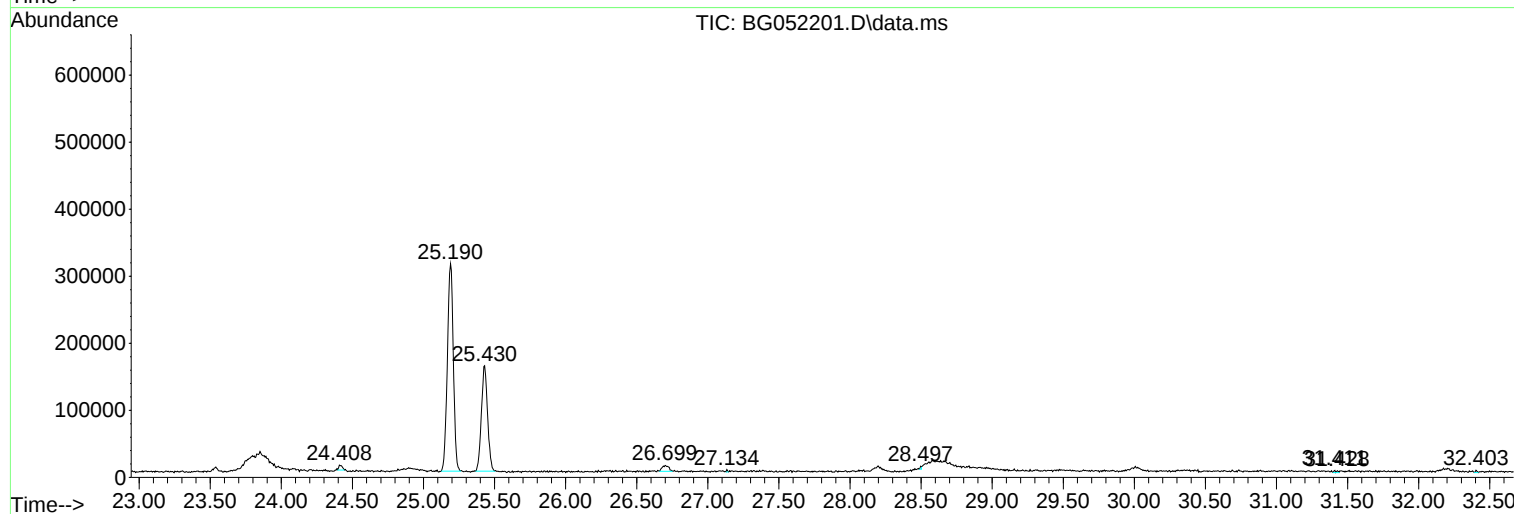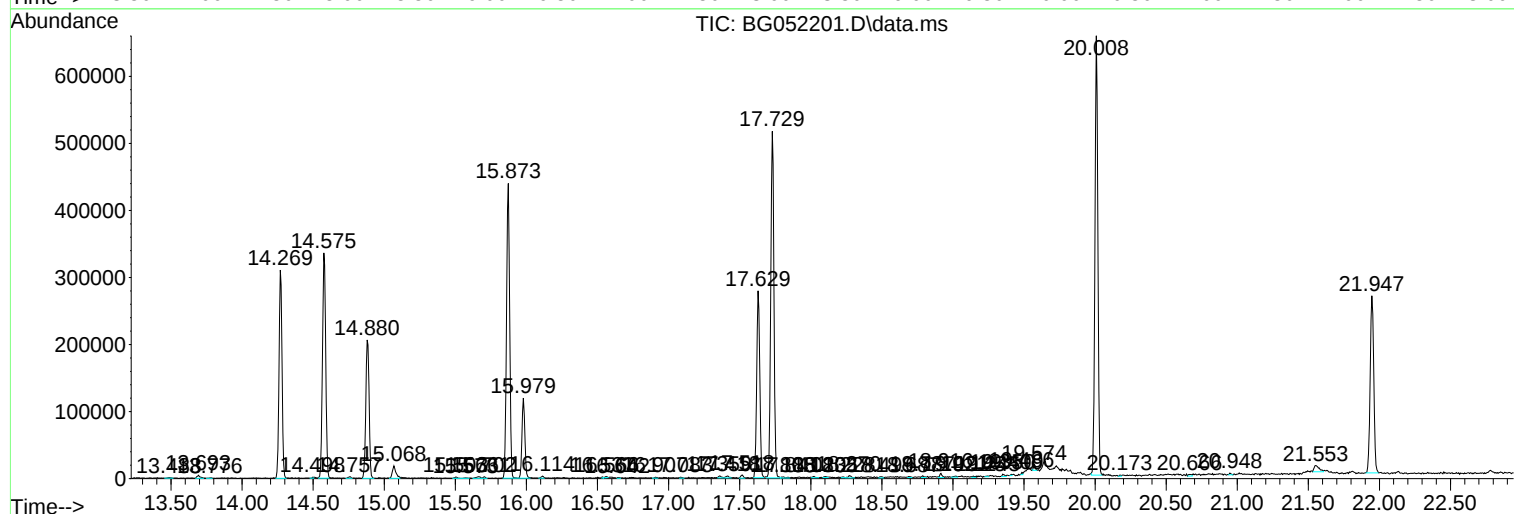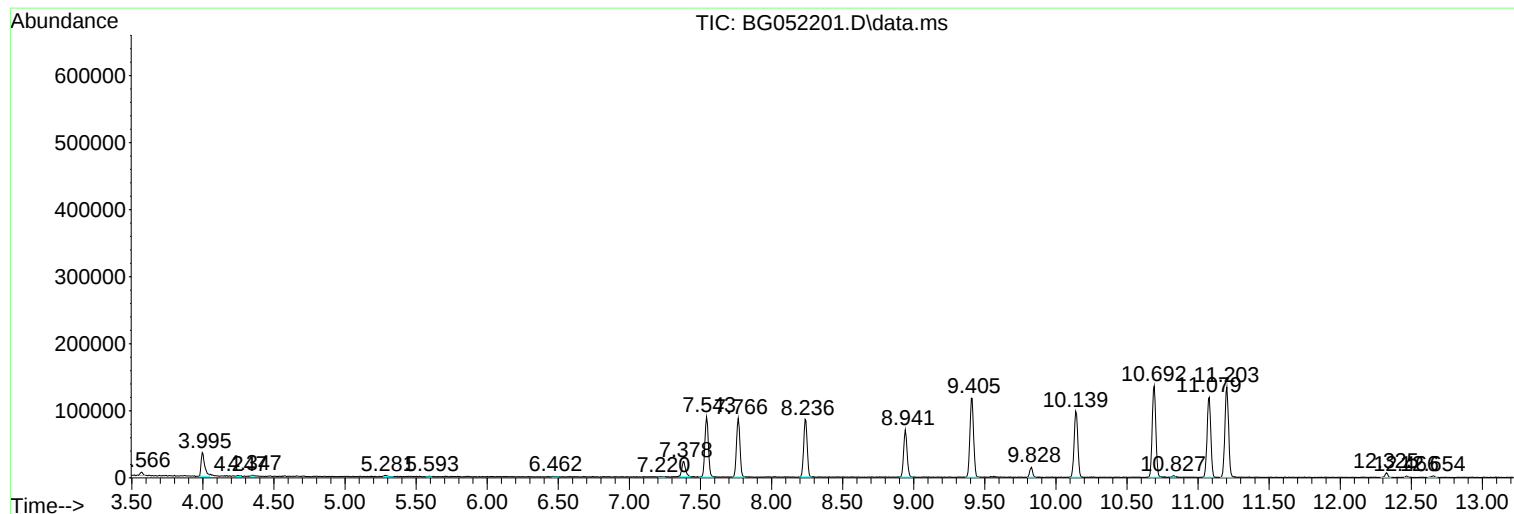

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052201.D
Acq On : 28 Jan 2022 1:30
Operator : CG/JU
Sample : N1302-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F31

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052201.D
Acq On : 28 Jan 2022 1:30
Operator : CG/JU
Sample : N1302-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0F31

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc