

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052210.D
 Acq On : 28 Jan 2022 10:27
 Operator : CG/JU
 Sample : N1273-05DL 10X
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HK4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052210.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.543	3	9	15	rBV	104007	182452	28.63%	4.624%
2	3.601	15	19	32	rVB	29413	48976	7.69%	1.241%
3	3.731	39	41	42	rVB2	1099	712	0.11%	0.018%
4	3.989	83	85	87	rBV2	906	862	0.14%	0.022%
5	4.018	87	90	96	rVV4	2622	4266	0.67%	0.108%
6	4.171	114	116	117	rVB2	1676	897	0.14%	0.023%
7	4.195	117	120	123	rBV2	1233	1335	0.21%	0.034%
8	4.271	131	133	137	rBV3	929	1431	0.22%	0.036%
9	4.441	160	162	165	rBV2	1199	1379	0.22%	0.035%
10	4.618	190	192	193	rBV	972	733	0.12%	0.019%
11	4.776	216	219	220	rBV2	993	819	0.13%	0.021%
12	4.894	233	239	250	rVB	164077	274477	43.07%	6.956%
13	5.276	301	304	307	rBV	626	973	0.15%	0.025%
14	5.375	319	321	323	rBV	1084	778	0.12%	0.020%
15	5.528	345	347	350	rVB2	1193	1132	0.18%	0.029%
16	5.558	350	352	353	rBV	997	717	0.11%	0.018%
17	5.628	361	364	370	rVB3	3010	4312	0.68%	0.109%
18	5.699	373	376	379	rVV2	852	1088	0.17%	0.028%
19	5.751	382	385	386	rBV	1592	1063	0.17%	0.027%
20	5.916	410	413	414	rBV	1055	696	0.11%	0.018%
21	6.403	493	496	498	rVB2	1134	1243	0.20%	0.031%
22	6.603	528	530	535	rBV2	689	1066	0.17%	0.027%
23	6.715	548	549	553	rVB	883	731	0.11%	0.019%
24	7.390	658	664	671	rVB3	2330	4691	0.74%	0.119%
25	7.543	684	690	697	rVB3	10632	17240	2.71%	0.437%
26	7.719	717	720	723	rBV	644	720	0.11%	0.018%
27	7.760	723	727	734	rVB3	8762	15220	2.39%	0.386%
28	8.236	801	808	816	rVB	106844	179329	28.14%	4.544%
29	8.941	922	928	934	rBV4	7053	11545	1.81%	0.293%
30	9.411	1001	1008	1016	rVB	13256	23962	3.76%	0.607%
31	10.140	1127	1132	1138	rVB2	8635	14725	2.31%	0.373%
32	10.210	1142	1144	1149	rVB2	466	711	0.11%	0.018%
33	10.692	1220	1226	1235	rBV3	12203	22872	3.59%	0.580%
34	11.074	1284	1291	1299	rBV	150353	271733	42.64%	6.886%
35	11.203	1308	1313	1322	rVB2	12295	20542	3.22%	0.521%
36	11.450	1352	1355	1359	rBV2	421	779	0.12%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052210.D
 Acq On : 28 Jan 2022 10:27
 Operator : CG/JU
 Sample : N1273-05DL 10X
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HK4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	12.859	1593	1595	1599	rVB	658	763	0.12%	0.019%
38	13.741	1741	1745	1747	rVB	914	1257	0.20%	0.032%
39	14.269	1829	1835	1840	rBV	36813	52783	8.28%	1.338%
40	14.487	1866	1872	1881	rBV5	7132	16608	2.61%	0.421%
41	14.575	1881	1887	1893	rVB	42345	64353	10.10%	1.631%
42	14.669	1901	1903	1906	rBV2	797	890	0.14%	0.023%
43	14.804	1925	1926	1930	rBV2	721	999	0.16%	0.025%
44	14.880	1932	1939	1947	rVV	276322	422626	66.32%	10.710%
45	15.074	1968	1972	1973	rBV	804	693	0.11%	0.018%
46	15.362	2019	2021	2025	rVB	811	829	0.13%	0.021%
47	15.556	2051	2054	2056	rBV2	638	796	0.12%	0.020%
48	15.638	2067	2068	2071	rBV	655	728	0.11%	0.018%
49	15.867	2101	2107	2115	rVB	53222	82599	12.96%	2.093%
50	15.985	2122	2127	2133	rBV2	3540	4800	0.75%	0.122%
51	16.284	2177	2178	2183	rBV2	796	961	0.15%	0.024%
52	16.554	2219	2224	2225	rVB	758	716	0.11%	0.018%
53	17.007	2299	2301	2305	rBV2	548	812	0.13%	0.021%
54	17.124	2317	2321	2323	rBV3	521	777	0.12%	0.020%
55	17.248	2341	2342	2345	rVB	884	737	0.12%	0.019%
56	17.359	2356	2361	2362	rBV	691	918	0.14%	0.023%
57	17.412	2367	2370	2374	rVB3	1373	2216	0.35%	0.056%
58	17.629	2400	2407	2417	rVV	363835	537867	84.41%	13.630%
59	17.729	2417	2424	2431	rVV2	62004	99150	15.56%	2.513%
60	17.782	2431	2433	2436	rVB3	644	692	0.11%	0.018%
61	17.976	2463	2466	2468	rBV2	538	713	0.11%	0.018%
62	18.487	2550	2553	2557	rBV	591	890	0.14%	0.023%
63	18.740	2593	2596	2599	rBV2	693	1035	0.16%	0.026%
64	19.362	2701	2702	2705	rBV	821	846	0.13%	0.021%
65	19.644	2748	2750	2753	rBV3	1046	800	0.13%	0.020%
66	19.715	2757	2762	2763	rBV2	974	1362	0.21%	0.035%
67	19.779	2772	2773	2775	rBV2	1218	759	0.12%	0.019%
68	19.903	2790	2794	2798	rBV4	4749	6464	1.01%	0.164%
69	19.938	2798	2800	2802	rVV2	1034	982	0.15%	0.025%
70	20.009	2806	2812	2818	rVB	81211	116517	18.28%	2.953%
71	20.314	2862	2864	2866	rBV3	1390	1345	0.21%	0.034%
72	20.338	2866	2868	2870	rVB3	1773	1426	0.22%	0.036%
73	20.361	2870	2872	2873	rBV2	1300	766	0.12%	0.019%
74	20.420	2880	2882	2885	rBV3	1389	1262	0.20%	0.032%
75	20.502	2894	2896	2899	rBV3	1340	1362	0.21%	0.035%
76	20.631	2916	2918	2919	rBV2	1420	838	0.13%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
 Data File : BG052210.D
 Acq On : 28 Jan 2022 10:27
 Operator : CG/JU
 Sample : N1273-05DL 10X
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HK4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	20.749	2936	2938	2940	rVB3	1342	827	0.13%	0.021%
78	20.772	2940	2942	2944	rBV3	1747	1341	0.21%	0.034%
79	20.884	2959	2961	2965	rBV3	2054	2777	0.44%	0.070%
80	21.013	2981	2983	2988	rBV5	2026	2939	0.46%	0.074%
81	21.853	3124	3126	3127	rBV2	2550	1696	0.27%	0.043%
82	21.947	3135	3142	3149	rBV	338900	583341	91.54%	14.782%
83	22.123	3170	3172	3178	rVB6	4193	5649	0.89%	0.143%
84	22.347	3208	3210	3211	rBV2	1915	1126	0.18%	0.029%
85	22.787	3281	3285	3288	rVB4	5343	7381	1.16%	0.187%
86	22.840	3292	3294	3295	rBV	2234	1208	0.19%	0.031%
87	23.533	3407	3412	3418	rVB5	8171	16855	2.65%	0.427%
88	24.408	3558	3561	3568	rVB3	11550	22672	3.56%	0.575%
89	25.178	3684	3692	3706	rVB3	36204	104684	16.43%	2.653%
90	25.425	3724	3734	3749	rVB2	201031	637239	100.00%	16.148%
91	26.629	3937	3939	3941	rBV3	2631	2401	0.38%	0.061%
92	27.040	4008	4009	4013	rBV3	2489	2243	0.35%	0.057%
93	27.128	4022	4024	4025	rBV2	2448	1506	0.24%	0.038%
94	31.986	4850	4851	4852	rBV	3010	1152	0.18%	0.029%




Sum of corrected areas: 3946181

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052210.D
Acq On : 28 Jan 2022 10:27
Operator : CG/JU
Sample : N1273-05DL 10X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HK4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

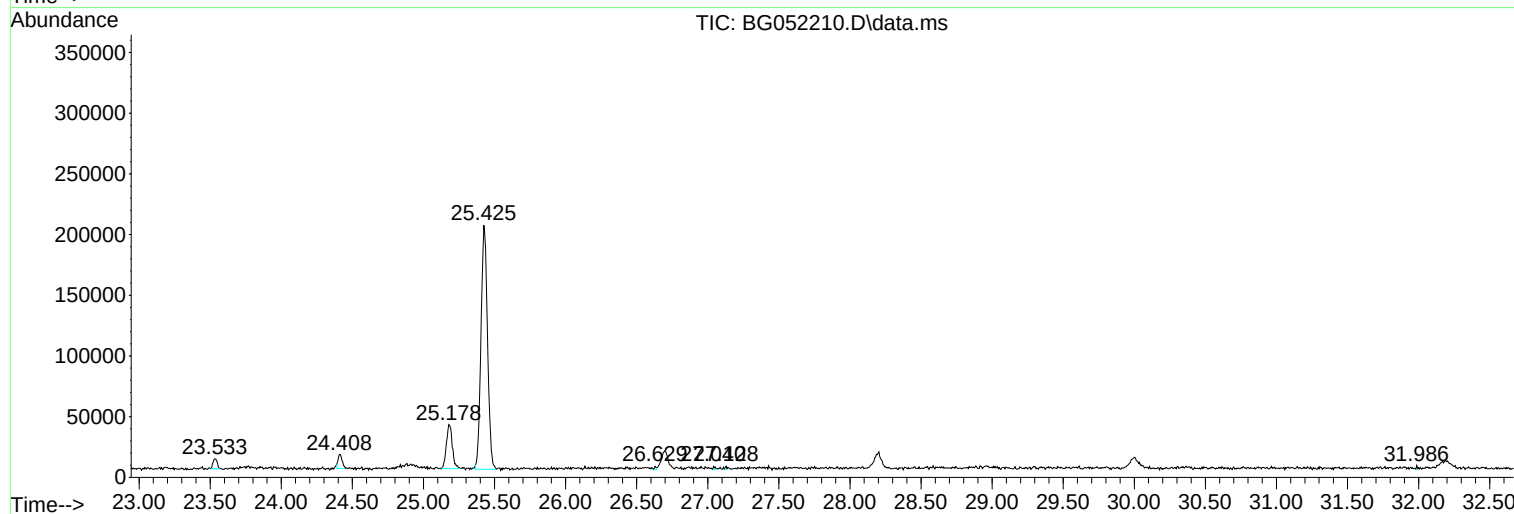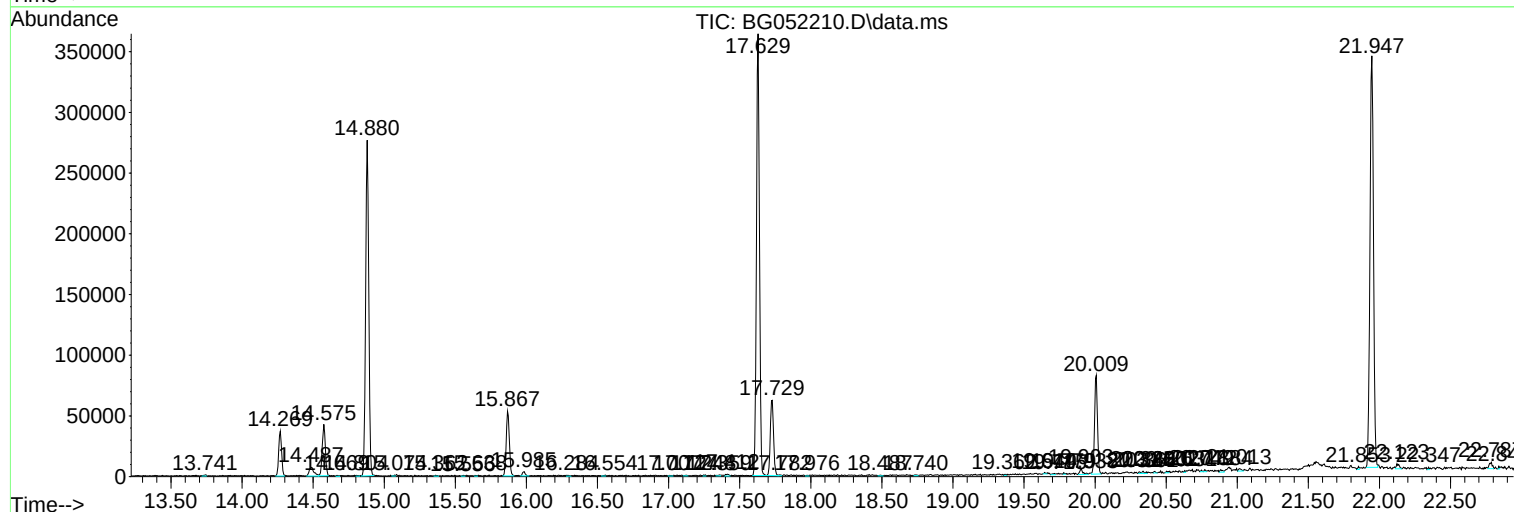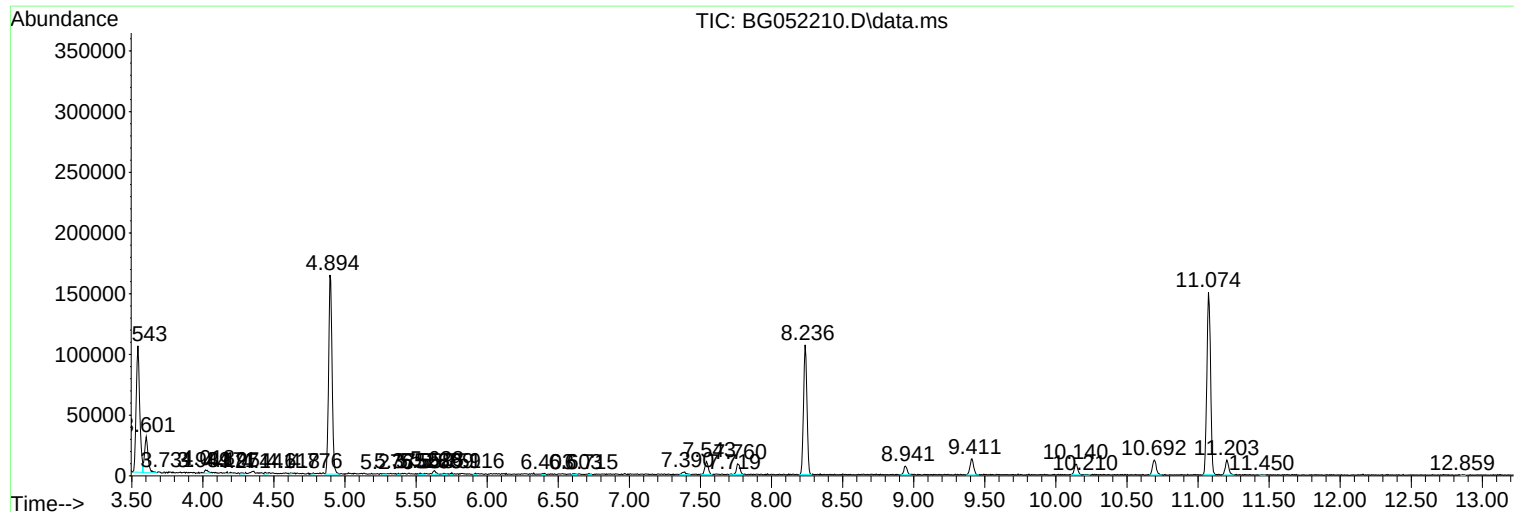

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052210.D
Acq On : 28 Jan 2022 10:27
Operator : CG/JU
Sample : N1273-05DL 10X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HK4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012622\
Data File : BG052210.D
Acq On : 28 Jan 2022 10:27
Operator : CG/JU
Sample : N1273-05DL 10X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HK4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc