
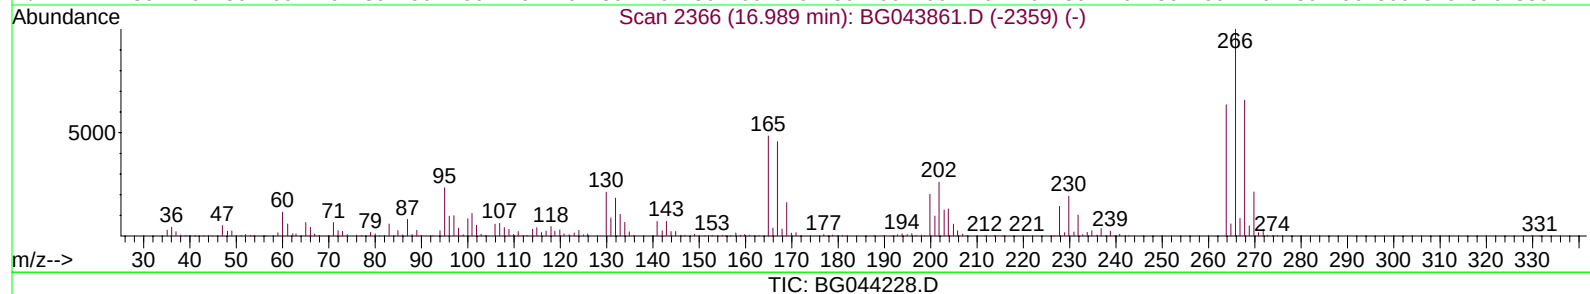
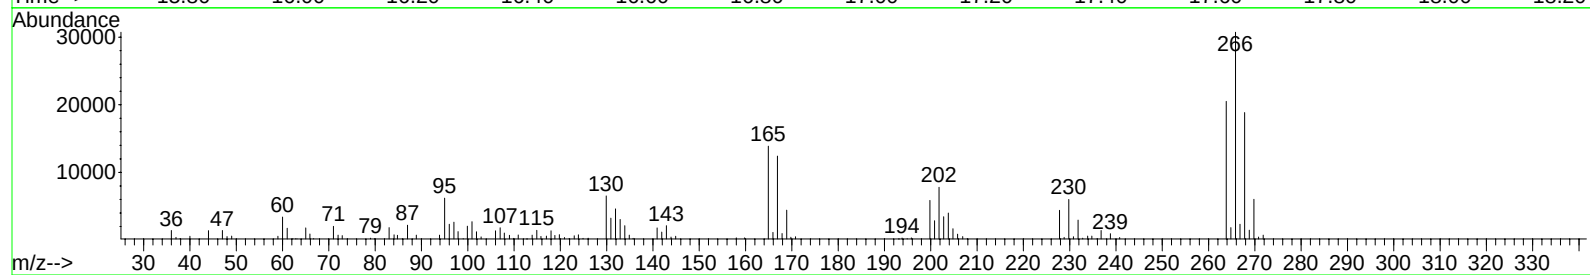


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012820\
Data File : BG044228.D
Acq On : 28 Jan 2020 10:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 18:00:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 28 15:57:24 2020
Response via : Initial Calibration

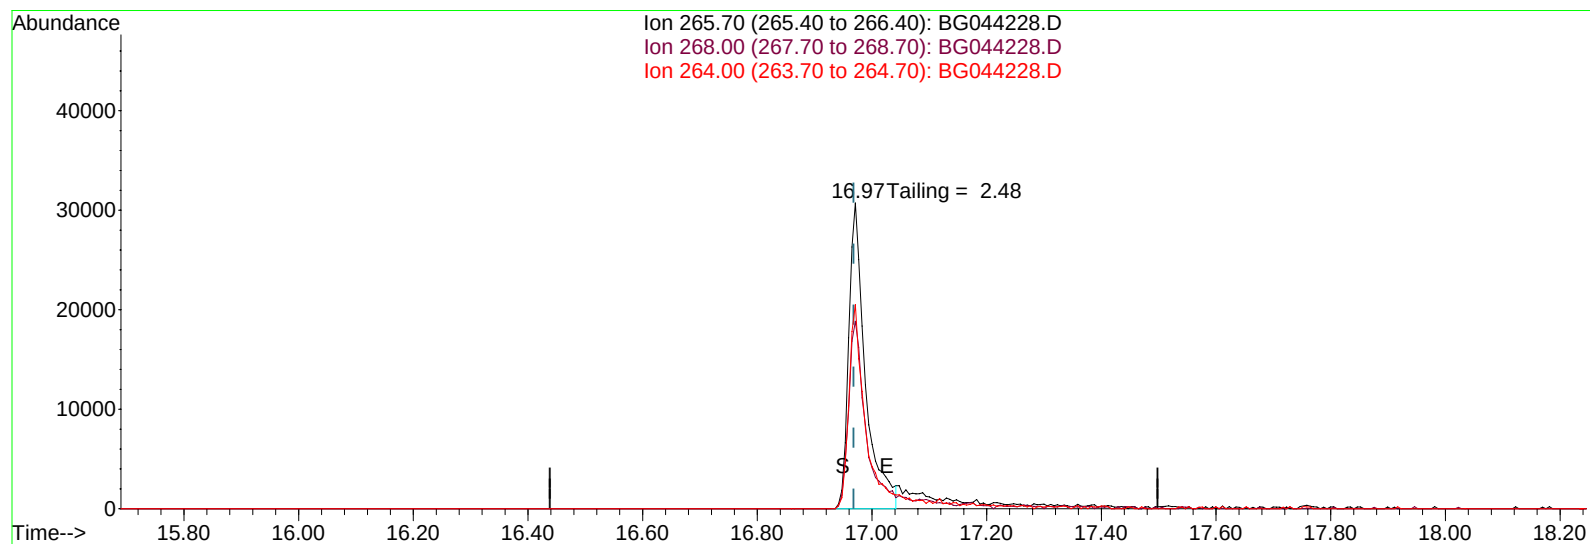

(70) Pentachlorophenol (C)




16.971min (+0.003) 17741.24ng

response 65898

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	61.31
264.00	63.00	66.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012820\
Data File : BG044228.D
Acq On : 28 Jan 2020 10:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 18:00:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 28 15:57:24 2020
Response via : Initial Calibration

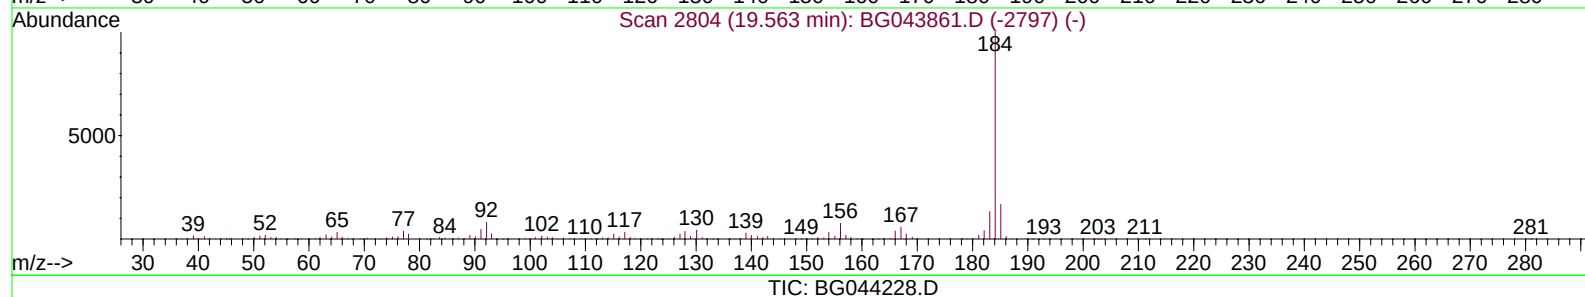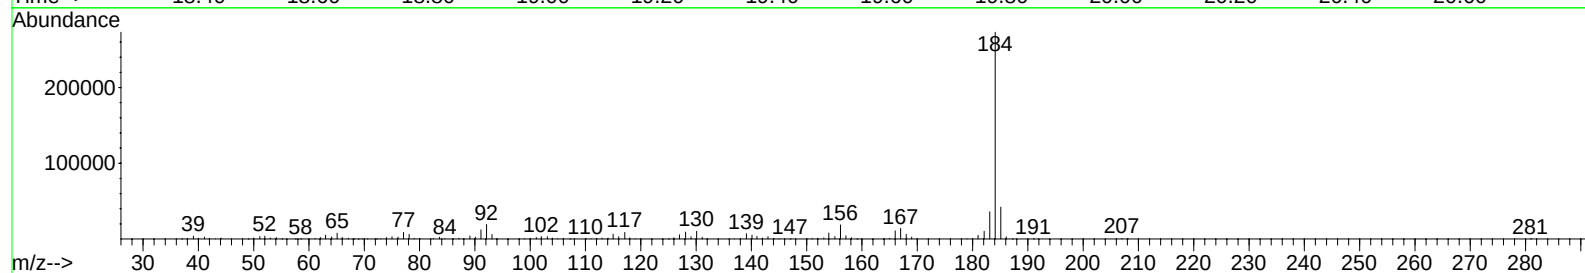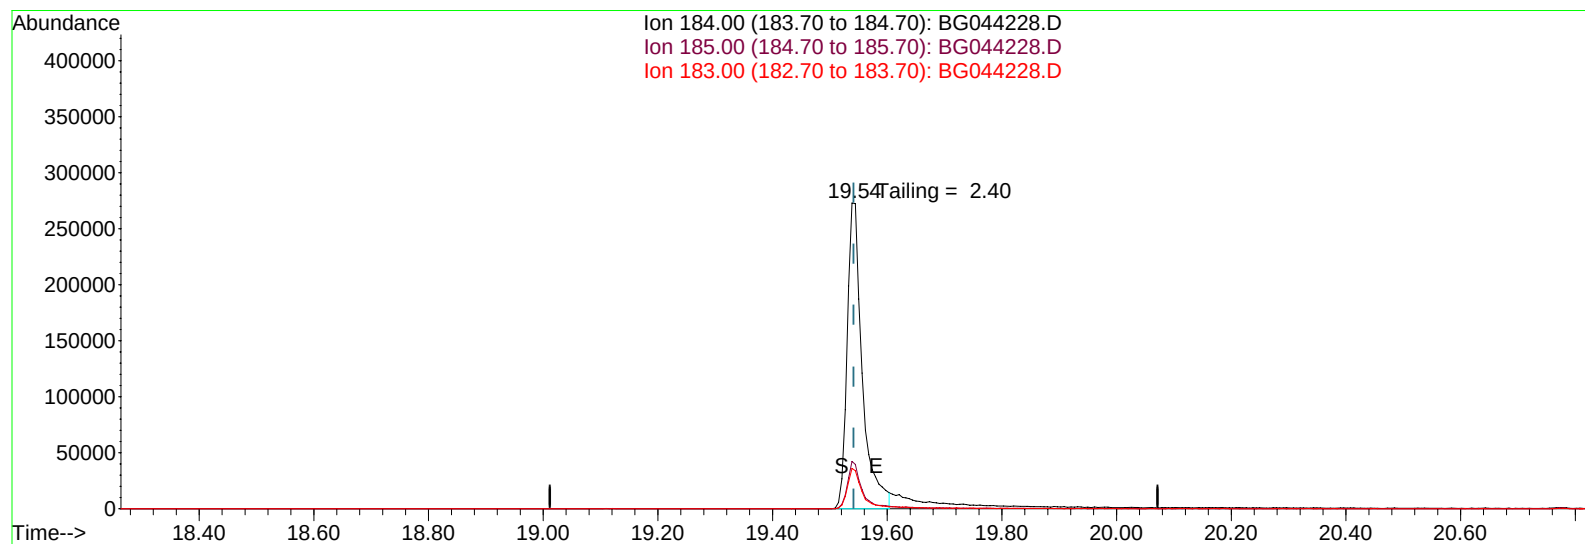

(77) Benzidine

19.539min (-0.003) 0.00ng

response 538336

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.49
183.00	13.10	13.20
0.00	0.00	0.00