


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012820\
 Data File : BG044228.D
 Acq On : 28 Jan 2020 10:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 28 15:57:24 2020

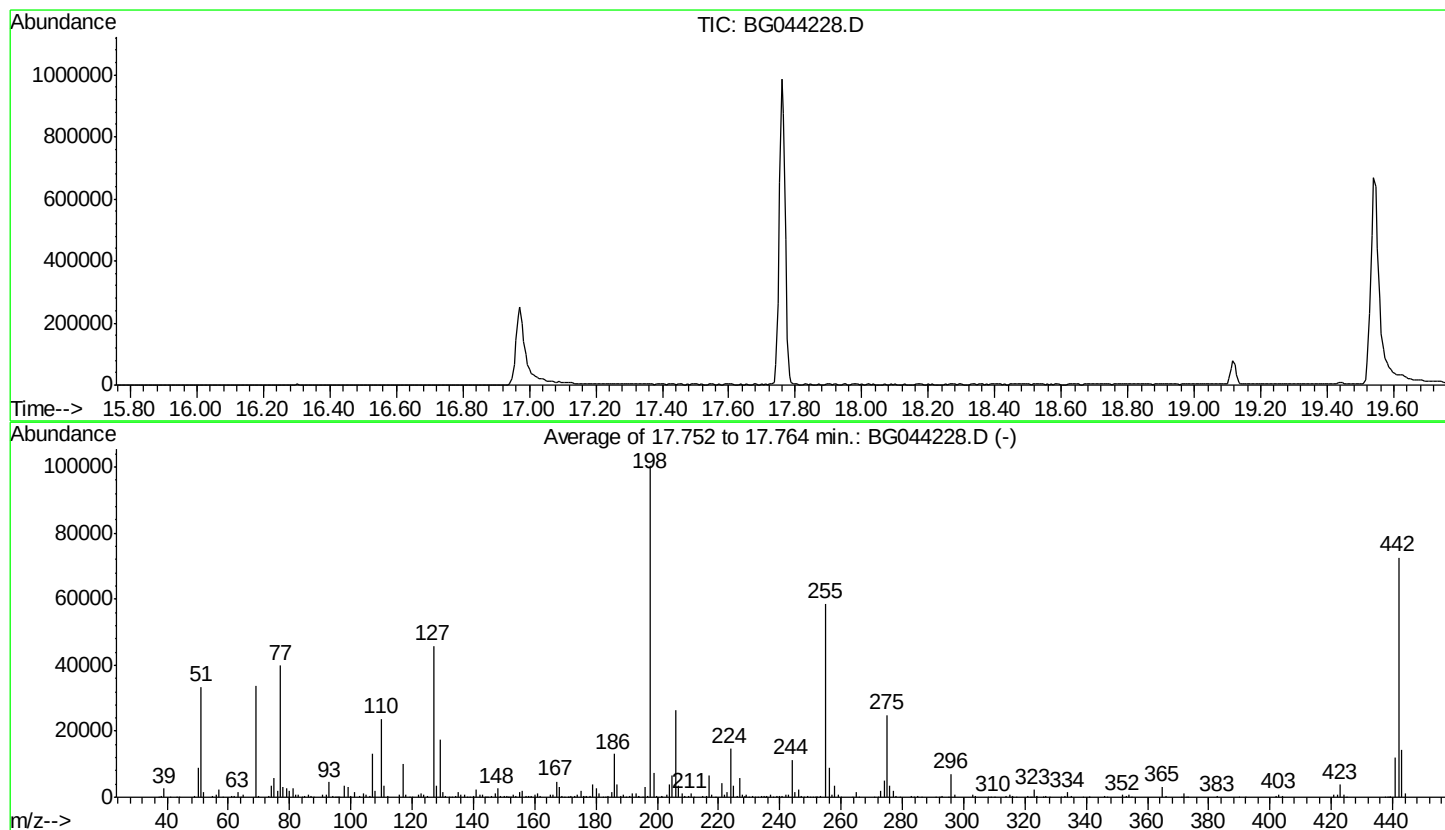

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	33501	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.7	33874	PASS
70	69	0.00	2	0.7	227	PASS
127	198	10	80	45.7	45874	PASS
197	198	0.00	2	0.3	254	PASS
198	198	100	100	100.0	100456	PASS
199	198	5	9	7.5	7533	PASS
275	198	10	60	24.7	24848	PASS
365	198	1	100	3.2	3222	PASS
441	198	0.01	100	12.1	12158	PASS
442	198	50	100	72.2	72520	PASS
443	442	15	24	19.8	14341	PASS