
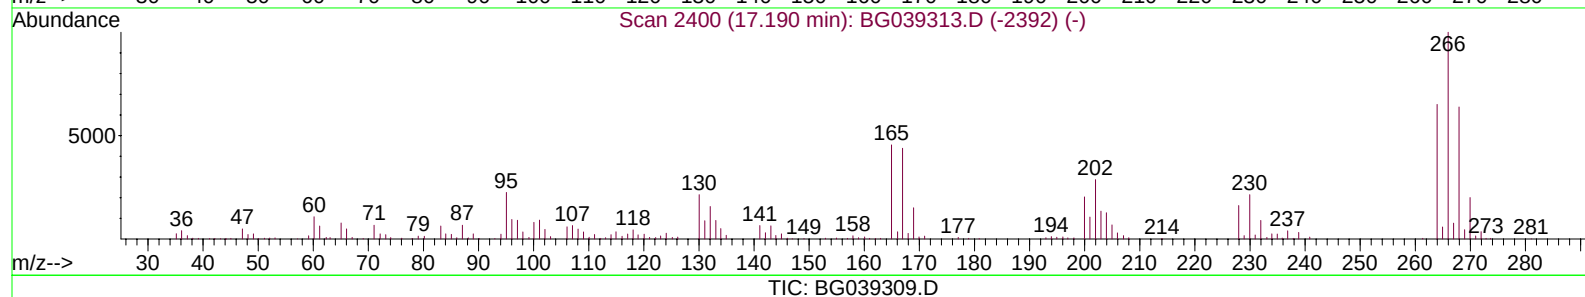
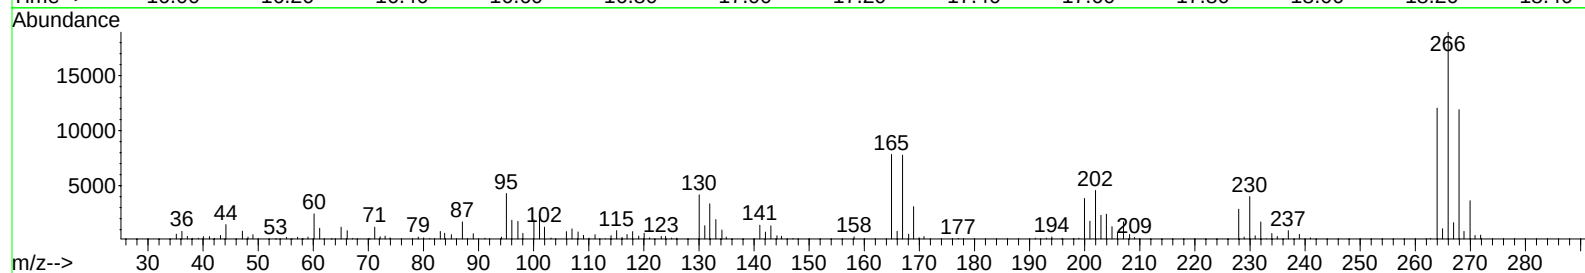


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012919\
Data File : BG039309.D
Acq On : 29 Jan 2019 8:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 17:07:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

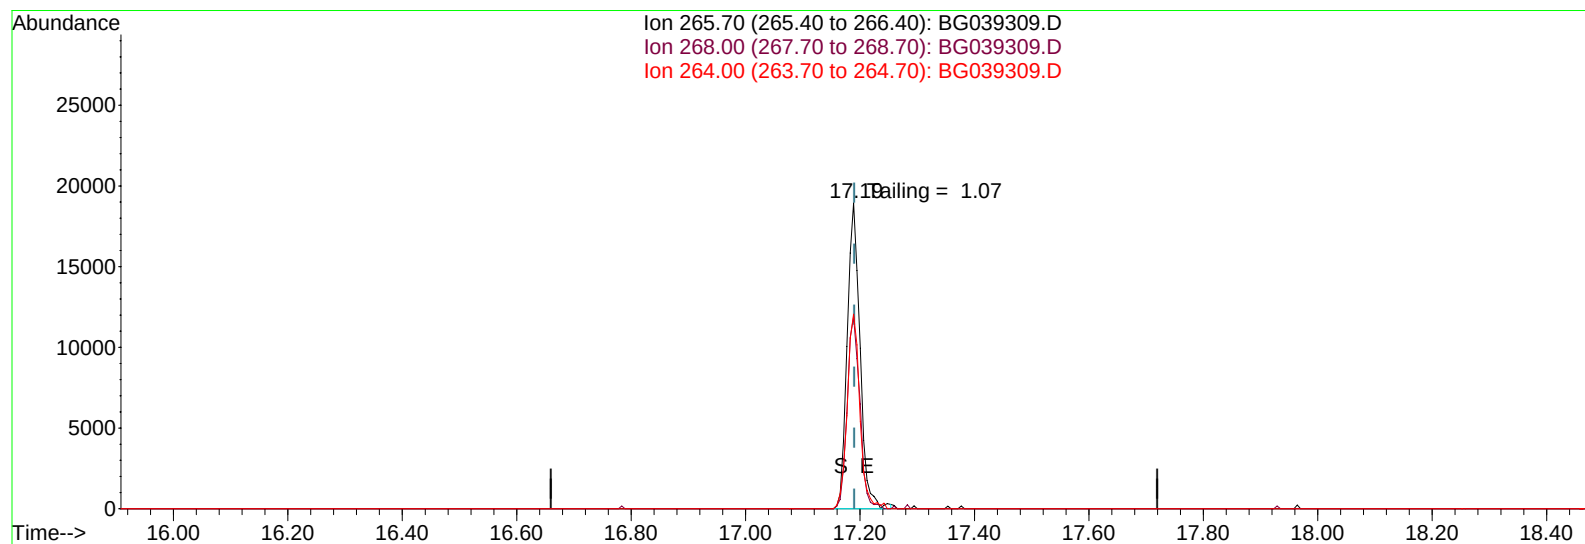

(70) Pentachlorophenol (C)




17.189min (-0.001) 28007.96ng

response 29250

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.87
264.00	65.10	63.63
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012919\  
Data File  : BG039309.D  
Acq On     : 29 Jan 2019      8:55  
Operator   : JU/SJ  
Sample     : DFTPP  
Misc       :  
ALS Vial   : 1      Sample Multiplier: 1
```

Quant Time: Jan 29 17:07:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

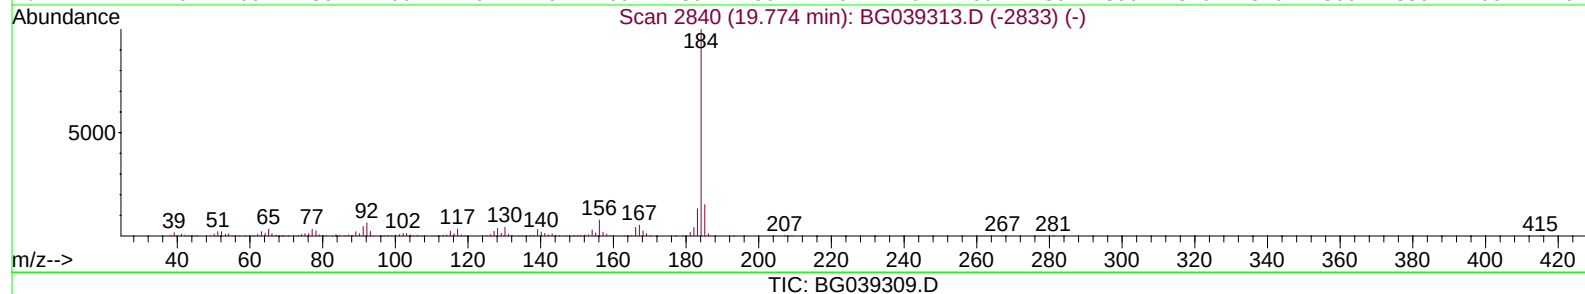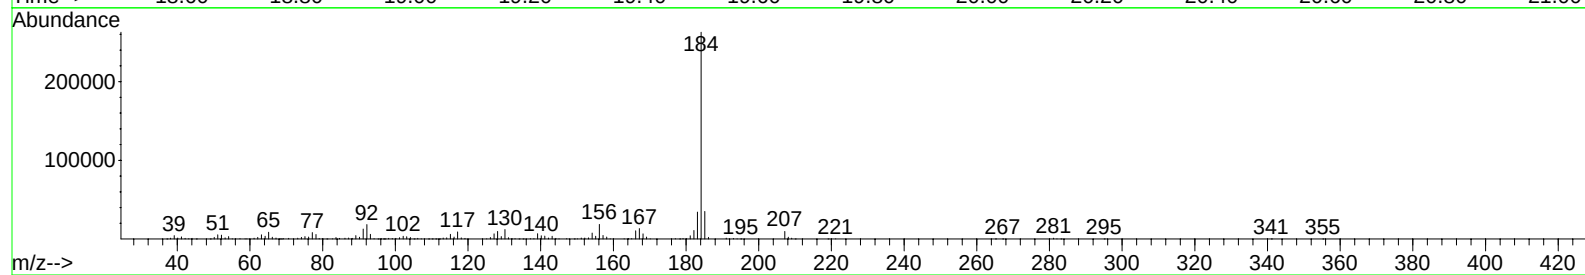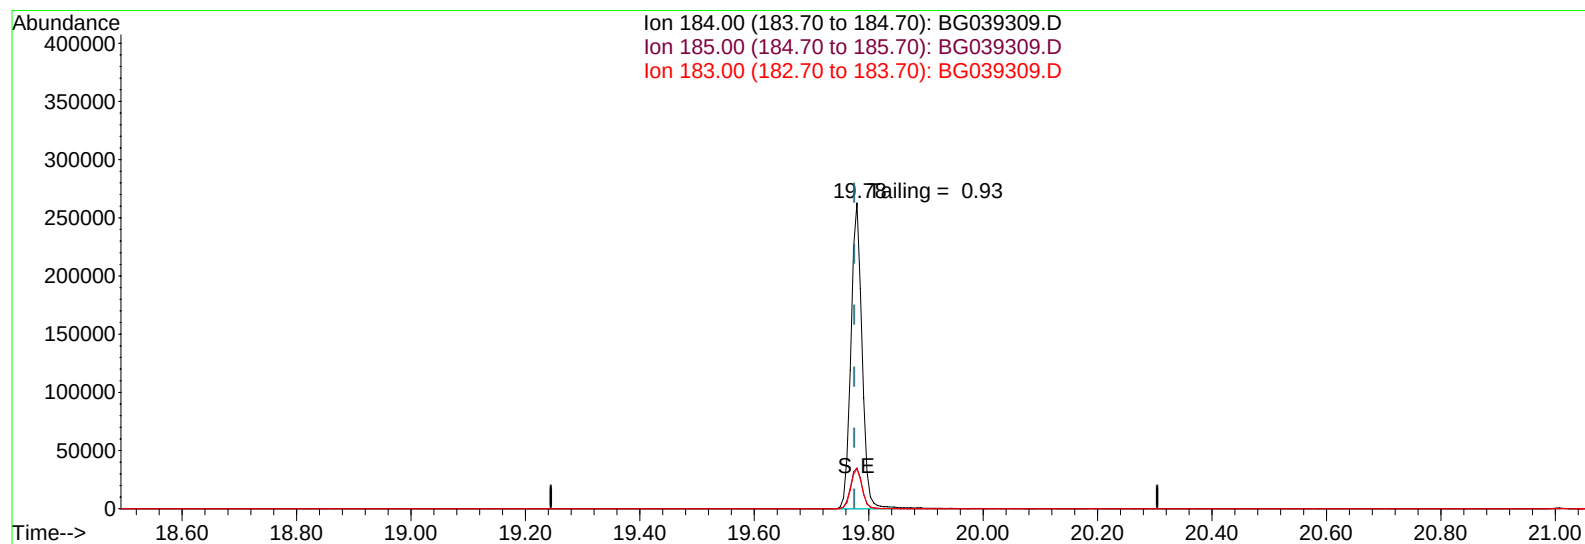

(77) Benzidine

19.779min (+0.005) 0.00ng

response 355583

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.33
183.00	13.20	13.06
0.00	0.00	0.00