
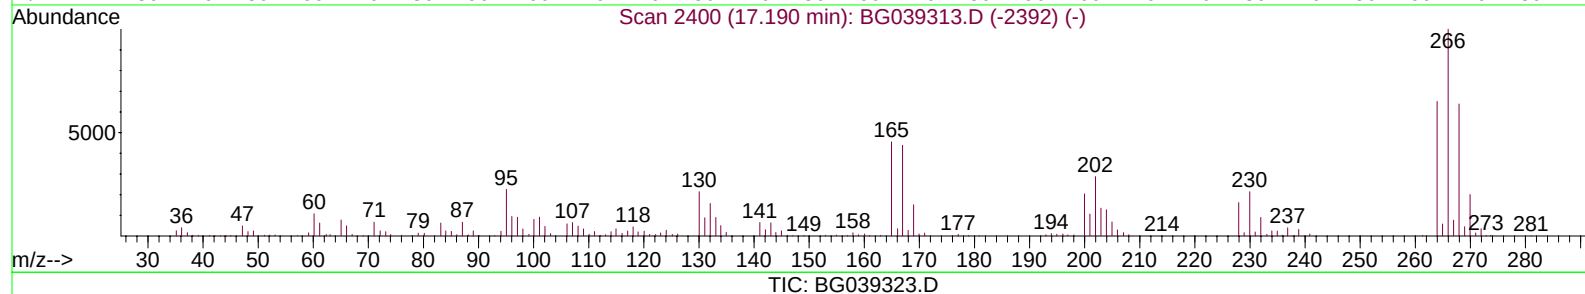
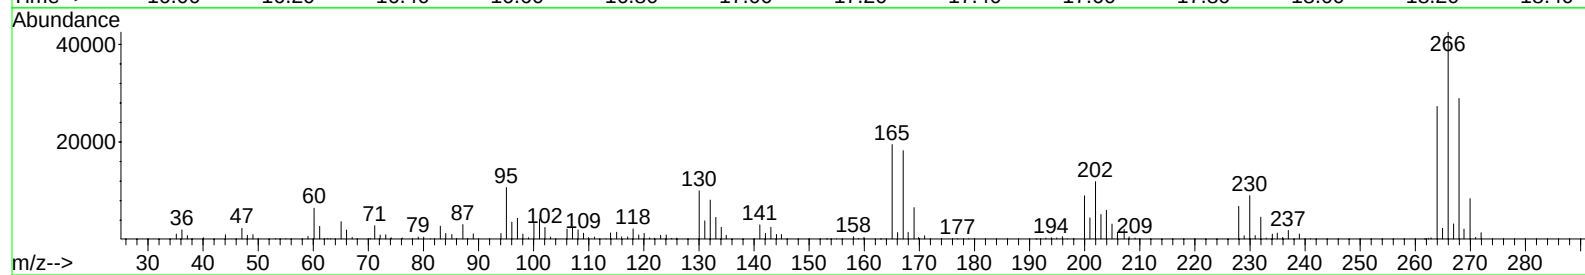


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG013019\
Data File : BG039323.D
Acq On : 30 Jan 2019 11:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 18:07:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

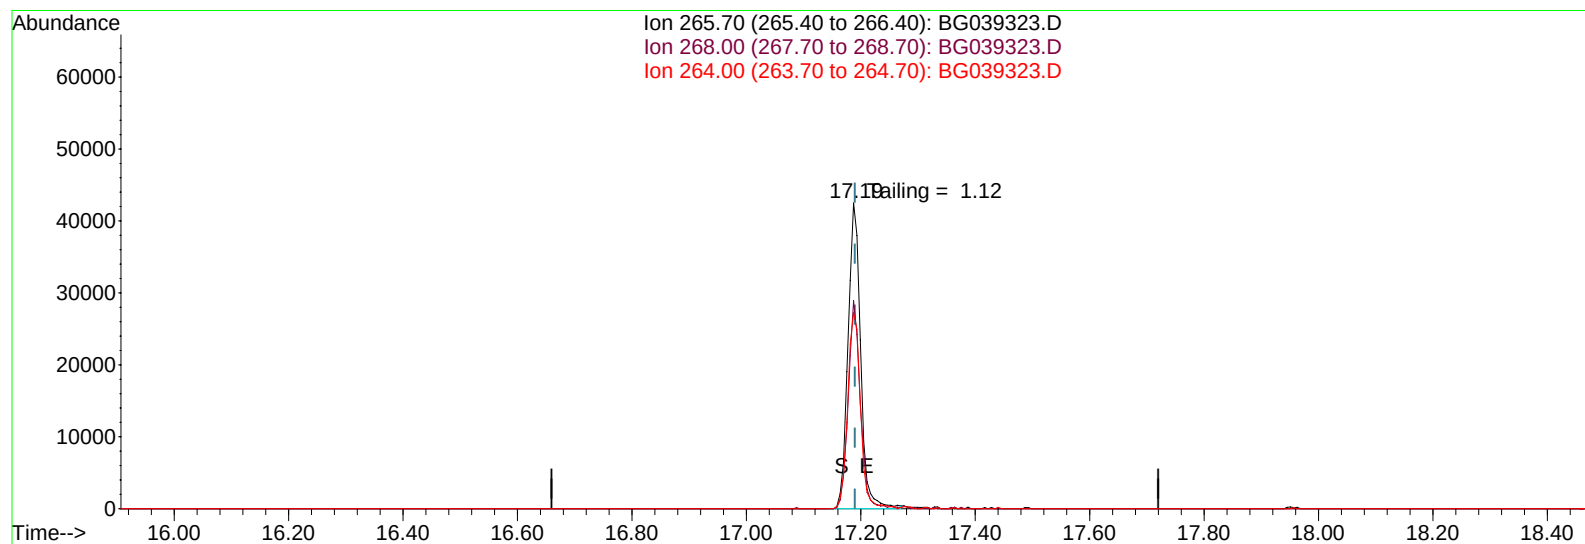

(70) Pentachlorophenol (C)




17.187min (-0.002) 25969.96ng

response 64891

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.05
264.00	65.10	64.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG013019\
Data File : BG039323.D
Acq On : 30 Jan 2019 11:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 18:07:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

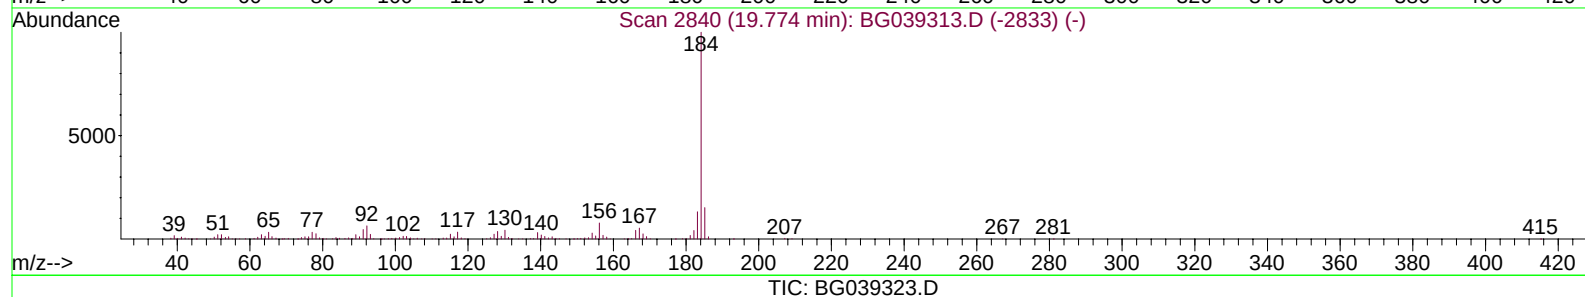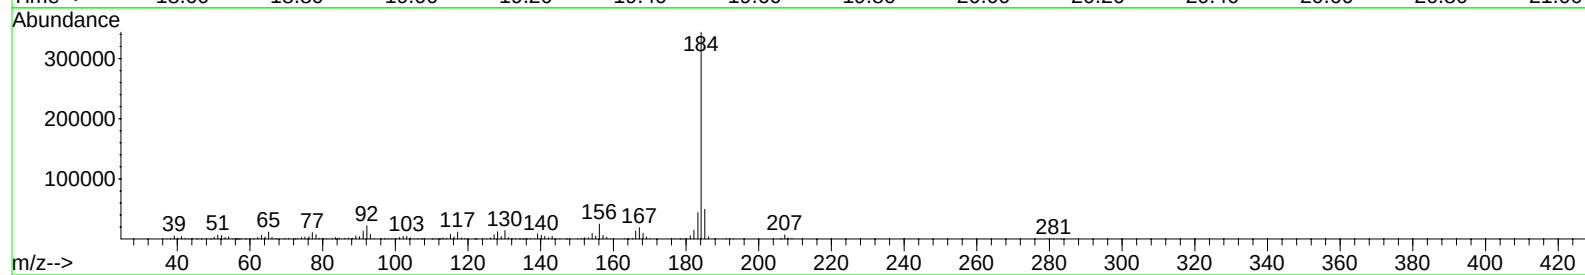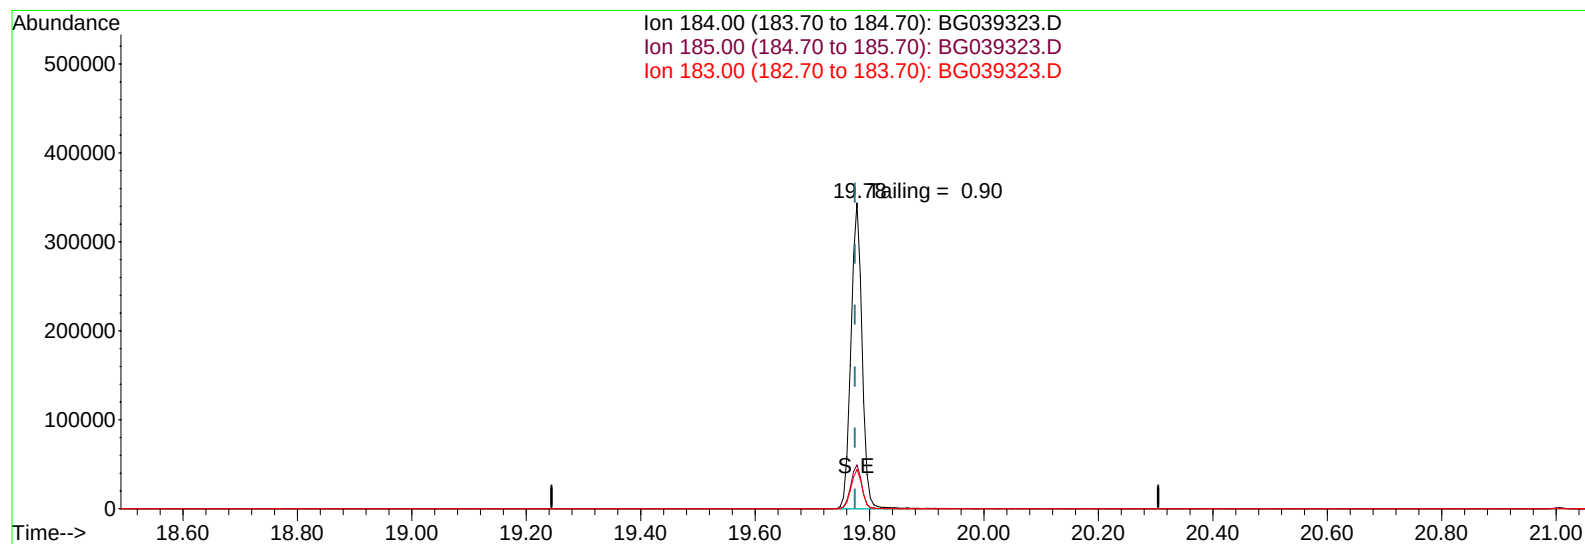

(77) Benzidine

19.778min (+0.004) 109241.60ng

response 462020

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.35
183.00	13.20	12.82
0.00	0.00	0.00