


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG013019\
 Data File : BG039323.D
 Acq On : 30 Jan 2019 11:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

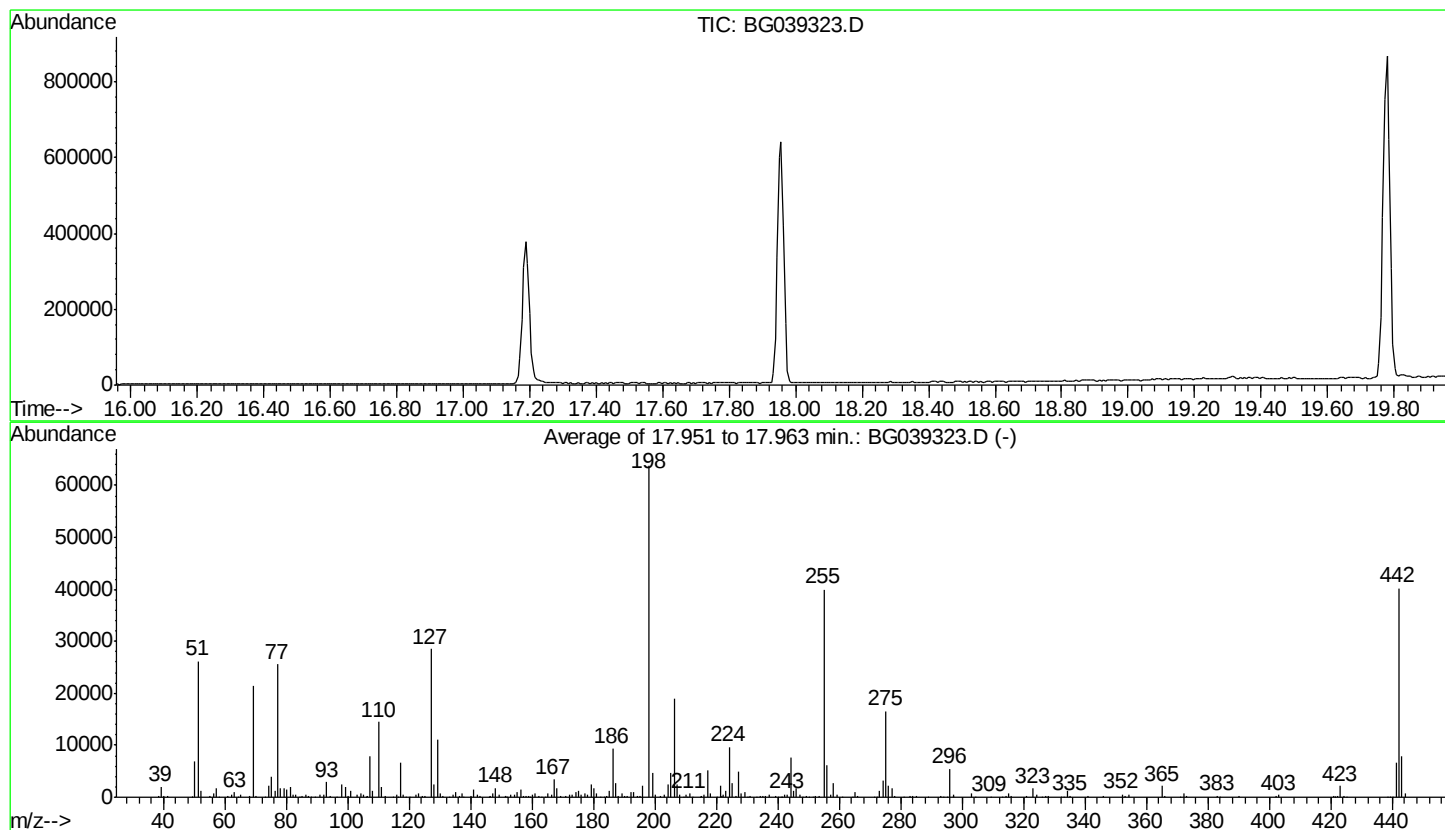

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	26208	PASS
68	69	0.00	2	1.4	307	PASS
69	198	0.00	100	33.5	21347	PASS
70	69	0.00	2	0.6	136	PASS
127	198	10	80	44.7	28504	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63805	PASS
199	198	5	9	7.2	4576	PASS
275	198	10	60	25.9	16549	PASS
365	198	1	100	3.5	2212	PASS
441	198	0.01	100	10.3	6579	PASS
442	198	50	100	63.1	40264	PASS
443	442	15	24	19.3	7789	PASS