
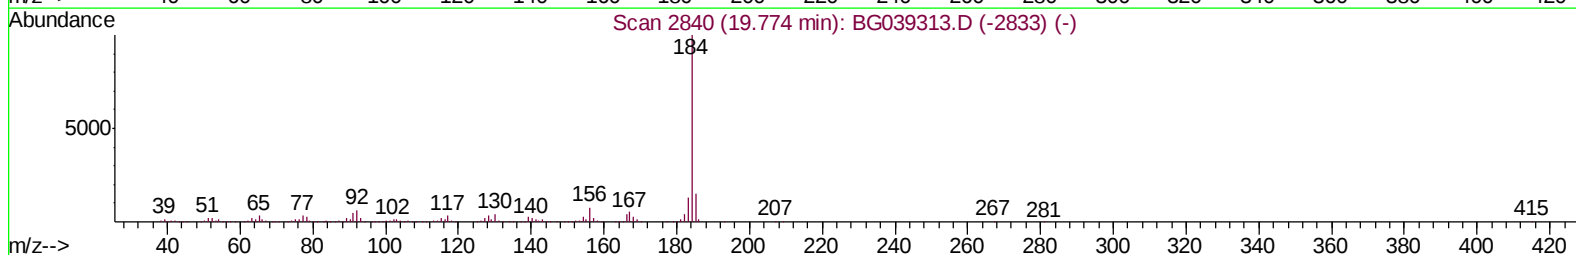
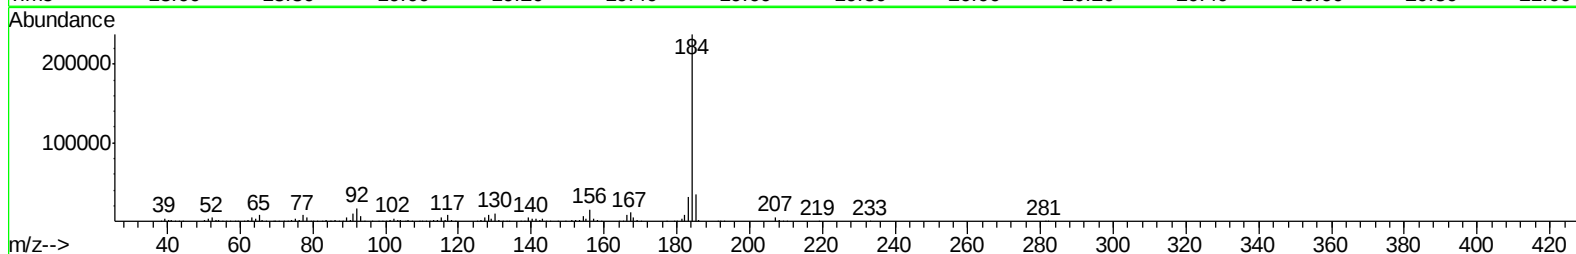


Data File : BG039342.D
Acq On : 1 Feb 2019 13:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 02:19:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

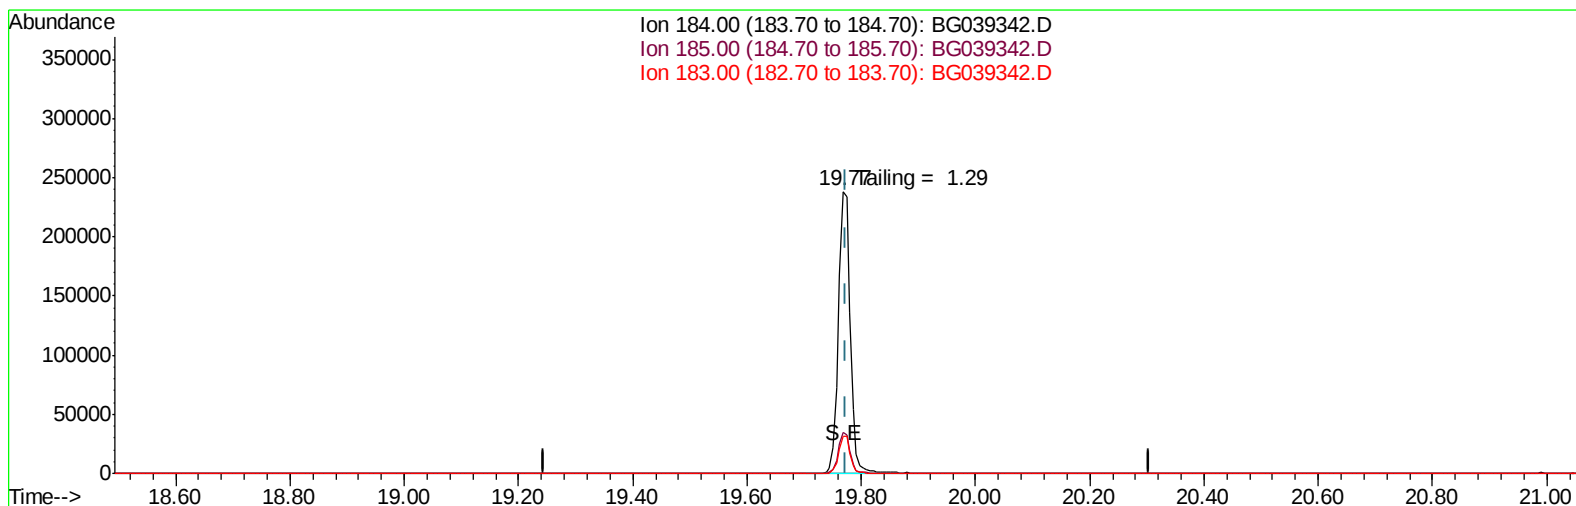

TIC: BG039342.D

(77) Benzidine

19.768min (-0.006) 37101.73ng m

response 341809

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.62
183.00	13.20	13.37
0.00	0.00	0.00

Data File : BG039342.D

Acq On : 1 Feb 2019 13:21

Operator : JU/SJ

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Feb 02 02:19:27 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jan 29 15:41:51 2019

Response via : Initial Calibration

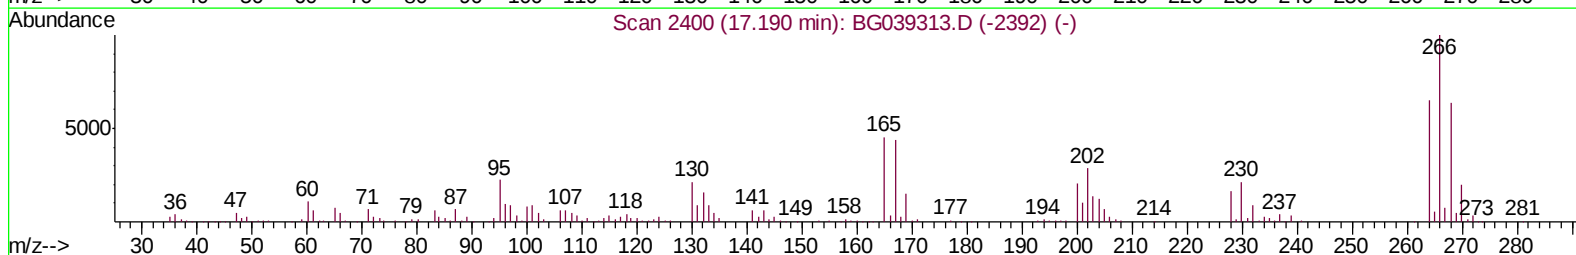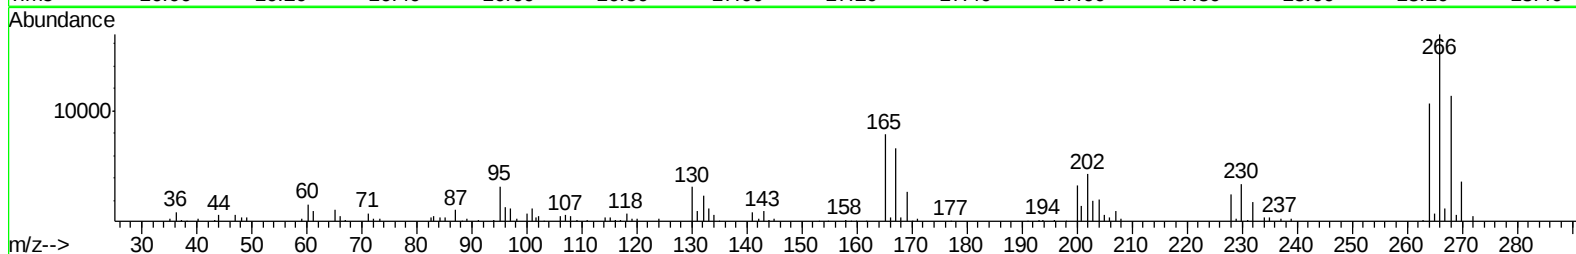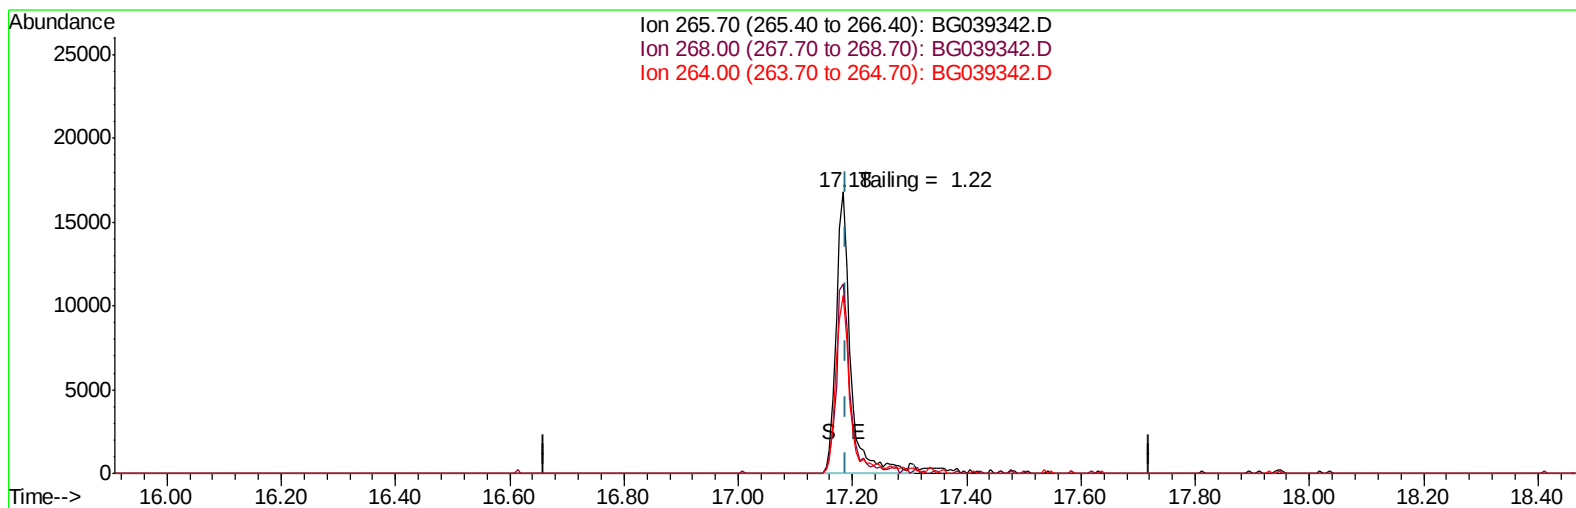

TIC: BG039342.D

(70) Pentachlorophenol (C)

17.183min (-0.006) 65933.23ng

response 29073

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.13
264.00	65.10	63.14
0.00	0.00	0.00