


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG020119\
 Data File : BG039342.D
 Acq On : 1 Feb 2019 13:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

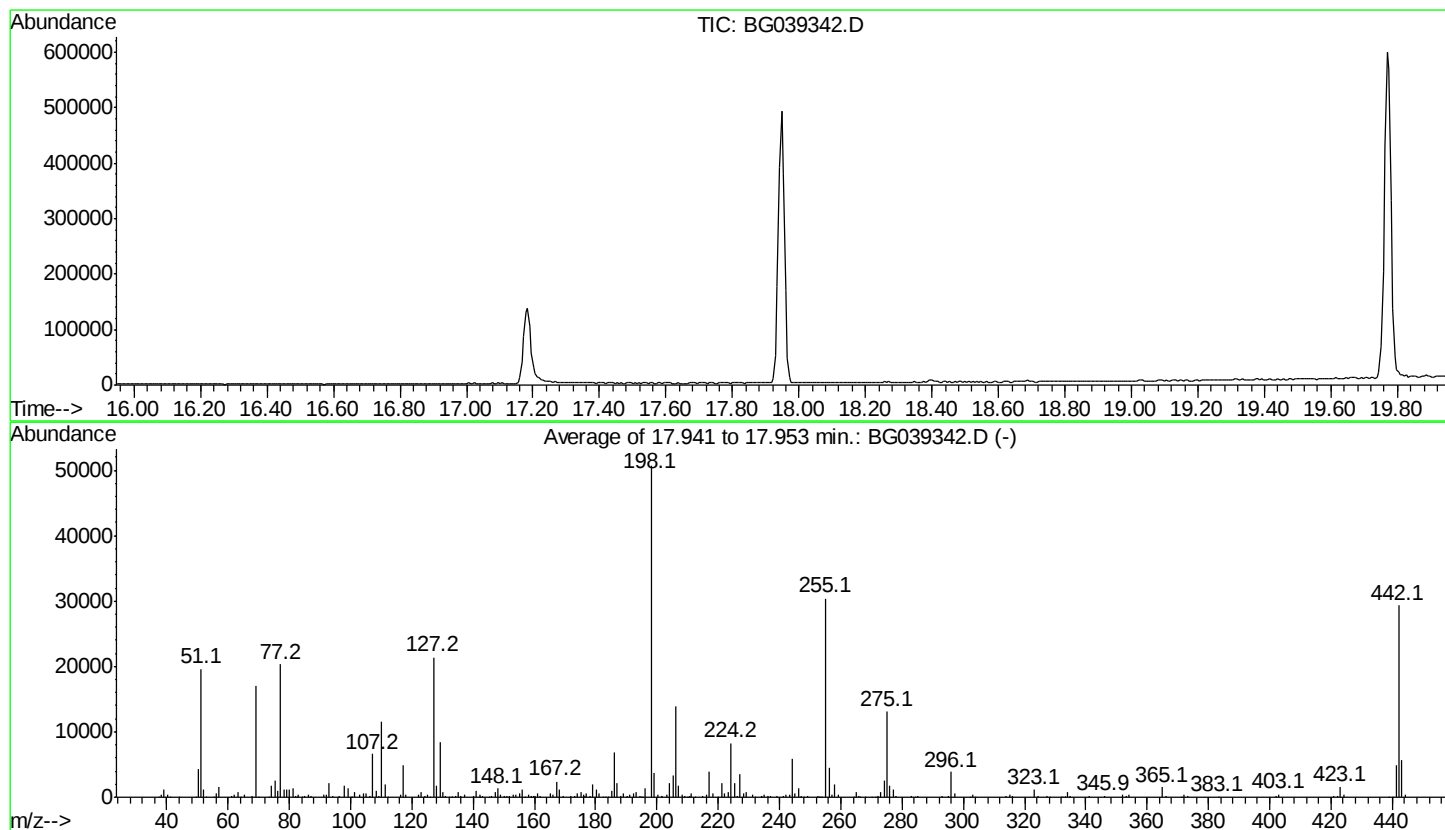

AutoFind: Scans 2528, 2529, 2530; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	19582	PASS
68	69	0.00	2	0.6	106	PASS
69	198	0.00	100	33.6	17017	PASS
70	69	0.00	2	0.5	78	PASS
127	198	10	80	42.2	21410	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50698	PASS
199	198	5	9	7.5	3784	PASS
275	198	10	60	25.7	13035	PASS
365	198	1	100	3.0	1535	PASS
441	198	0.01	100	9.7	4939	PASS
442	198	50	100	57.8	29298	PASS
443	442	15	24	19.2	5634	PASS