

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
 Data File : BG052228.D
 Acq On : 1 Feb 2022 14:01
 Operator : CG/JU
 Sample : N1318-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P031-TW001-B-01

Quant Time: Feb 01 14:49:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 18:07:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.234	152	30381	20.000	ng/ul	0.00
20) Naphthalene-d8	11.071	136	126871	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.878	164	88716	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.627	188	210470	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.939	240	206882	20.000	ng/ul	# 0.00
88) Perylene-d12	25.410	264	203816	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.564	96	3537	4.697	ng/uL	0.00
4) Pyridine-d5	4.004	84	9499	4.055	ng/ul	0.02
7) Phenol-d5	7.376	99	21488	7.776	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.540	67	53898	32.104	ng/ul	0.00
11) 2-Chlorophenol-d4	7.764	132	50048	25.990	ng/ul	0.00
15) 4-Methylphenol-d8	8.939	113	35808	17.075	ng/ul	0.00
21) Nitrobenzene-d5	9.409	128	31993	30.970	ng/ul	0.00
24) 2-Nitrophenol-d4	10.137	143	33885	30.018	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.689	165	59923	27.230	ng/ul	0.00
31) 4-Chloroaniline-d4	11.200	131	60877	21.809	ng/ul	0.00
46) Dimethylphthalate-d6	14.267	166	222443	31.899	ng/ul	0.00
49) Acenaphthylene-d8	14.572	160	276805	31.847	ng/ul	0.00
54) 4-Nitrophenol-d4	15.060	143	6903	6.536	ng/ul	0.00
60) Fluorene-d10	15.865	176	197784	32.374	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.976	200	34044	26.200	ng/ul	0.00
73) Anthracene-d10	17.721	188	342818	34.550	ng/ul	0.00
81) Pyrene-d10	20.000	212	410439	33.103	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.175	264	384185	35.481	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.798	149	11661	1.627	ng/ul#	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052228.D
Acq On : 1 Feb 2022 14:01
Operator : CG/JU
Sample : N1318-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P031-TW001-B-01


Quant Time: Feb 01 14:49:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

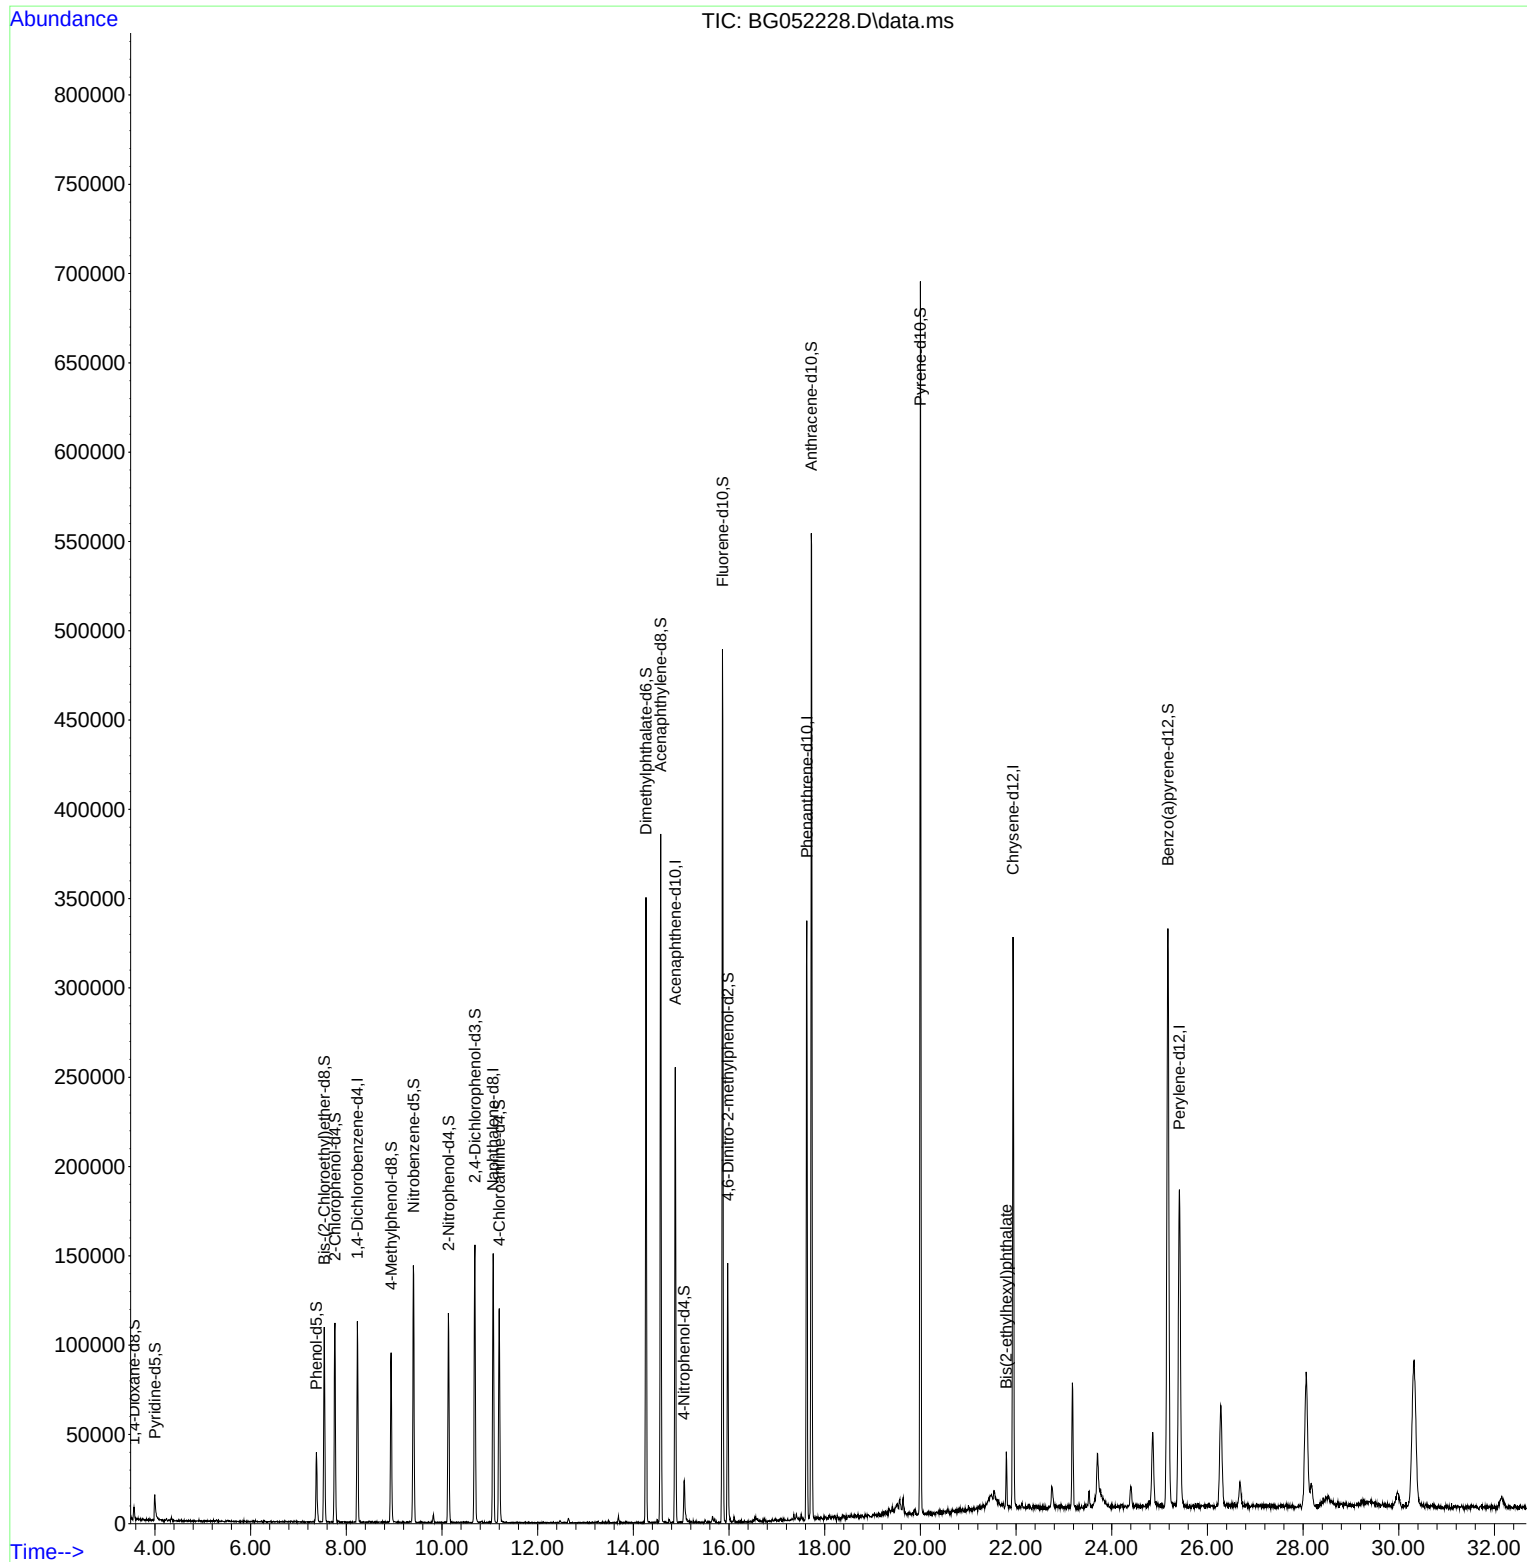

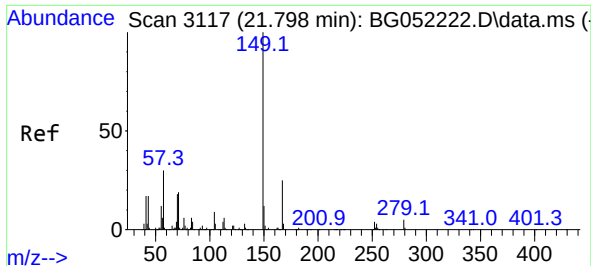

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.627 ng/ul
 RT: 21.798 min Scan# 3117
 Delta R.T. -0.006 min
 Lab File: BG052228.D
 Acq: 1 Feb 2022 14:01

Instrument :
 BNA_G
 ClientSampleId :
 P031-TW001-B-01

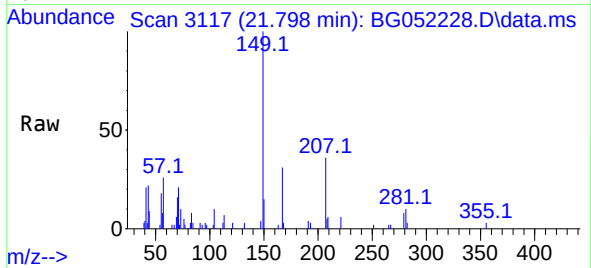

Tgt Ion:149 Resp: 11661
 Ion Ratio Lower Upper
 149 100
 167 30.7 21.1 31.7
 279 8.4 2.7 4.1#

