

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
 Data File : BG052224.D
 Acq On : 1 Feb 2022 11:30
 Operator : CG/JU
 Sample : PB142408BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK408

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.565	8	13	19	rBV	9106	14050	1.50%	0.157%
2	3.988	81	85	98	rBV	104563	187654	20.07%	2.090%
3	4.346	143	146	148	rBV2	1402	1547	0.17%	0.017%
4	7.377	654	662	669	rBV	136873	241106	25.79%	2.686%
5	7.542	683	690	700	rVV	104962	179280	19.18%	1.997%
6	7.759	720	727	735	rBV	133011	231228	24.74%	2.576%
7	8.235	800	808	818	rVB	85096	143270	15.33%	1.596%
8	8.940	920	928	939	rVV	161740	284309	30.41%	3.167%
9	9.404	999	1007	1014	rBV	140298	241516	25.84%	2.690%
10	10.138	1124	1132	1139	rBV	117335	204869	21.92%	2.282%
11	10.684	1218	1225	1236	rBV	166856	291838	31.22%	3.251%
12	11.072	1283	1291	1301	rBV	114814	203981	21.82%	2.272%
13	11.195	1305	1312	1324	rBV	159350	291303	31.16%	3.245%
14	12.646	1553	1559	1565	rBV3	2263	3929	0.42%	0.044%
15	14.268	1826	1835	1842	rBV	336673	480308	51.38%	5.351%
16	14.573	1878	1887	1895	rBV	346062	561388	60.06%	6.254%
17	14.879	1932	1939	1948	rVB	197008	299065	31.99%	3.332%
18	15.061	1963	1970	1980	rBV	107950	192651	20.61%	2.146%
19	15.143	1982	1984	1989	rVB5	1330	1975	0.21%	0.022%
20	15.866	2100	2107	2115	rBV	451391	693547	74.19%	7.726%
21	15.977	2120	2126	2136	rVV	125691	195629	20.93%	2.179%
22	16.101	2143	2147	2151	rBV4	1529	2495	0.27%	0.028%
23	17.628	2398	2407	2413	rBV	254822	388538	41.56%	4.328%
24	17.722	2416	2423	2438	rBV2	514870	790486	84.56%	8.806%
25	19.572	2733	2738	2741	rBV4	7465	10539	1.13%	0.117%
26	19.643	2746	2750	2754	rBV	6673	9723	1.04%	0.108%
27	20.001	2805	2811	2822	rBV	633274	934781	100.00%	10.413%
28	20.078	2822	2824	2826	rVV3	1744	1656	0.18%	0.018%
29	20.683	2925	2927	2929	rVV3	1421	1530	0.16%	0.017%
30	20.730	2933	2935	2937	rBV2	1903	1536	0.16%	0.017%
31	20.882	2957	2961	2963	rBV4	1392	2096	0.22%	0.023%
32	20.959	2972	2974	2976	rBV3	2282	2048	0.22%	0.023%
33	21.223	3017	3019	3020	rBV	1575	1488	0.16%	0.017%
34	21.258	3024	3025	3027	rBV2	1606	1520	0.16%	0.017%
35	21.452	3056	3058	3060	rVV2	2427	2739	0.29%	0.031%
36	21.476	3060	3062	3067	rVB6	2894	4363	0.47%	0.049%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
 Data File : BG052224.D
 Acq On : 1 Feb 2022 11:30
 Operator : CG/JU
 Sample : PB142408BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK408

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	21.540	3070	3073	3074	rBV3	2074	2039	0.22%	0.023%
38	21.846	3123	3125	3128	rBV2	1999	2367	0.25%	0.026%
39	21.940	3134	3141	3148	rBV	240424	399173	42.70%	4.447%
40	22.122	3168	3172	3175	rBV5	2429	3541	0.38%	0.039%
41	22.280	3197	3199	3202	rBV4	1627	1955	0.21%	0.022%
42	22.774	3281	3283	3284	rBV2	1959	1628	0.17%	0.018%
43	22.827	3290	3292	3295	rVB2	2500	2573	0.28%	0.029%
44	22.856	3295	3297	3299	rBV3	1890	2116	0.23%	0.024%
45	23.009	3320	3323	3325	rBV4	1357	1585	0.17%	0.018%
46	23.391	3386	3388	3391	rBV3	1657	1898	0.20%	0.021%
47	23.532	3407	3412	3418	rVB6	4654	8687	0.93%	0.097%
48	23.726	3443	3445	3447	rVB3	2197	1655	0.18%	0.018%
49	23.861	3466	3468	3471	rVB3	2397	2769	0.30%	0.031%
50	23.925	3475	3479	3482	rBV4	2229	3182	0.34%	0.035%
51	23.972	3486	3487	3489	rBV2	2515	2054	0.22%	0.023%
52	24.401	3555	3560	3566	rBV10	6718	15659	1.68%	0.174%
53	24.489	3573	3575	3577	rBV3	1983	1452	0.16%	0.016%
54	24.630	3596	3599	3600	rBV2	2281	2449	0.26%	0.027%
55	24.748	3617	3619	3621	rVB3	2737	1722	0.18%	0.019%
56	25.077	3673	3675	3677	rBV2	1813	1866	0.20%	0.021%
57	25.177	3679	3692	3704	rVV2	294401	882300	94.39%	9.829%
58	25.294	3711	3712	3715	rBV3	3486	2830	0.30%	0.032%
59	25.411	3721	3732	3745	rBV3	132747	420146	44.95%	4.680%
60	25.635	3768	3770	3772	rBV3	2130	1750	0.19%	0.019%
61	25.846	3805	3806	3809	rVB3	2823	1793	0.19%	0.020%
62	25.911	3815	3817	3822	rVB5	1834	2481	0.27%	0.028%
63	26.134	3853	3855	3857	rVB3	2706	2166	0.23%	0.024%
64	26.340	3888	3890	3892	rVB3	2915	1970	0.21%	0.022%
65	26.398	3898	3900	3902	rBV3	1812	1652	0.18%	0.018%
66	26.686	3943	3949	3957	rVB3	8337	21721	2.32%	0.242%
67	26.992	3999	4001	4004	rVV3	2409	2109	0.23%	0.023%
68	27.092	4016	4018	4021	rVB4	2789	2395	0.26%	0.027%
69	27.121	4021	4023	4024	rBV2	2298	1770	0.19%	0.020%
70	27.162	4029	4030	4031	rBV	3043	1832	0.20%	0.020%
71	27.285	4048	4051	4054	rBV4	2397	3933	0.42%	0.044%
72	27.908	4155	4157	4160	rVB4	3036	2101	0.22%	0.023%
73	28.167	4198	4201	4202	rBV3	3878	4334	0.46%	0.048%
74	28.360	4232	4234	4236	rBV3	2074	2018	0.22%	0.022%
75	28.537	4262	4264	4266	rBV3	1796	1734	0.19%	0.019%
76	28.584	4270	4272	4275	rBV3	1765	1703	0.18%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
 Data File : BG052224.D
 Acq On : 1 Feb 2022 11:30
 Operator : CG/JU
 Sample : PB142408BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK408

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

77	28.760	4301	4302	4305	rBV3	2699	2383	0.25%	0.027%
78	29.142	4364	4367	4368	rBV3	2172	2245	0.24%	0.025%
79	29.471	4421	4423	4426	rVB4	2210	1714	0.18%	0.019%
80	29.618	4446	4448	4453	rVB5	2492	2397	0.26%	0.027%
81	29.858	4487	4489	4493	rBV5	1618	2305	0.25%	0.026%
82	29.911	4497	4498	4499	rBV	2734	1476	0.16%	0.016%
83	30.275	4556	4560	4562	rBV4	3520	4758	0.51%	0.053%
84	30.534	4603	4604	4606	rBV2	1995	1424	0.15%	0.016%
85	30.857	4657	4659	4662	rBV4	1942	2451	0.26%	0.027%
86	31.069	4691	4695	4697	rBV4	2065	1895	0.20%	0.021%
87	31.398	4749	4751	4753	rBV3	2294	2119	0.23%	0.024%
88	31.474	4762	4764	4767	rVB4	1914	1504	0.16%	0.017%
89	31.574	4780	4781	4784	rVB2	3356	1993	0.21%	0.022%
90	31.609	4784	4787	4788	rBV3	2110	2016	0.22%	0.022%
91	31.632	4789	4791	4793	rVB2	4314	3189	0.34%	0.036%
92	31.650	4793	4794	4796	rBV	2615	2596	0.28%	0.029%
93	31.738	4807	4809	4812	rVB3	2744	2357	0.25%	0.026%
94	31.779	4812	4816	4818	rBV5	2475	3725	0.40%	0.041%
95	31.897	4834	4836	4839	rBV4	1560	1668	0.18%	0.019%
96	32.032	4858	4859	4862	rVB3	2427	2223	0.24%	0.025%
97	32.061	4862	4864	4866	rBV3	1435	1778	0.19%	0.020%
98	32.108	4870	4872	4874	rVV3	2495	2344	0.25%	0.026%
99	32.343	4910	4912	4916	rVB5	1893	1508	0.16%	0.017%
100	32.420	4923	4925	4928	rVB4	2953	1596	0.17%	0.018%




Sum of corrected areas: 8976753

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052224.D
Acq On : 1 Feb 2022 11:30
Operator : CG/JU
Sample : PB142408BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

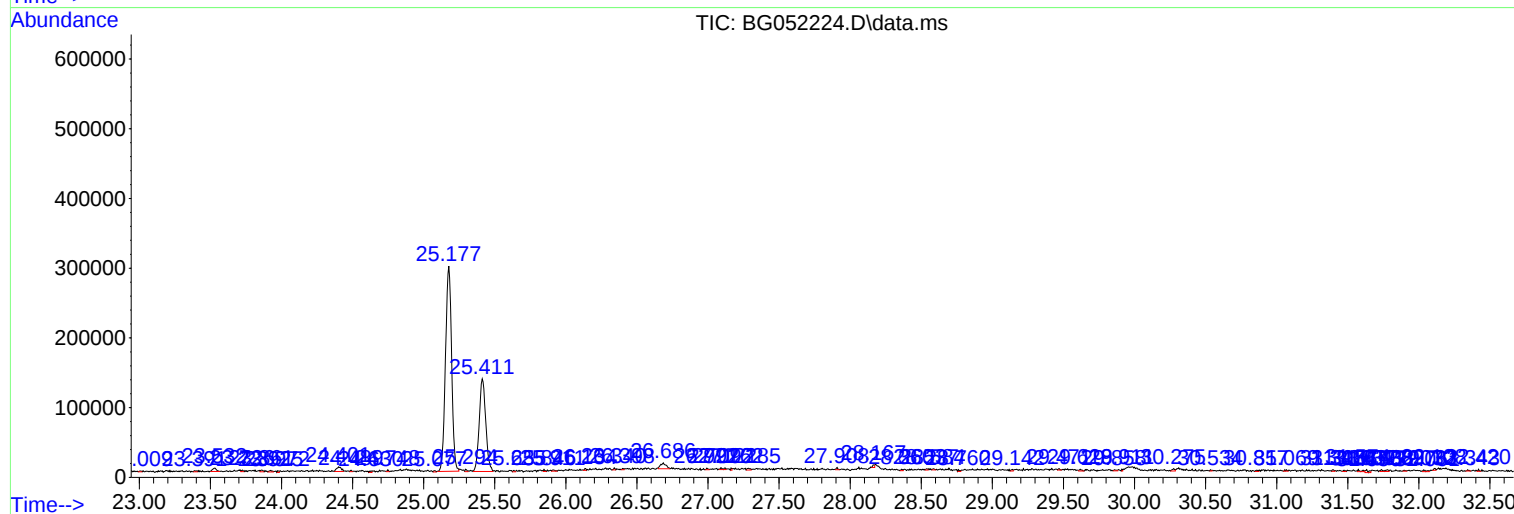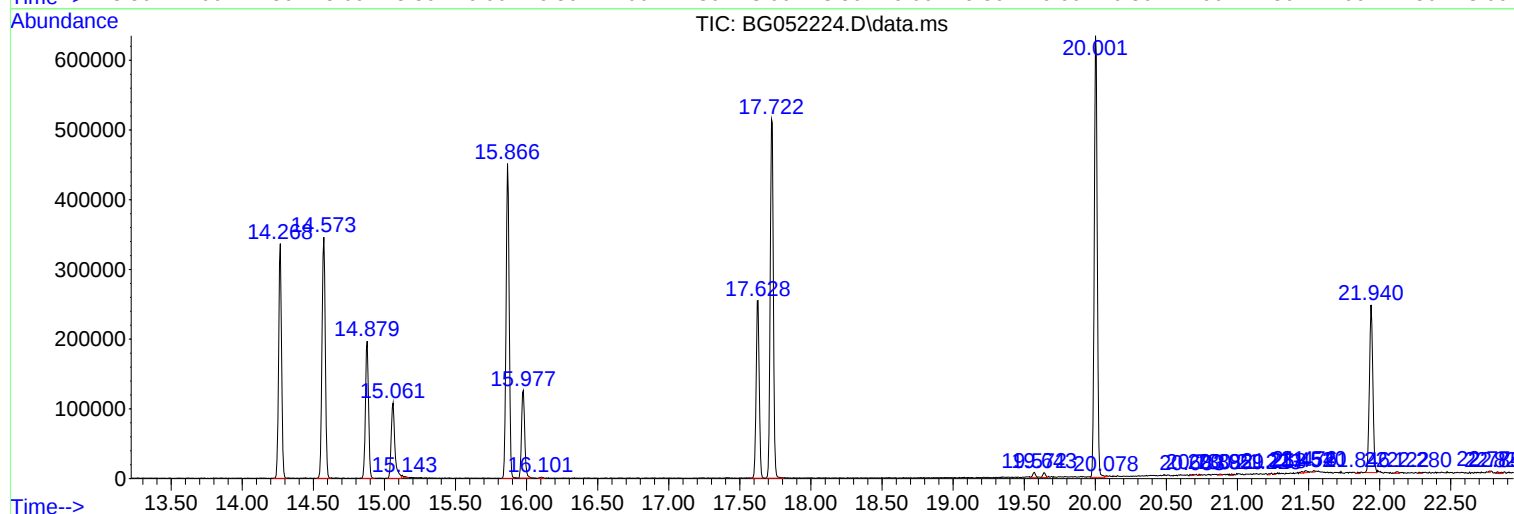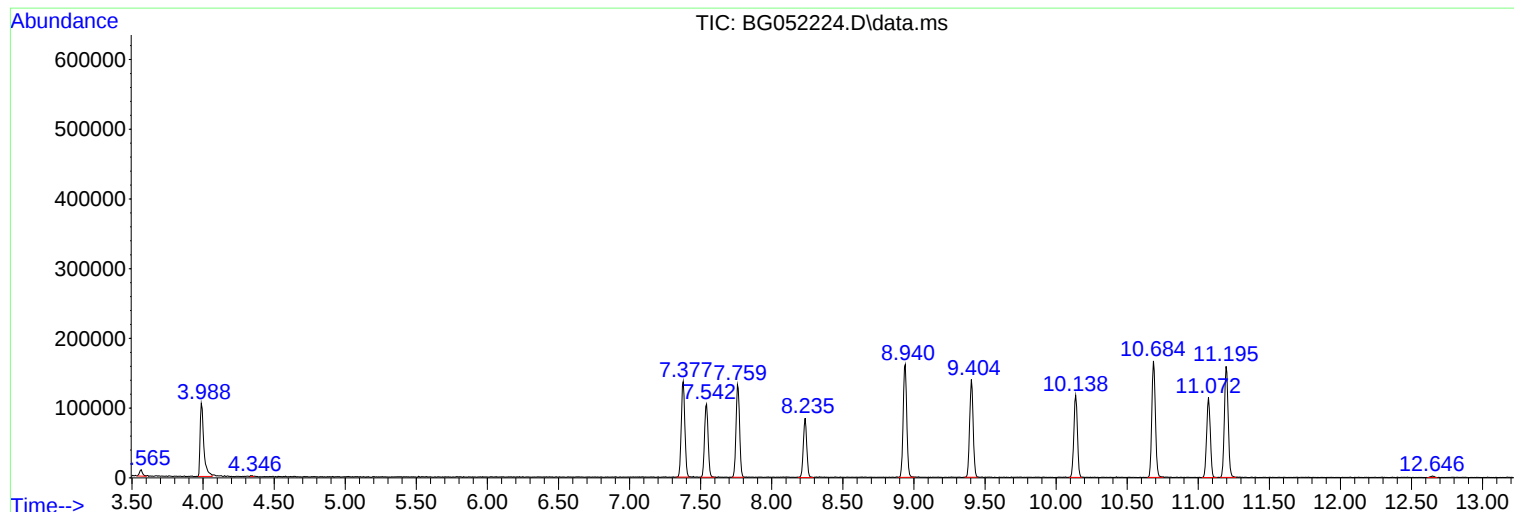

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052224.D
Acq On : 1 Feb 2022 11:30
Operator : CG/JU
Sample : PB142408BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052224.D
Acq On : 1 Feb 2022 11:30
Operator : CG/JU
Sample : PB142408BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc