

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
 Data File : BG052234.D
 Acq On : 1 Feb 2022 17:49
 Operator : CG/JU
 Sample : N1328-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COHM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.564	8	13	18	rVB2	6083	9322	0.93%	0.103%
2	3.993	83	86	100	rBV2	21604	43557	4.34%	0.483%
3	4.239	126	128	131	rBV	1321	1355	0.13%	0.015%
4	4.339	143	145	151	rBV2	2743	3798	0.38%	0.042%
5	5.279	301	305	311	rBV3	1581	2938	0.29%	0.033%
6	7.376	651	662	671	rVB3	25959	52680	5.25%	0.584%
7	7.541	684	690	697	rBV	104166	175684	17.50%	1.948%
8	7.764	720	728	736	rBV	98848	174070	17.34%	1.930%
9	8.234	798	808	815	rBV	109267	185812	18.51%	2.060%
10	8.281	815	816	821	rVB3	1420	1577	0.16%	0.017%
11	8.939	921	928	938	rBV2	75543	131571	13.11%	1.459%
12	9.403	999	1007	1015	rBV	138001	242778	24.18%	2.692%
13	9.820	1073	1078	1083	rVB3	5185	7864	0.78%	0.087%
14	10.137	1125	1132	1139	rVB2	108876	194685	19.39%	2.158%
15	10.684	1218	1225	1233	rBV	143494	256622	25.56%	2.845%
16	10.819	1243	1248	1255	rBV4	6245	9889	0.99%	0.110%
17	11.071	1283	1291	1302	rBV	149609	271815	27.08%	3.013%
18	11.195	1305	1312	1324	rVB	126473	239398	23.85%	2.654%
19	12.464	1523	1528	1533	rVB2	2734	4569	0.46%	0.051%
20	12.651	1556	1560	1565	rVB3	2683	3294	0.33%	0.037%
21	13.262	1662	1664	1670	rVB2	1979	2185	0.22%	0.024%
22	13.362	1674	1681	1683	rBV2	1424	2152	0.21%	0.024%
23	13.409	1687	1689	1692	rVB3	1456	1421	0.14%	0.016%
24	13.691	1729	1737	1745	rBV3	7736	10395	1.04%	0.115%
25	14.267	1828	1835	1841	rBV	343171	491448	48.96%	5.448%
26	14.496	1871	1874	1878	rBV4	2025	2898	0.29%	0.032%
27	14.572	1880	1887	1896	rVB	359902	567140	56.50%	6.288%
28	14.749	1913	1917	1924	rVB3	3688	4850	0.48%	0.054%
29	14.878	1932	1939	1948	rVB	258234	396155	39.46%	4.392%
30	15.066	1965	1971	1979	rBV3	16305	32222	3.21%	0.357%
31	15.659	2066	2072	2074	rBV3	1736	2442	0.24%	0.027%
32	15.694	2076	2078	2083	rVB	2912	3491	0.35%	0.039%
33	15.865	2100	2107	2116	rVB	485149	737668	73.48%	8.178%
34	15.976	2120	2126	2136	rVB	141503	211045	21.02%	2.340%
35	16.100	2146	2147	2152	rVB3	2403	2117	0.21%	0.023%
36	16.253	2170	2173	2178	rVB	1543	2103	0.21%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
 Data File : BG052234.D
 Acq On : 1 Feb 2022 17:49
 Operator : CG/JU
 Sample : N1328-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COHM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	16.305	2180	2182	2190	rVB3	1652	2945	0.29%	0.033%
38	16.499	2211	2215	2218	rBV2	1297	1747	0.17%	0.019%
39	16.534	2218	2221	2222	rBV3	1841	1743	0.17%	0.019%
40	16.558	2223	2225	2229	rVB4	2046	2038	0.20%	0.023%

41	16.752	2251	2258	2260	rBV2	2682	3712	0.37%	0.041%
42	16.787	2261	2264	2269	rVB2	952	1393	0.14%	0.015%
43	16.846	2269	2274	2279	rVB3	964	1973	0.20%	0.022%
44	16.905	2279	2284	2287	rBV4	1494	2568	0.26%	0.028%
45	17.075	2309	2313	2316	rVB2	1533	1711	0.17%	0.019%

46	17.357	2358	2361	2366	rBV4	4102	5434	0.54%	0.060%
47	17.404	2366	2369	2373	rVV4	2455	3029	0.30%	0.034%
48	17.510	2385	2387	2390	rVB3	1448	1452	0.14%	0.016%
49	17.627	2400	2407	2415	rBV	326066	507361	50.54%	5.625%
50	17.727	2417	2424	2436	rVB	550444	854136	85.08%	9.469%

51	17.815	2436	2439	2440	rBV	1043	1386	0.14%	0.015%
52	17.915	2451	2456	2458	rBV3	1905	2770	0.28%	0.031%
53	18.021	2473	2474	2479	rVB3	1759	1454	0.14%	0.016%
54	18.097	2485	2487	2489	rBV3	1780	1742	0.17%	0.019%
55	18.267	2513	2516	2519	rVB4	4138	4921	0.49%	0.055%

56	18.338	2524	2528	2531	rBV3	1434	1915	0.19%	0.021%
57	18.414	2537	2541	2545	rVB4	2652	4558	0.45%	0.051%
58	18.444	2545	2546	2550	rBV3	1585	1957	0.19%	0.022%
59	18.491	2550	2554	2558	rBV5	2968	4667	0.46%	0.052%
60	18.784	2601	2604	2606	rBV2	1680	2072	0.21%	0.023%

61	19.002	2637	2641	2642	rBV2	1396	1849	0.18%	0.020%
62	19.572	2734	2738	2740	rBV2	7171	7295	0.73%	0.081%
63	19.642	2746	2750	2755	rBV2	7162	9134	0.91%	0.101%
64	19.871	2785	2789	2790	rBV3	2132	1797	0.18%	0.020%
65	20.006	2805	2812	2818	rBV	692179	1003866	100.00%	11.129%

66	20.282	2857	2859	2862	rBV4	1321	1416	0.14%	0.016%
67	20.729	2933	2935	2938	rBV4	2132	2098	0.21%	0.023%
68	21.005	2980	2982	2986	rBV5	2645	3622	0.36%	0.040%
69	21.539	3069	3073	3081	rBV7	16006	26961	2.69%	0.299%
70	21.939	3134	3141	3153	rVB	303867	539366	53.73%	5.980%

71	23.819	3459	3461	3463	rBV3	3088	2649	0.26%	0.029%
72	25.176	3681	3692	3705	rVB2	334554	946578	94.29%	10.494%
73	25.417	3722	3733	3744	rBV2	182063	561110	55.89%	6.221%
74	26.873	3979	3981	3984	rBV4	2875	2006	0.20%	0.022%
75	28.436	4245	4247	4249	rBV3	2470	1727	0.17%	0.019%

76	31.943	4842	4844	4846	rBV2	2700	2315	0.23%	0.026%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052234.D
Acq On : 1 Feb 2022 17:49
Operator : CG/JU
Sample : N1328-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HM7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Title : SVOA CALIBRATION

77	32.137	4875	4877	4878	rBV2	4039	3199	0.32%	0.035%
78	32.366	4915	4916	4917	rBV	2447	1380	0.14%	0.015%




Sum of corrected areas: 9020062

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052234.D
Acq On : 1 Feb 2022 17:49
Operator : CG/JU
Sample : N1328-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HM7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

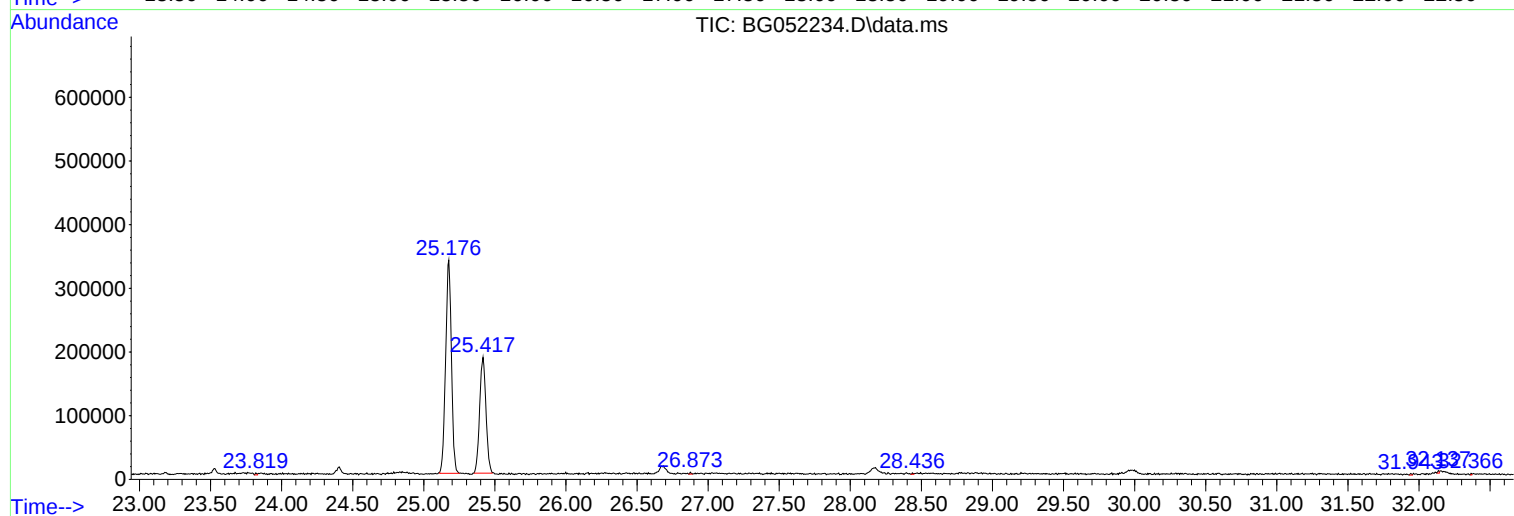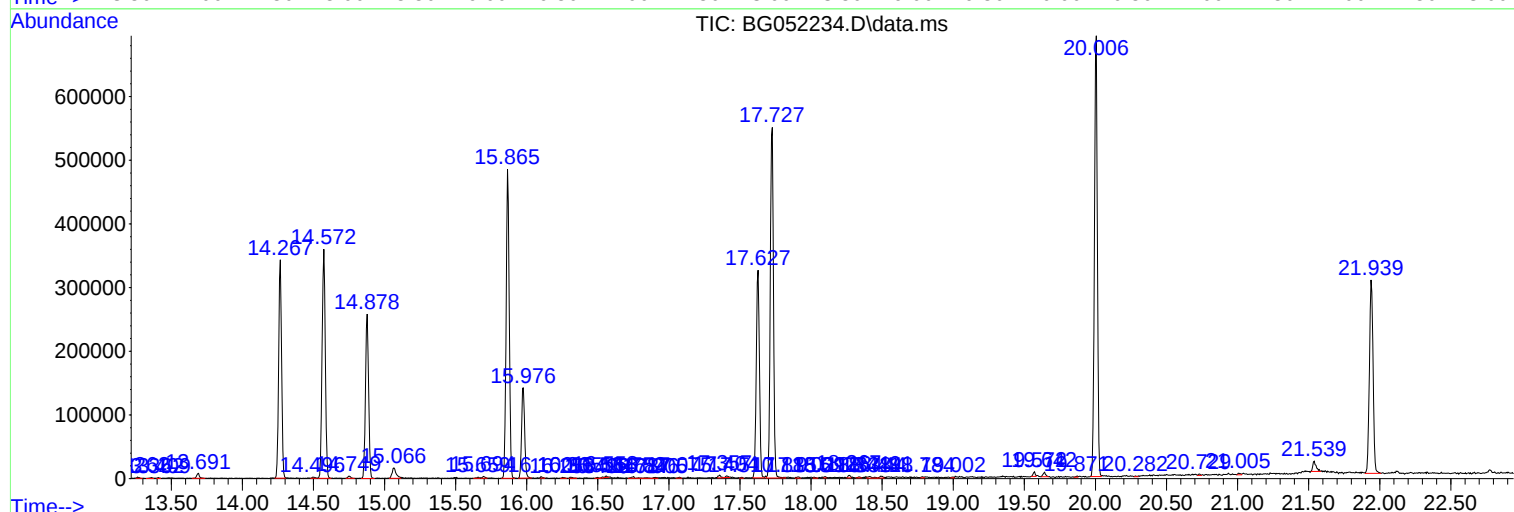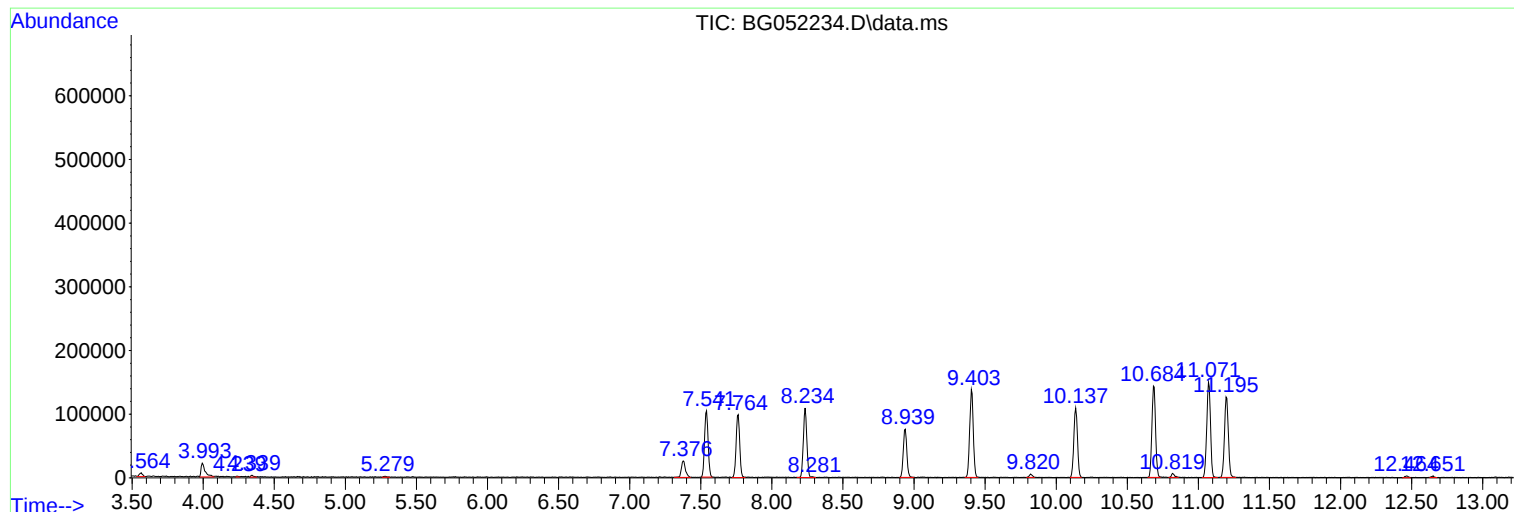

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052234.D
Acq On : 1 Feb 2022 17:49
Operator : CG/JU
Sample : N1328-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HM7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052234.D
Acq On : 1 Feb 2022 17:49
Operator : CG/JU
Sample : N1328-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HM7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc