

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
 Data File : BG052240.D
 Acq On : 1 Feb 2022 22:13
 Operator : CG/JU
 Sample : PB142389BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK389

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.558	8	12	19	rBV	8581	12362	1.29%	0.124%
2	3.987	80	85	98	rVV	108488	188811	19.66%	1.895%
3	4.075	98	100	101	rVV2	1853	1403	0.15%	0.014%
4	4.340	141	145	146	rBV	1847	2078	0.22%	0.021%
5	7.377	655	662	671	rVV	145222	243148	25.32%	2.440%
6	7.541	682	690	698	rVB	103553	180043	18.75%	1.807%
7	7.758	719	727	737	rBV	137553	233111	24.27%	2.340%
8	8.234	801	808	816	rVB	114717	196165	20.42%	1.969%
9	8.933	920	927	937	rBV	170195	289918	30.19%	2.910%
10	9.403	1000	1007	1016	rBV	136555	244089	25.41%	2.450%
11	10.138	1125	1132	1140	rBV	118929	204594	21.30%	2.053%
12	10.684	1218	1225	1236	rBV	163998	295095	30.73%	2.962%
13	11.072	1283	1291	1301	rVB	160713	291718	30.37%	2.928%
14	11.195	1305	1312	1321	rBV	156016	291532	30.35%	2.926%
15	12.652	1554	1560	1563	rBV2	2810	3580	0.37%	0.036%
16	14.267	1828	1835	1844	rBV	334294	485821	50.58%	4.876%
17	14.573	1880	1887	1895	rVV	377914	574904	59.86%	5.770%
18	14.878	1931	1939	1949	rVB	280218	428186	44.58%	4.298%
19	15.060	1963	1970	1987	rBV	112741	205879	21.44%	2.066%
20	15.865	2100	2107	2115	rBV	480092	706394	73.55%	7.090%
21	15.971	2120	2125	2137	rBV	132053	204390	21.28%	2.051%
22	16.106	2144	2148	2151	rVB2	2032	2513	0.26%	0.025%
23	17.416	2367	2371	2372	rBV2	1410	1436	0.15%	0.014%
24	17.622	2400	2406	2414	rVB	357981	547199	56.97%	5.492%
25	17.721	2416	2423	2432	rBV	529083	814015	84.76%	8.170%
26	19.460	2717	2719	2723	rVB	1324	1644	0.17%	0.017%
27	19.566	2732	2737	2741	rBV3	6906	10613	1.11%	0.107%
28	19.637	2745	2749	2755	rBV2	6825	10080	1.05%	0.101%
29	19.789	2772	2775	2780	rBV6	1081	1625	0.17%	0.016%
30	20.001	2805	2811	2820	rBV	672147	960430	100.00%	9.639%
31	20.077	2822	2824	2827	rVB4	1755	1767	0.18%	0.018%
32	20.118	2827	2831	2833	rBV3	1147	1828	0.19%	0.018%
33	20.388	2873	2877	2879	rBV3	1302	1377	0.14%	0.014%
34	20.477	2890	2892	2893	rBV2	2533	1413	0.15%	0.014%
35	20.547	2902	2904	2909	rBV4	1266	2740	0.29%	0.028%
36	20.800	2944	2947	2950	rBV4	1550	2107	0.22%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
 Data File : BG052240.D
 Acq On : 1 Feb 2022 22:13
 Operator : CG/JU
 Sample : PB142389BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK389

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	21.017	2981	2984	2986	rVB3	2466	2035	0.21%	0.020%
38	21.293	3030	3031	3033	rBV2	1785	1574	0.16%	0.016%
39	21.452	3056	3058	3059	rBV2	2123	1538	0.16%	0.015%
40	21.469	3059	3061	3064	rVB4	2433	2784	0.29%	0.028%
41	21.534	3069	3072	3073	rBV2	1658	1833	0.19%	0.018%
42	21.651	3091	3092	3095	rBV3	2082	1980	0.21%	0.020%
43	21.810	3116	3119	3121	rVV3	2210	2588	0.27%	0.026%
44	21.939	3132	3141	3150	rBV	335203	584225	60.83%	5.864%
45	22.110	3169	3170	3172	rBV2	1800	1622	0.17%	0.016%
46	22.204	3183	3186	3189	rBV5	1978	2702	0.28%	0.027%
47	22.362	3212	3213	3215	rBV	1695	1388	0.14%	0.014%
48	22.421	3218	3223	3224	rBV5	1769	2855	0.30%	0.029%
49	22.497	3234	3236	3239	rBV3	1262	1722	0.18%	0.017%
50	22.703	3269	3271	3272	rBV2	1987	1414	0.15%	0.014%
51	22.773	3281	3283	3287	rVB4	3783	5337	0.56%	0.054%
52	23.026	3323	3326	3329	rBV4	1620	2040	0.21%	0.020%
53	23.138	3344	3345	3347	rVB2	2557	1636	0.17%	0.016%
54	23.161	3347	3349	3351	rBV3	1749	1776	0.18%	0.018%
55	23.220	3356	3359	3361	rBV3	2450	3020	0.31%	0.030%
56	23.525	3405	3411	3416	rVB6	7254	12784	1.33%	0.128%
57	24.195	3522	3525	3529	rBV6	2274	2732	0.28%	0.027%
58	24.407	3553	3561	3567	rVB7	7972	19580	2.04%	0.197%
59	24.618	3594	3597	3600	rBV4	1812	2659	0.28%	0.027%
60	24.741	3616	3618	3621	rBV4	2707	2933	0.31%	0.029%
61	25.170	3678	3691	3706	rBV2	310732	928146	96.64%	9.315%
62	25.417	3721	3733	3747	rVB2	193308	607912	63.30%	6.101%
63	25.605	3763	3765	3768	rVB3	1914	1737	0.18%	0.017%
64	25.693	3778	3780	3782	rVV3	2203	1764	0.18%	0.018%
65	25.717	3782	3784	3787	rVB3	2070	2118	0.22%	0.021%
66	25.975	3825	3828	3831	rBV5	1620	2315	0.24%	0.023%
67	26.157	3857	3859	3862	rBV3	1528	1787	0.19%	0.018%
68	26.204	3866	3867	3869	rBV2	2653	1683	0.18%	0.017%
69	26.374	3894	3896	3900	rVB4	1752	2012	0.21%	0.020%
70	26.539	3920	3924	3929	rVB7	2309	3554	0.37%	0.036%
71	26.674	3943	3947	3948	rBV2	7993	10688	1.11%	0.107%
72	26.815	3967	3971	3974	rBV5	1800	2594	0.27%	0.026%
73	27.367	4064	4065	4070	rBV5	1756	1709	0.18%	0.017%
74	27.561	4094	4098	4101	rBV6	2241	4128	0.43%	0.041%
75	27.696	4119	4121	4122	rBV2	2069	1620	0.17%	0.016%
76	27.914	4155	4158	4159	rBV3	2326	2387	0.25%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
 Data File : BG052240.D
 Acq On : 1 Feb 2022 22:13
 Operator : CG/JU
 Sample : PB142389BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK389

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

77	28.013	4174	4175	4177	rBV2	2171	1855	0.19%	0.019%
78	28.066	4182	4184	4188	rVV5	1542	2295	0.24%	0.023%
79	28.178	4195	4203	4205	rBV6	7558	18629	1.94%	0.187%
80	29.018	4344	4346	4349	rBV3	1495	2085	0.22%	0.021%
81	29.100	4358	4360	4365	rBV5	1454	1415	0.15%	0.014%
82	29.382	4406	4408	4410	rVB2	3382	2250	0.23%	0.023%
83	29.506	4426	4429	4430	rBV3	2370	2571	0.27%	0.026%
84	29.776	4473	4475	4481	rVB5	1895	2393	0.25%	0.024%
85	29.970	4499	4508	4510	rBV8	7469	16996	1.77%	0.171%
86	30.246	4553	4555	4557	rVB3	2622	1785	0.19%	0.018%
87	30.686	4627	4630	4631	rVB3	2171	2118	0.22%	0.021%
88	30.898	4663	4666	4668	rBV4	1899	1906	0.20%	0.019%
89	31.062	4693	4694	4697	rBV3	1425	1410	0.15%	0.014%
90	31.262	4725	4728	4729	rBV3	1483	1705	0.18%	0.017%
91	31.297	4732	4734	4737	rVB3	1702	1599	0.17%	0.016%
92	31.368	4745	4746	4748	rBV2	1543	1428	0.15%	0.014%
93	31.391	4748	4750	4753	rVB3	1775	1530	0.16%	0.015%
94	31.697	4801	4802	4803	rBV	2410	1402	0.15%	0.014%
95	31.932	4839	4842	4843	rVB3	2874	2245	0.23%	0.023%
96	31.961	4846	4847	4854	rVB4	2983	4345	0.45%	0.044%
97	32.014	4854	4856	4857	rBV2	2294	1430	0.15%	0.014%
98	32.032	4857	4859	4861	rBV2	1894	1576	0.16%	0.016%
99	32.055	4861	4863	4865	rBV3	2052	2201	0.23%	0.022%
100	32.096	4868	4870	4871	rBV	2071	1435	0.15%	0.014%




Sum of corrected areas: 9963523

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052240.D
Acq On : 1 Feb 2022 22:13
Operator : CG/JU
Sample : PB142389BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK389

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

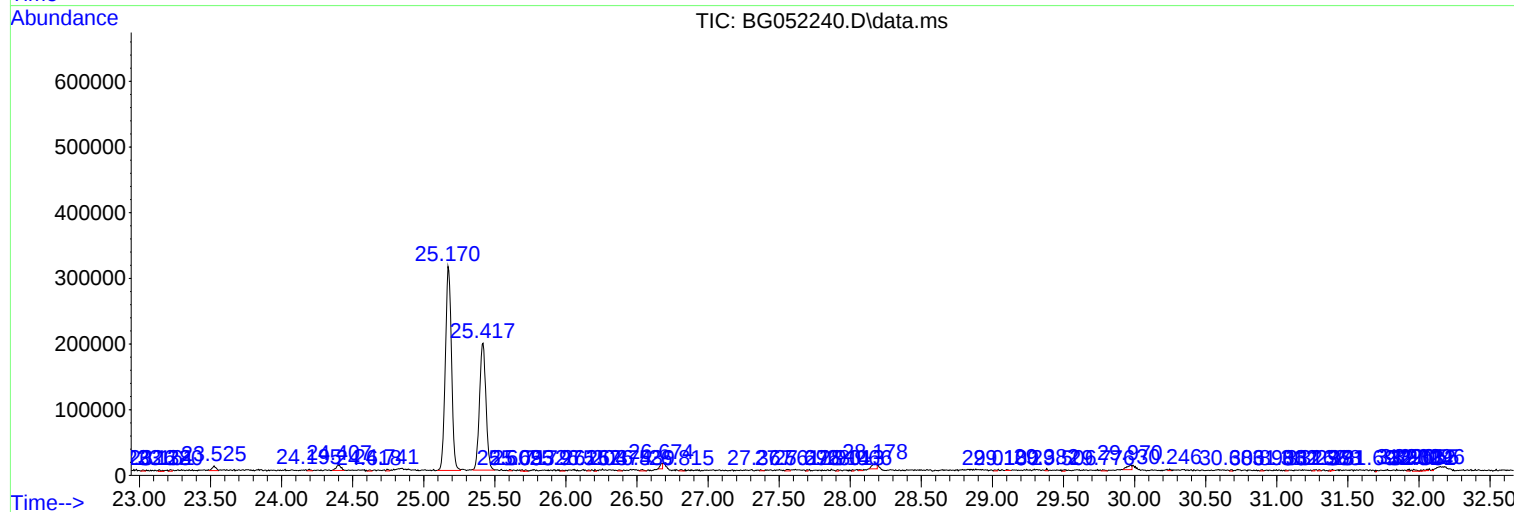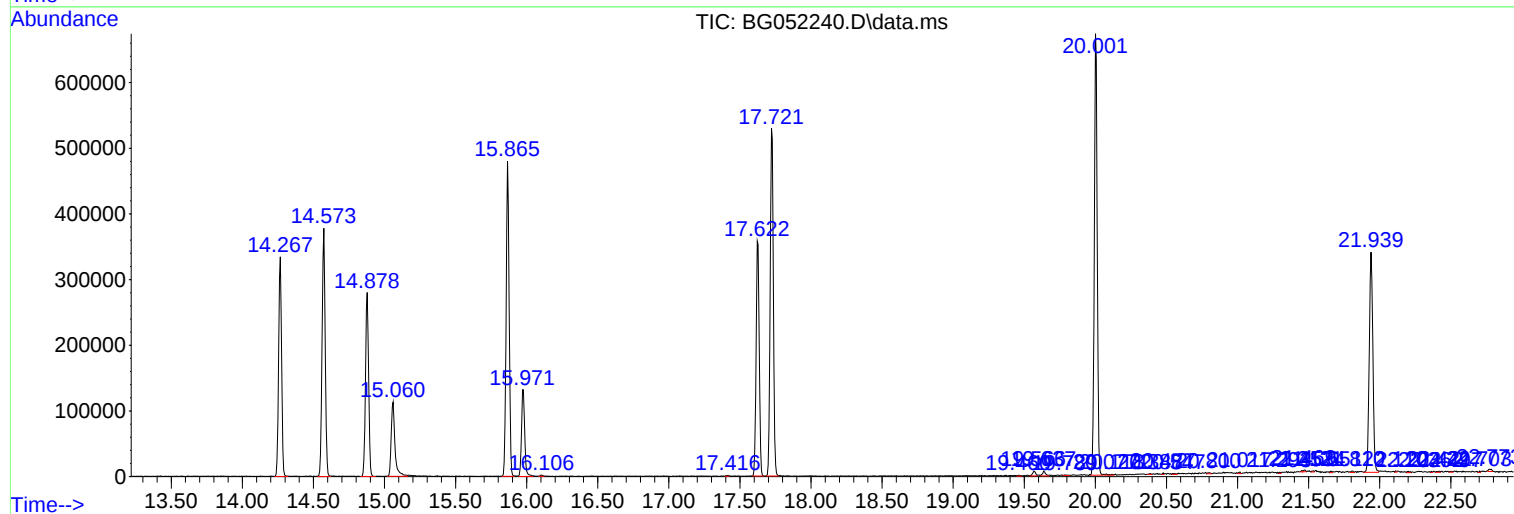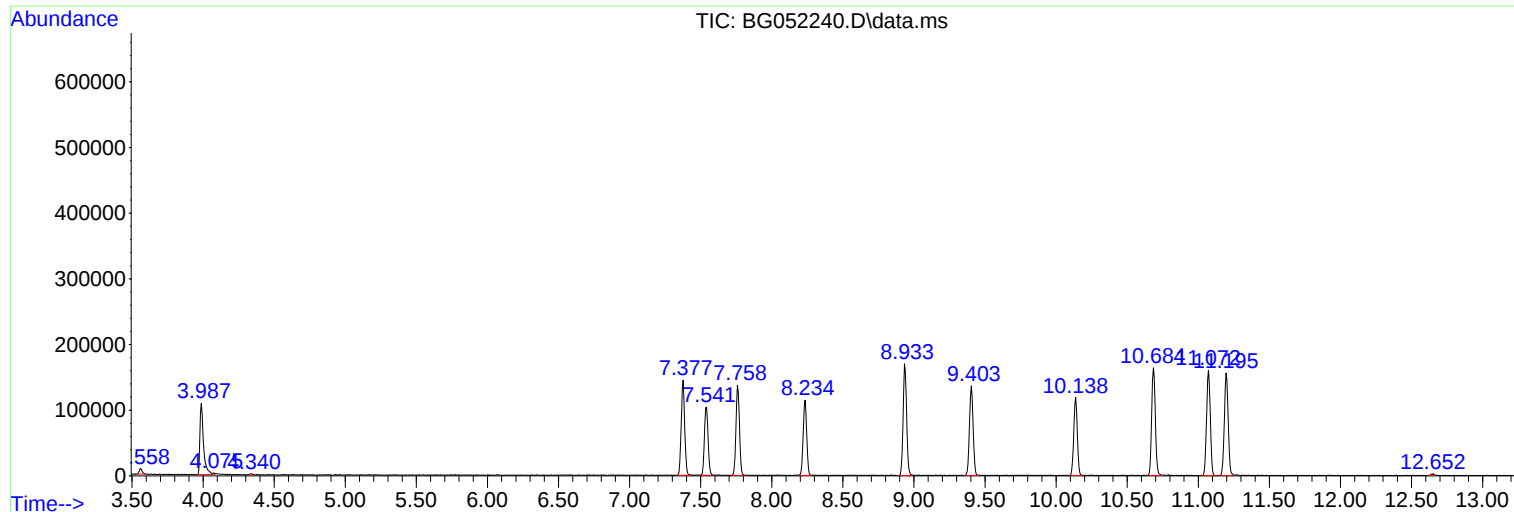

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052240.D
Acq On : 1 Feb 2022 22:13
Operator : CG/JU
Sample : PB142389BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK389

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020122\
Data File : BG052240.D
Acq On : 1 Feb 2022 22:13
Operator : CG/JU
Sample : PB142389BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK389

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc