


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020123\  
Data File : BG056494.D  
Acq On : 1 Feb 2023 9:01  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG012723.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Feb 01 01:15:52 2023

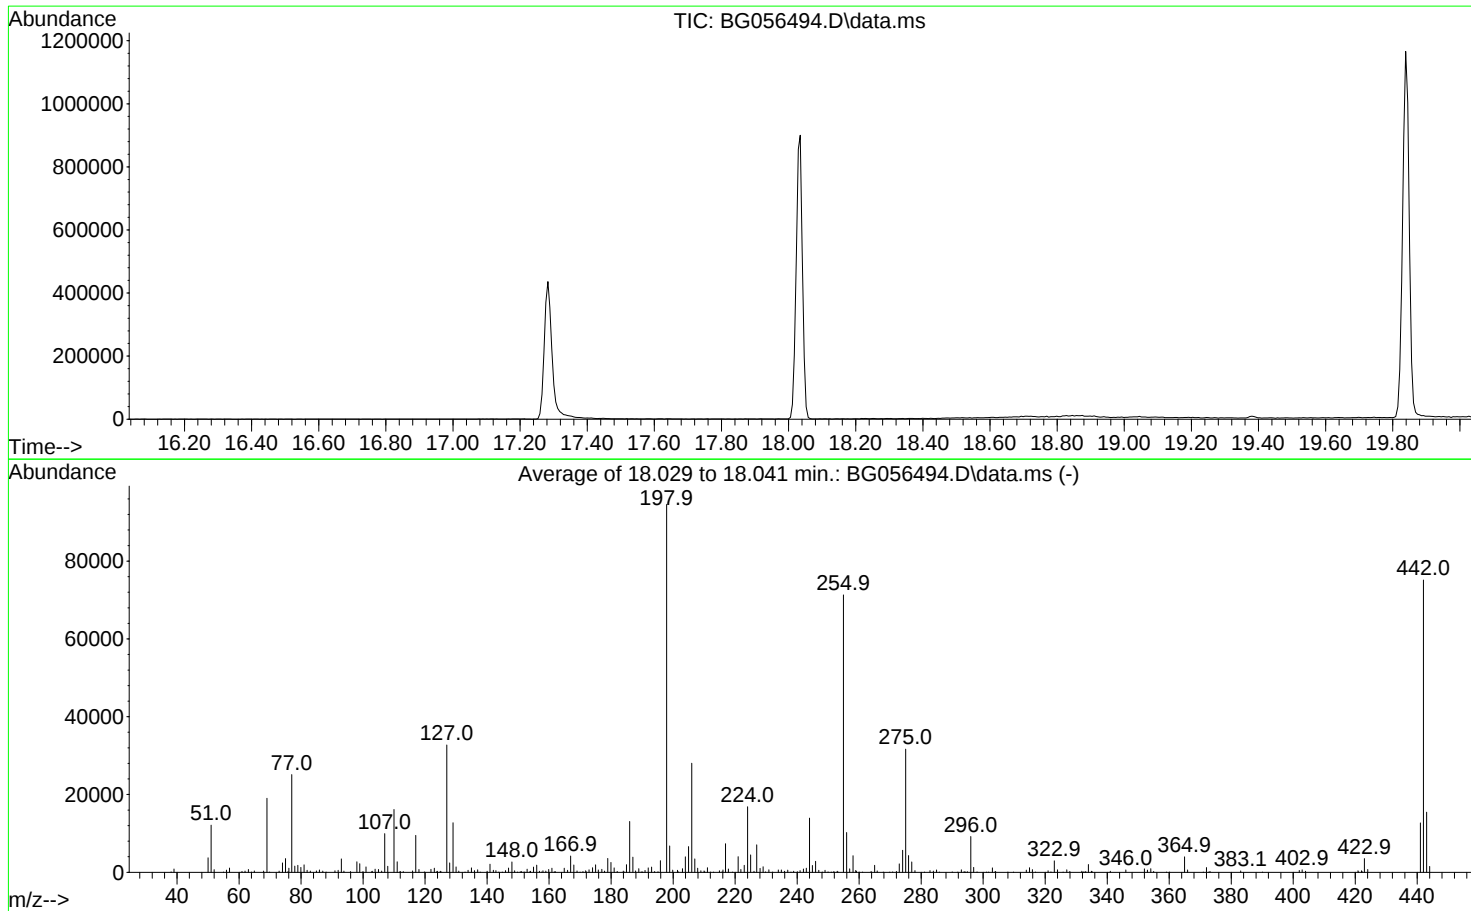




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 12.8         | 12110      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 302        | PASS                |
| 69             | 198             | 0.00            | 100             | 20.1         | 19021      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 78         | PASS                |
| 127            | 198             | 10              | 80              | 34.6         | 32739      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 94579      | PASS                |
| 199            | 198             | 5               | 9               | 7.1          | 6762       | PASS                |
| 275            | 198             | 10              | 60              | 33.5         | 31645      | PASS                |
| 365            | 198             | 1               | 100             | 4.2          | 3975       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.4         | 12714      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 75163      | PASS                |
| 443            | 442             | 15              | 24              | 20.5         | 15438      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020123\  
Data File : BG056494.D  
Acq On : 1 Feb 2023 9:01  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Feb 02 05:48:23 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG012723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Feb 01 01:15:52 2023  
Response via : Initial Calibration

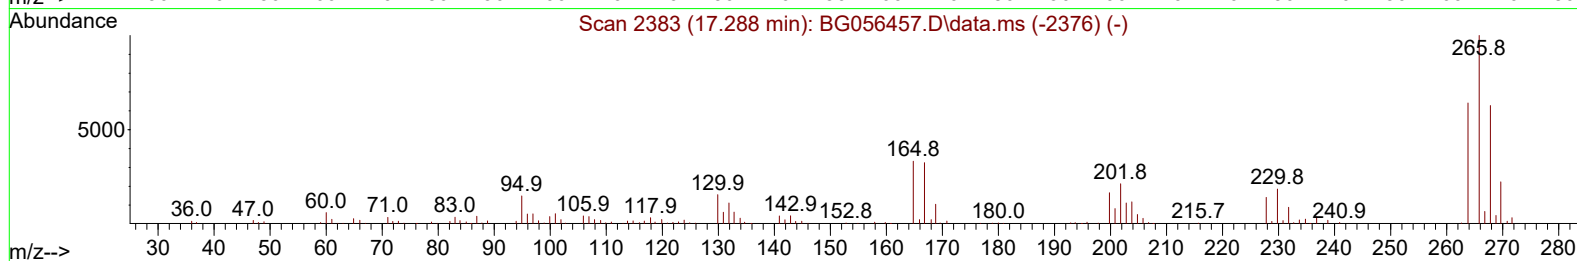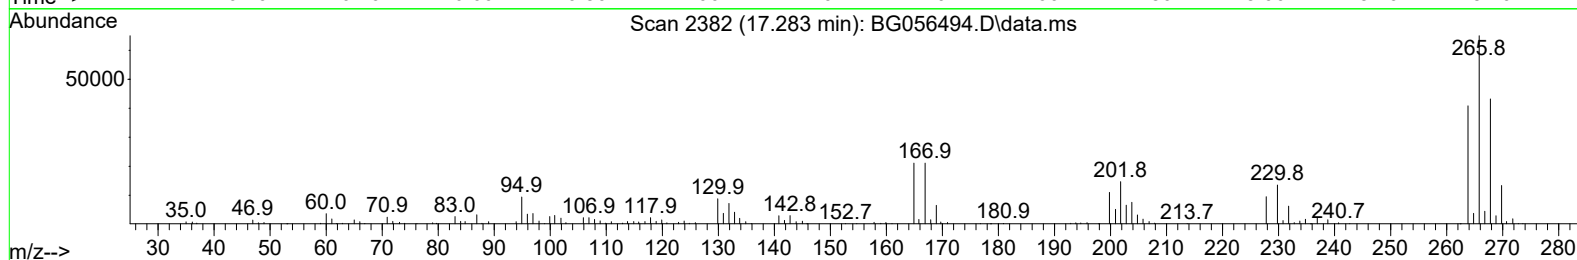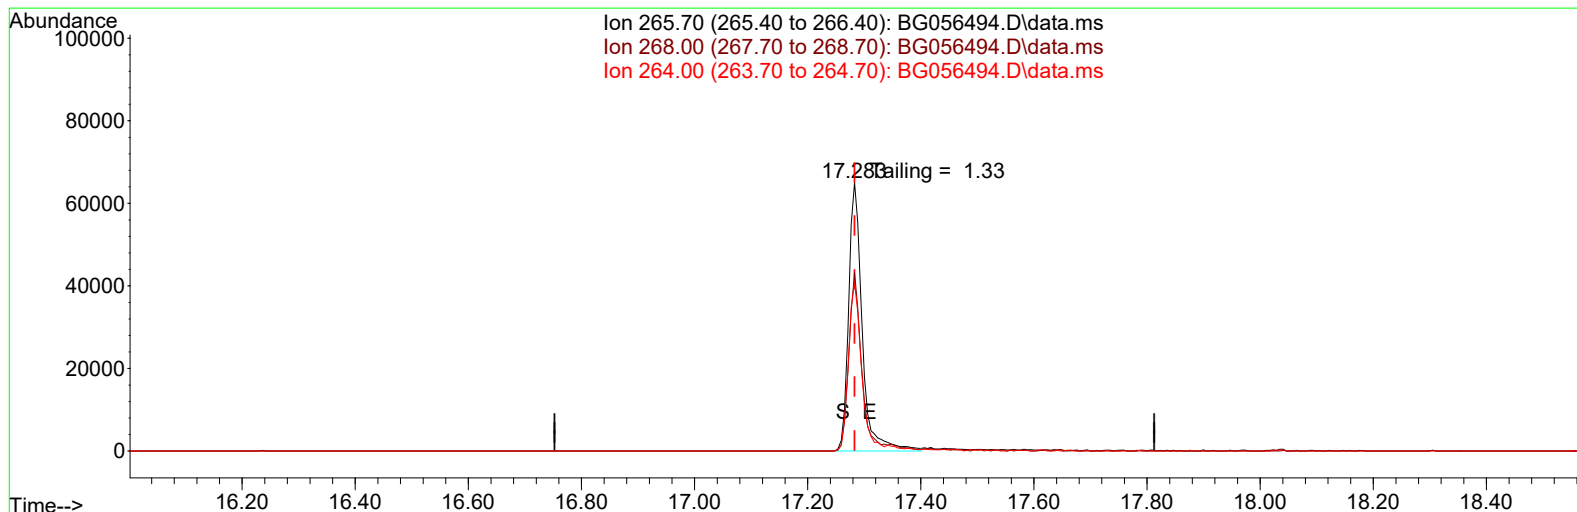

TIC: BG056494.D\data.ms

**(70) Pentachlorophenol (C)**

17.283min (+ 0.000) 243347.72 ng




response 108927

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.80  | 66.45  |
| 264.00 | 64.20  | 62.78  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020123\  
Data File : BG056494.D  
Acq On : 1 Feb 2023 9:01  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Feb 02 05:48:23 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG012723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Feb 01 01:15:52 2023  
Response via : Initial Calibration

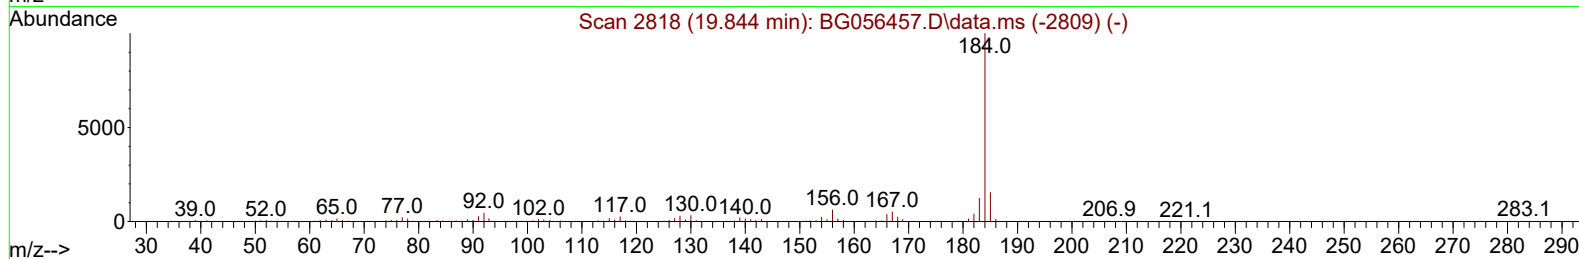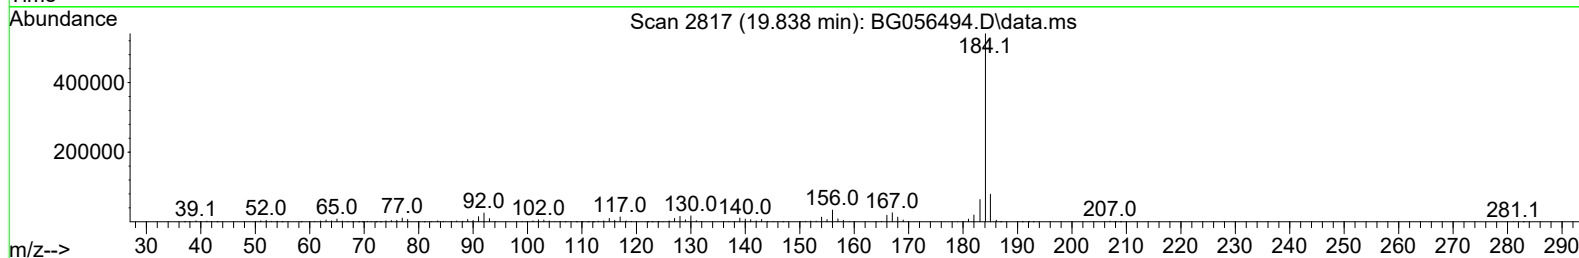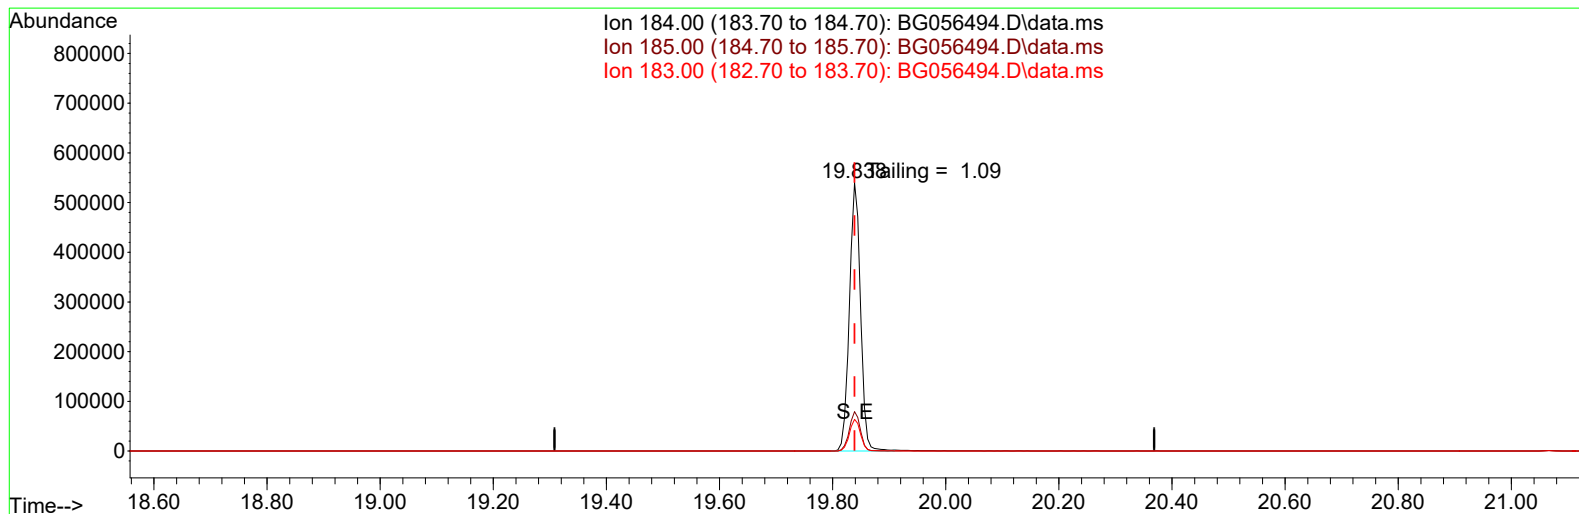

TIC: BG056494.D\data.ms

(77) Benzidine

19.838min (+ 0.000) 0.00 ng

response 742023

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.40  | 14.70  |
| 183.00 | 12.30  | 11.84  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/1/2023      | BNA_G            | <u>BG056494.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 368668           | 21.066             |
| DDD           | 9096             | 20.62              |
| DDE           | 261              | 20.115             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 9357          | 378025           | 2.48               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP