
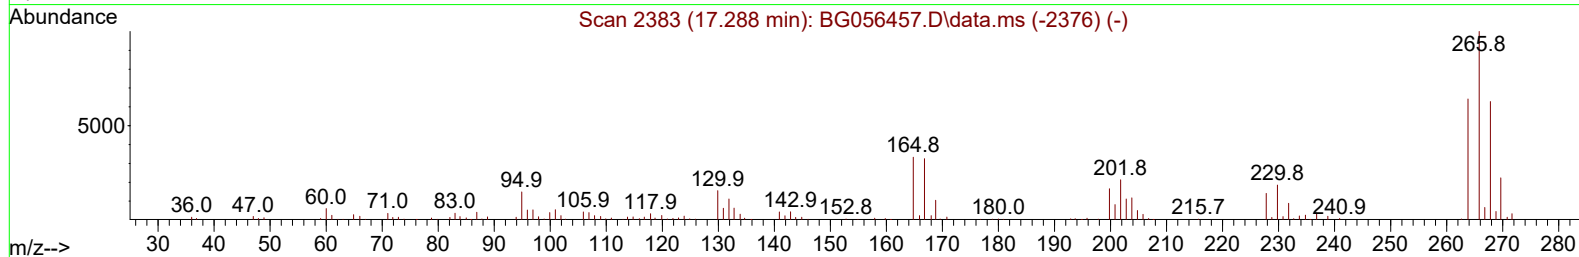
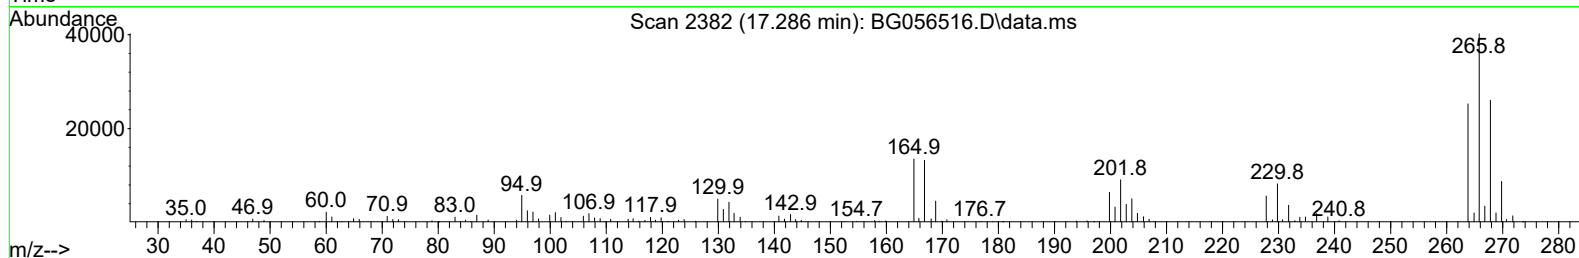


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056516.D
Acq On : 2 Feb 2023 16:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 07:03:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

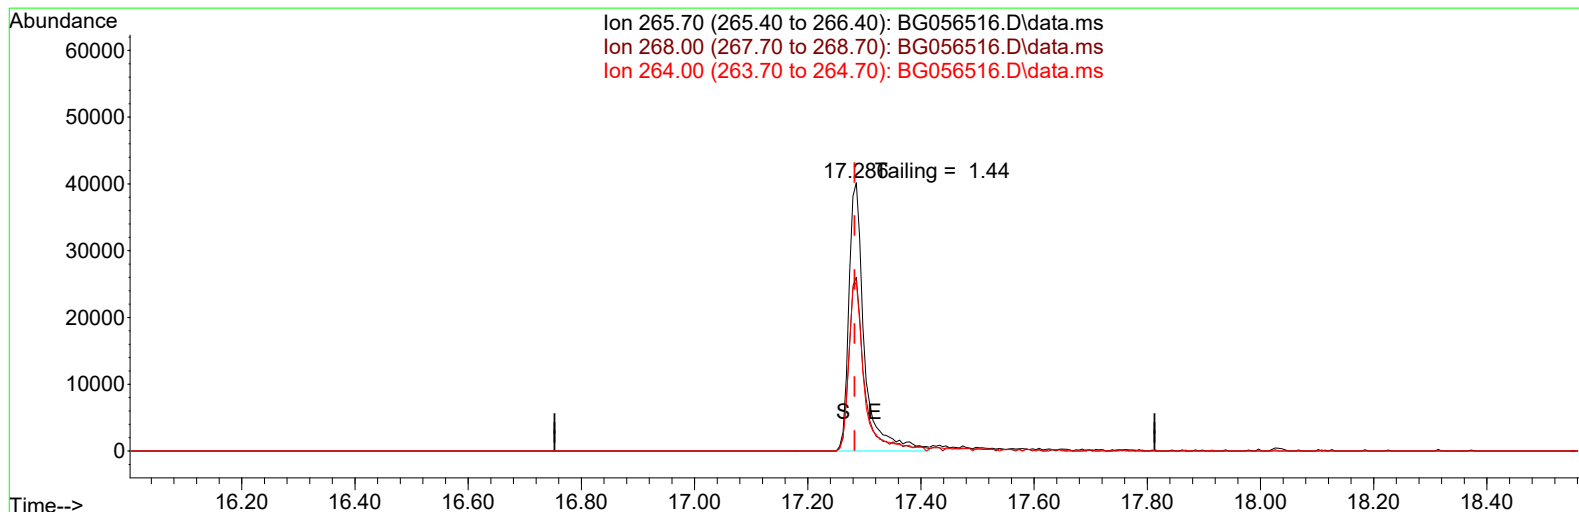

TIC: BG056516.D\data.ms

(70) **Pentachlorophenol (C)**




17.286min (+ 0.003) 23246.88 ng

response 77073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	64.75
264.00	64.20	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056516.D
Acq On : 2 Feb 2023 16:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 07:03:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

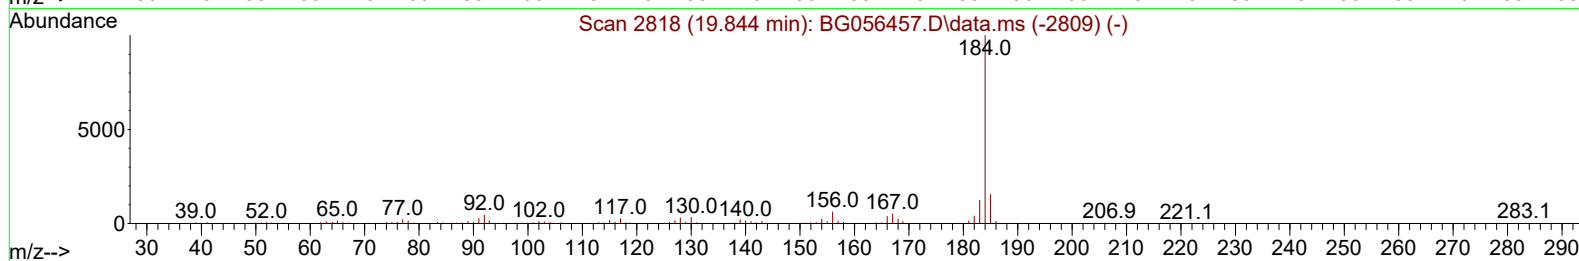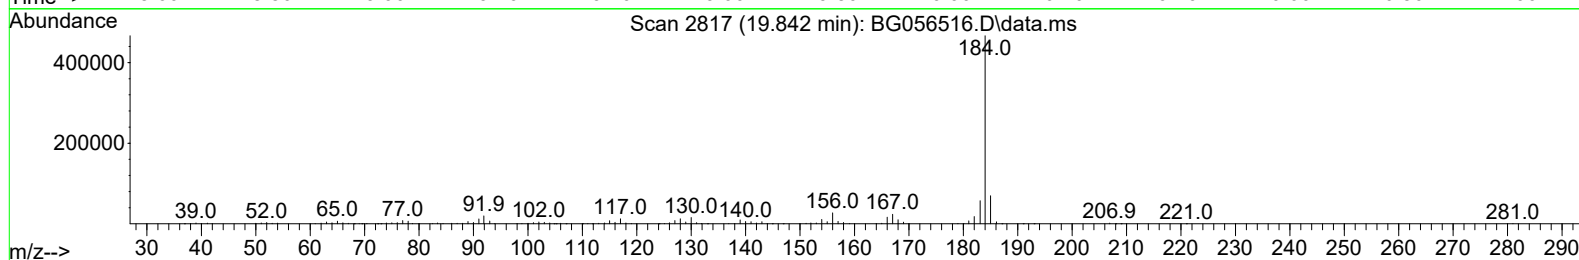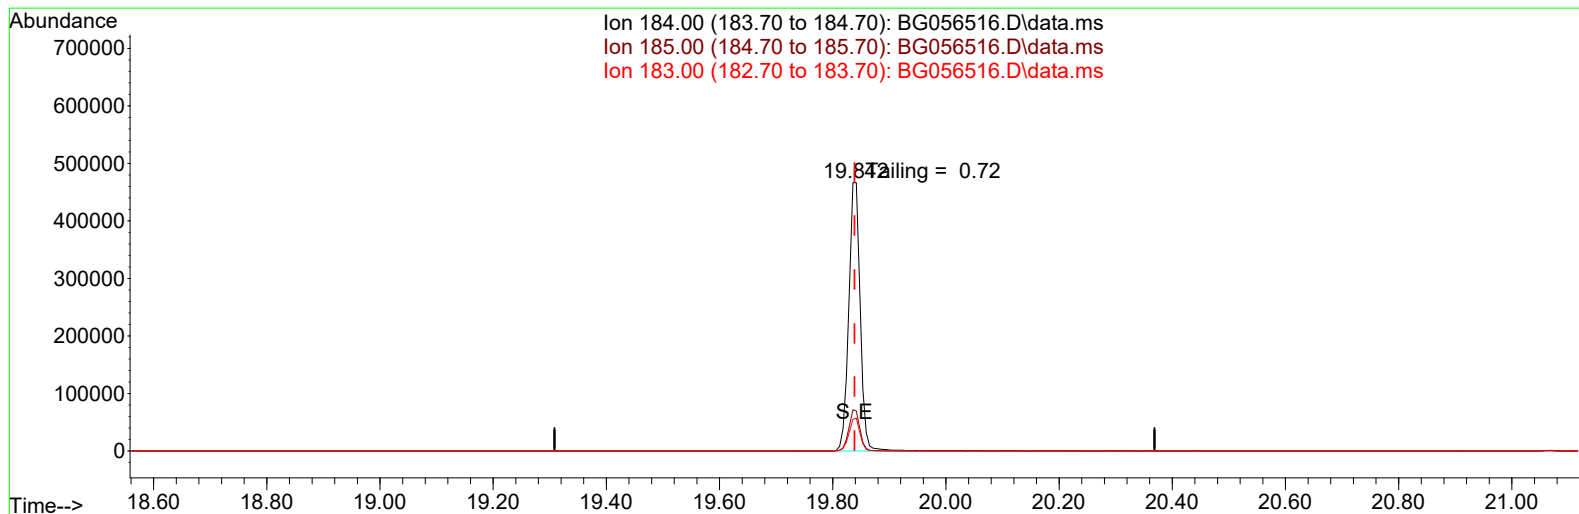

TIC: BG056516.D\data.ms

(77) Benzidine**19.842min (+ 0.003) 0.00 ng****response 655682**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.93
183.00	12.30	12.30
0.00	0.00	0.00