

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
 Data File : BG056531.D
 Acq On : 3 Feb 2023 2:22
 Operator : CG/JU
 Sample : 01390-01 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 STOCKPILE-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.312	340	344	349	rBV2	10391	15633	2.20%	0.359%
2	5.800	421	427	436	rBV	44237	73761	10.40%	1.694%
3	7.422	697	703	712	rBV	41046	74967	10.57%	1.722%
4	8.279	842	849	857	rBB	166550	274872	38.75%	6.314%
5	9.455	1042	1049	1058	rBB	26247	46685	6.58%	1.072%
6	11.111	1323	1331	1343	rBB	207918	369681	52.11%	8.492%
7	13.520	1735	1741	1749	rBV	98043	146089	20.59%	3.356%
8	14.901	1969	1976	1982	rVB	370537	568563	80.15%	13.060%
9	16.235	2198	2203	2208	rBV2	7225	10423	1.47%	0.239%
10	16.382	2220	2228	2237	rBV3	64644	108414	15.28%	2.490%
11	17.639	2433	2442	2446	rBV	459673	693612	97.78%	15.932%
12	17.680	2446	2449	2454	rVB	44445	61099	8.61%	1.403%
13	17.768	2461	2464	2469	rBV2	12077	18466	2.60%	0.424%
14	18.227	2537	2542	2545	rBV7	6252	12191	1.72%	0.280%
15	18.356	2559	2564	2569	rBV9	7344	15746	2.22%	0.362%
16	18.509	2585	2590	2594	rBV6	10829	24180	3.41%	0.555%
17	18.556	2594	2598	2603	rVB2	16399	24946	3.52%	0.573%
18	18.609	2603	2607	2609	rBV5	5736	8356	1.18%	0.192%
19	19.672	2784	2788	2793	rBV	87799	121777	17.17%	2.797%
20	20.036	2846	2850	2854	rVB	79726	108485	15.29%	2.492%
21	20.213	2876	2880	2885	rBV	161807	203171	28.64%	4.667%
22	21.928	3167	3172	3178	rVB	416526	709374	100.00%	16.294%
23	25.365	3750	3757	3769	rVB	219343	662985	93.46%	15.229%




Sum of corrected areas: 4353476

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056531.D
Acq On : 3 Feb 2023 2:22
Operator : CG/JU
Sample : 01390-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
STOCKPILE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

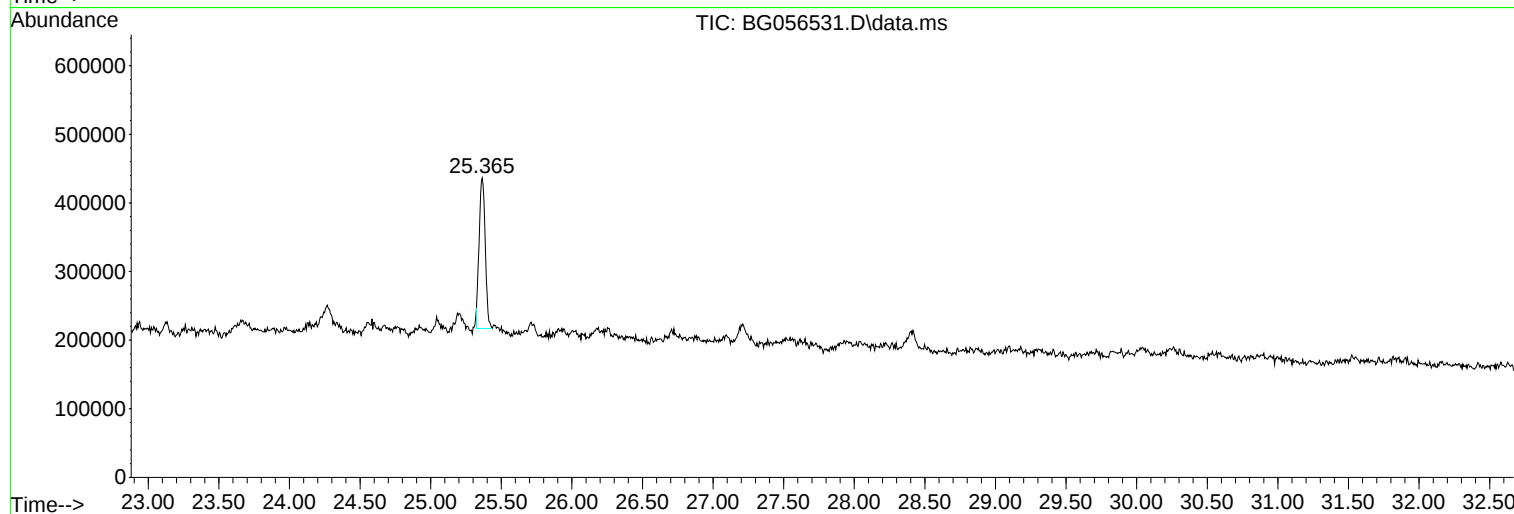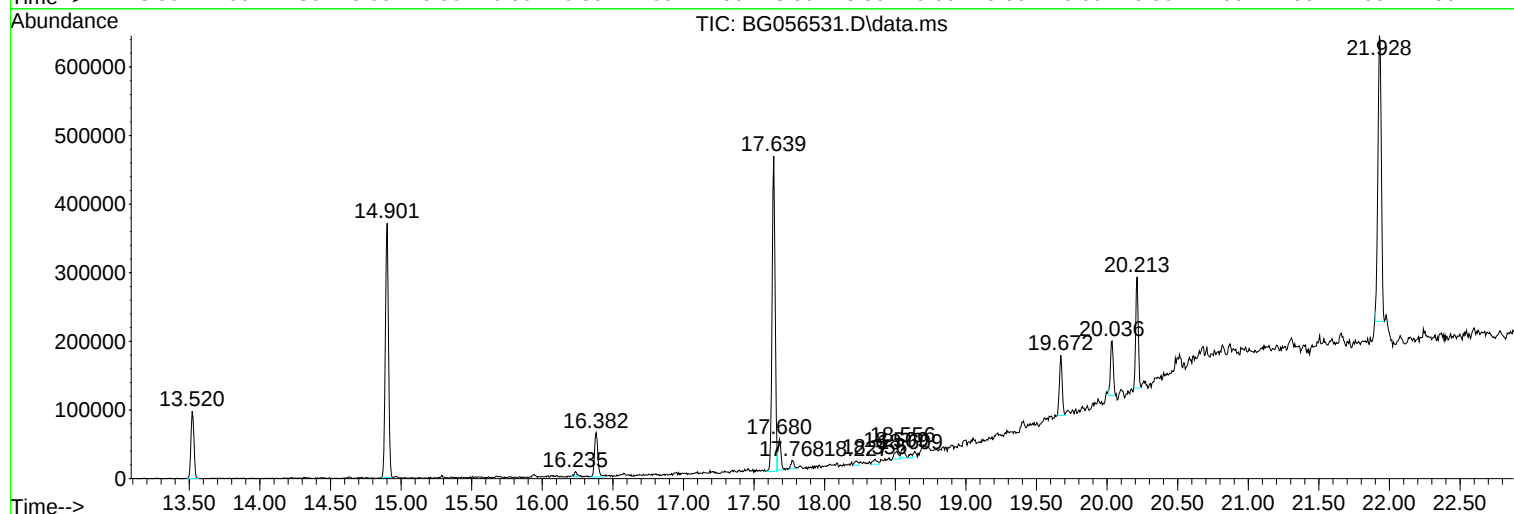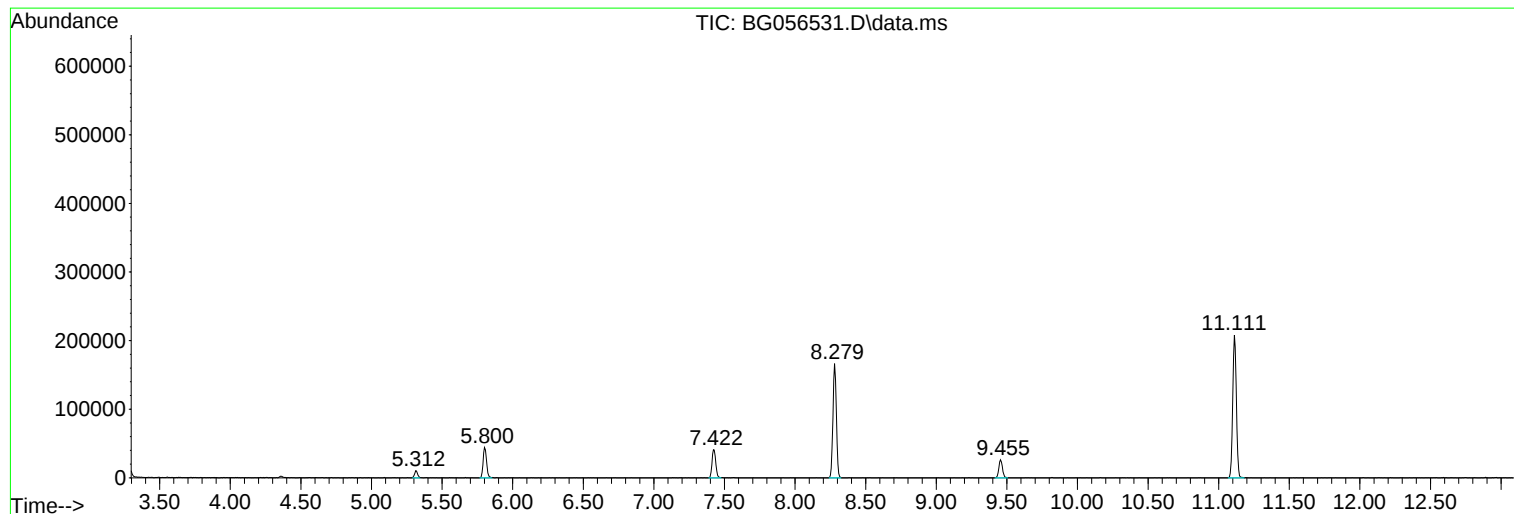

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056531.D
Acq On : 3 Feb 2023 2:22
Operator : CG/JU
Sample : 01390-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
STOCKPILE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056531.D
Acq On : 3 Feb 2023 2:22
Operator : CG/JU
Sample : 01390-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
STOCKPILE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------