


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056507.D
Acq On : 2 Feb 2023 9:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 01 01:15:52 2023

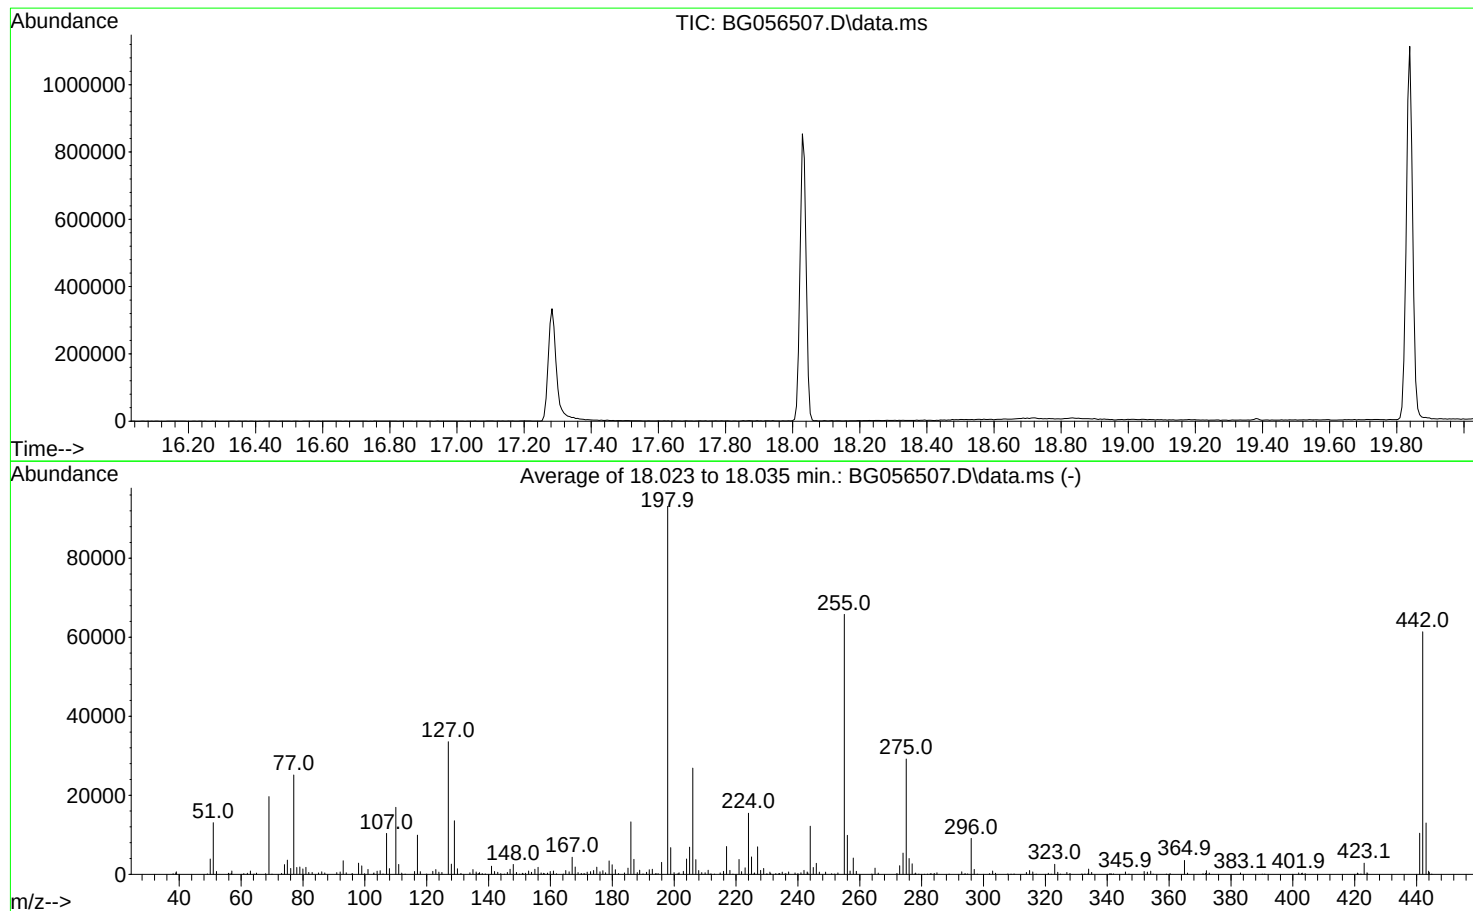




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.0	13065	PASS
68	69	0.00	2	0.7	129	PASS
69	198	0.00	100	21.1	19651	PASS
70	69	0.00	2	0.3	62	PASS
127	198	10	80	36.1	33571	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93117	PASS
199	198	5	9	7.2	6739	PASS
275	198	10	60	31.3	29176	PASS
365	198	1	100	3.8	3524	PASS
441	198	0.01	100	11.2	10409	PASS
442	442	50	100	100.0	61376	PASS
443	442	15	24	21.1	12970	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056507.D
Acq On : 2 Feb 2023 9:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 03 07:09:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

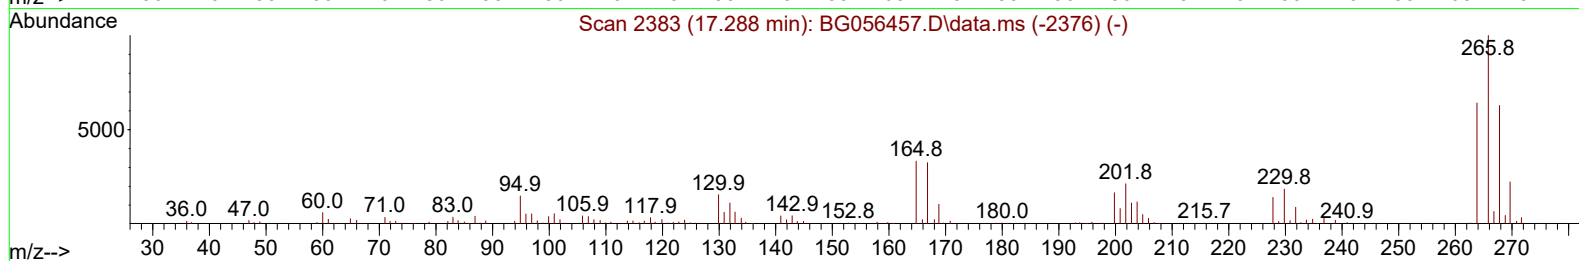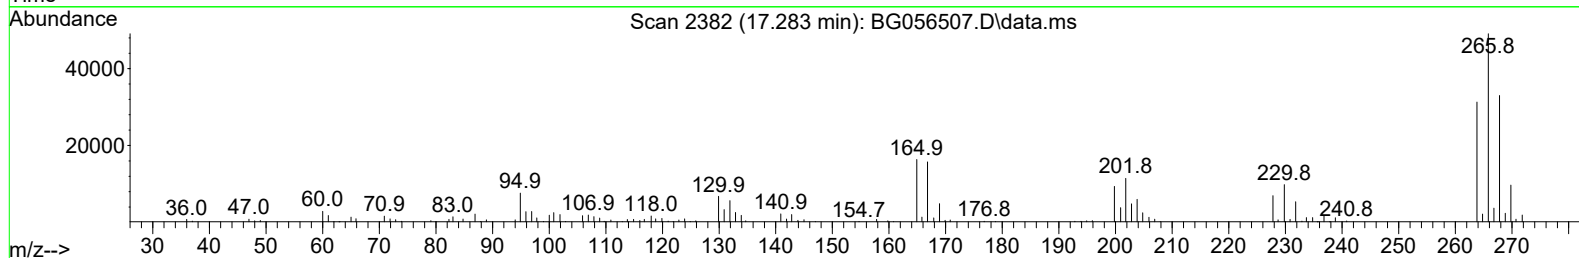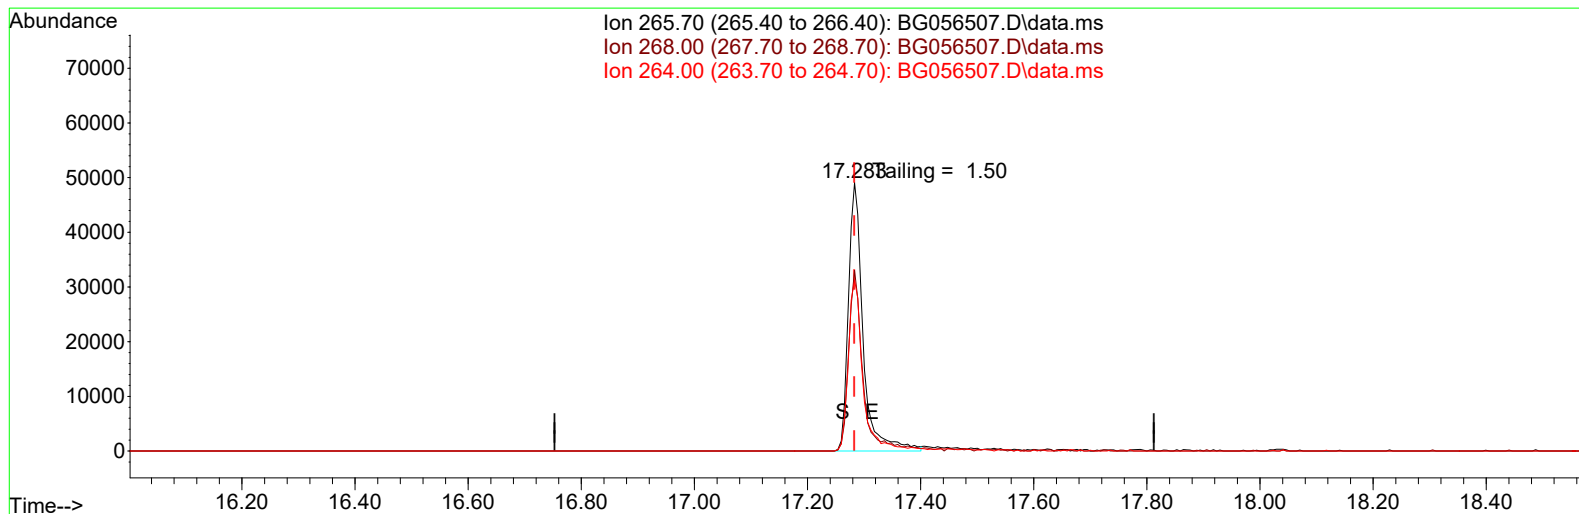

TIC: BG056507.D\data.ms

(70) Pentachlorophenol (C)

17.283min (+ 0.000) 19287.56 ng




response 88676

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	67.26
264.00	64.20	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056507.D
Acq On : 2 Feb 2023 9:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 03 07:09:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

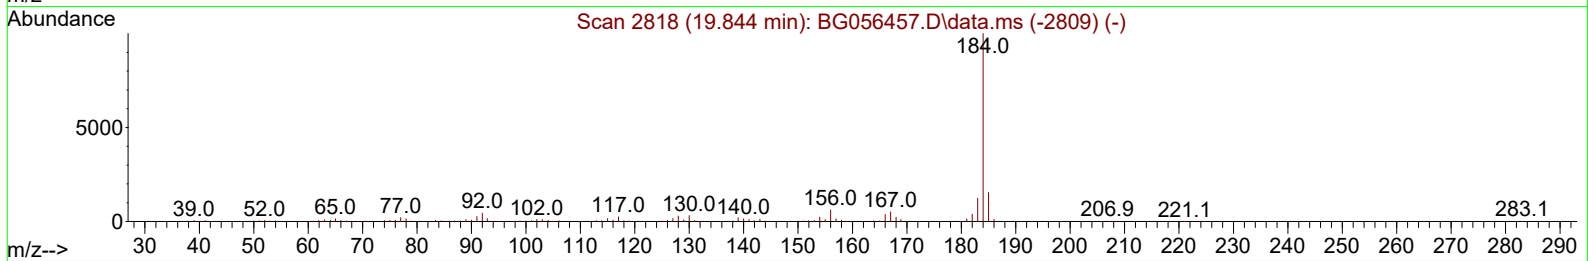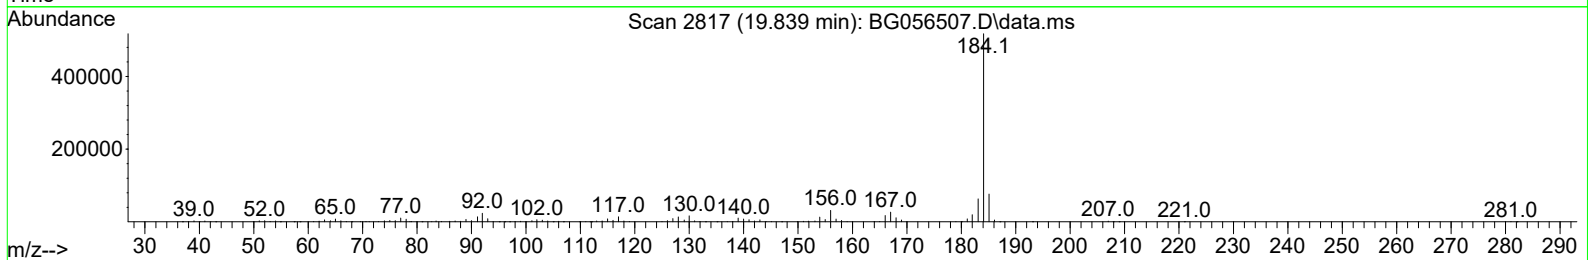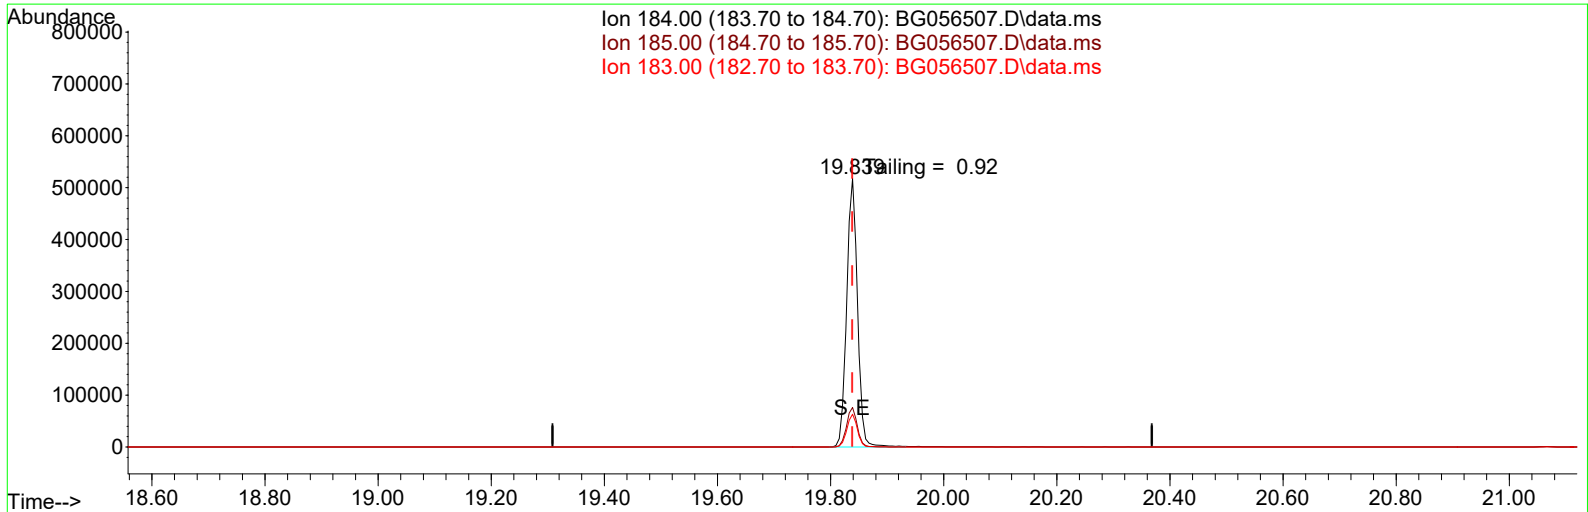

TIC: BG056507.D\data.ms

(77) Benzidine

19.839min (+ 0.000) 410555.52 ng

response 688828

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.72
183.00	12.30	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/2/2023	BNA_G	<u>BG056507.D</u>
Compound Name	Response	Retention Time
DDT	344787	21.067
DDD	8790	20.614
DDE	332	20.121
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9122	353909	2.58

Instrument :
BNA_G
ClientSampleId :
DFTPP