


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056516.D
Acq On : 2 Feb 2023 16:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 01 01:15:52 2023

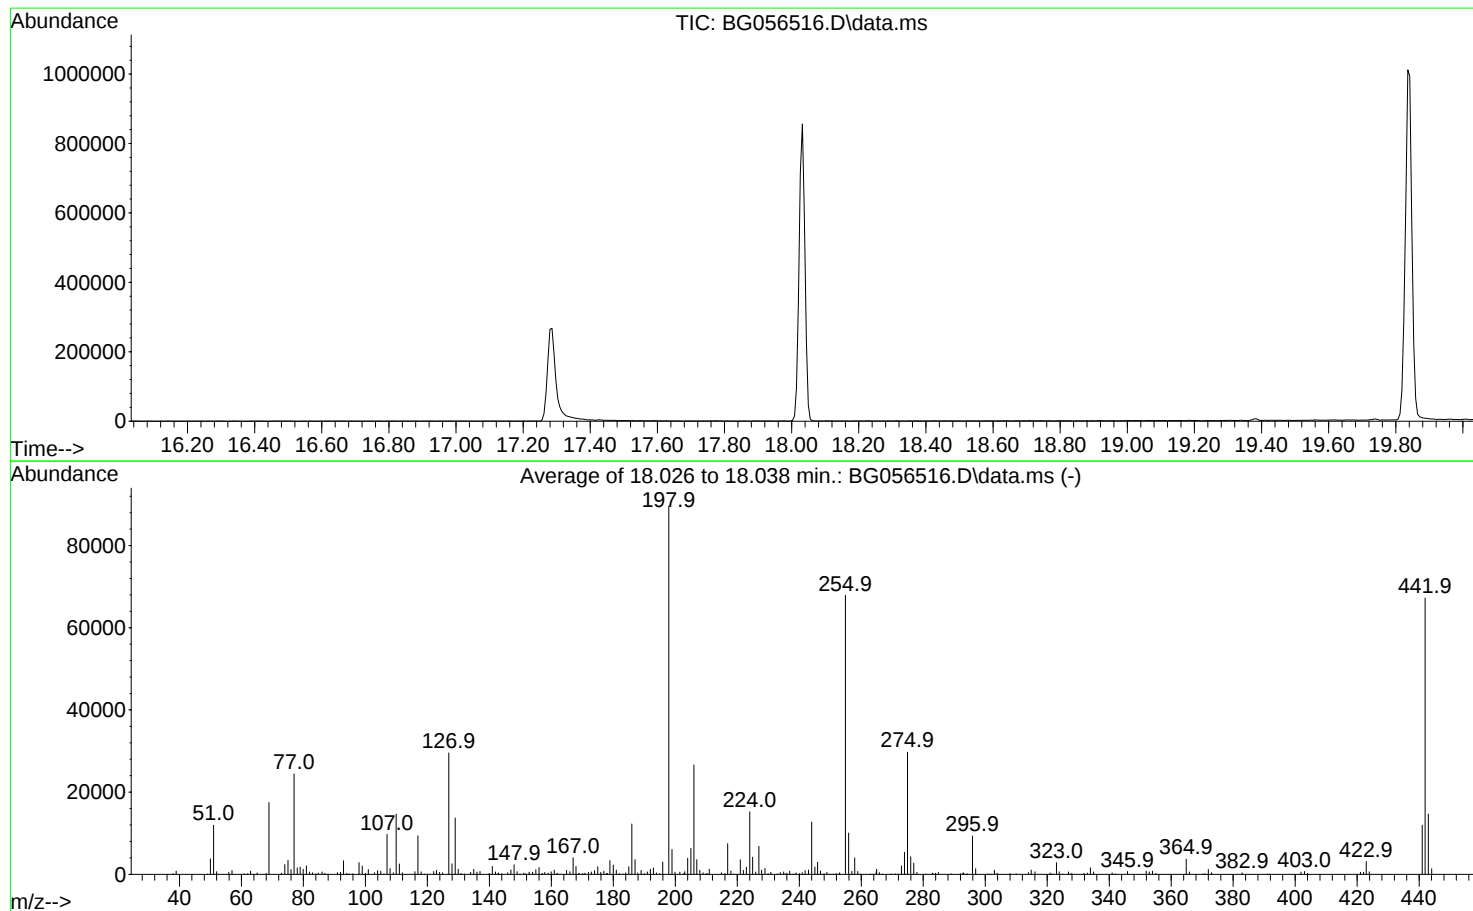




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	13.3	11925	PASS
68	69	0.00	2	1.6	275	PASS
69	198	0.00	100	19.5	17455	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.0	29528	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89525	PASS
199	198	5	9	6.7	6014	PASS
275	198	10	60	33.2	29696	PASS
365	198	1	100	4.1	3670	PASS
441	198	0.01	100	13.4	11952	PASS
442	442	50	100	100.0	67235	PASS
443	442	15	24	21.8	14650	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056516.D
Acq On : 2 Feb 2023 16:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 03 07:03:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

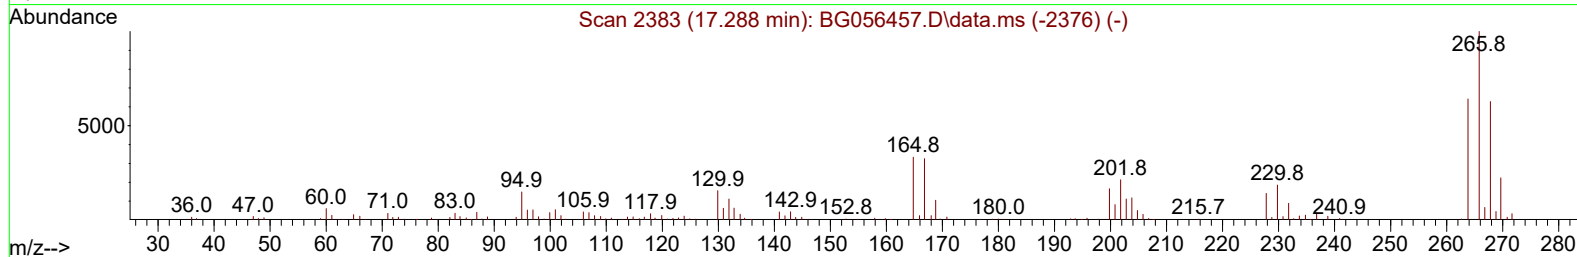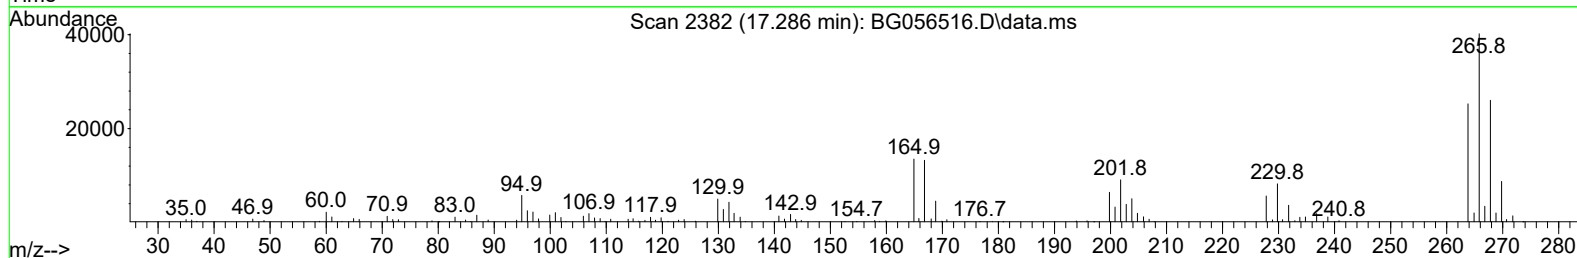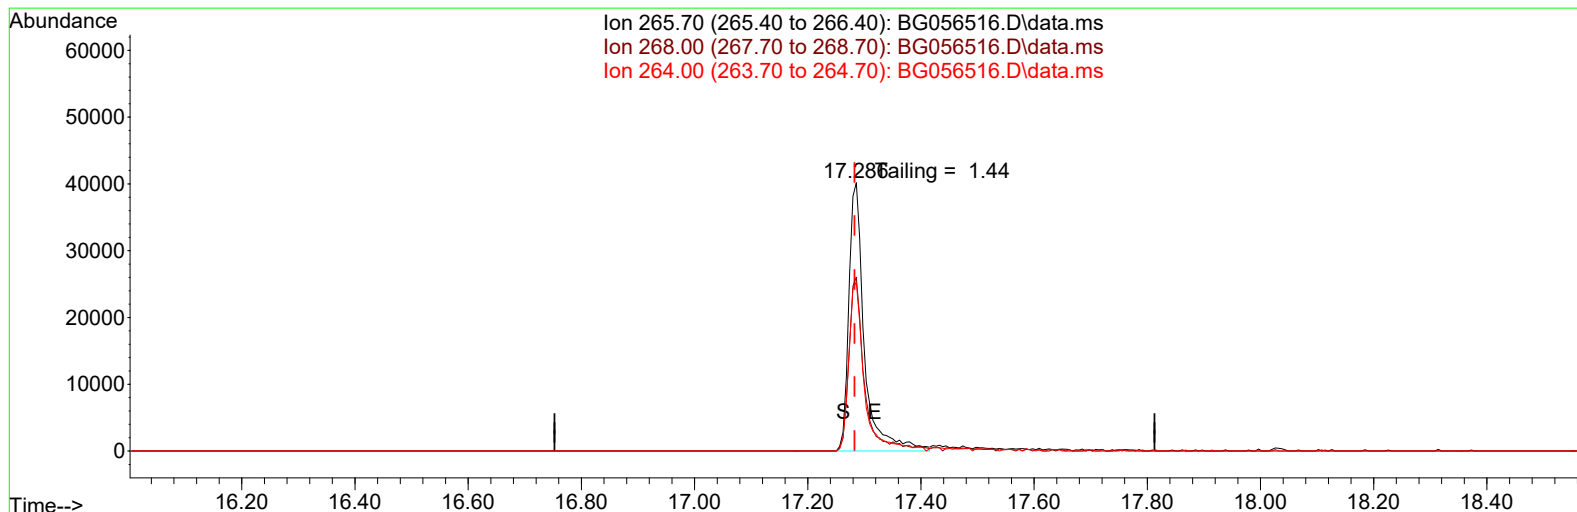

TIC: BG056516.D\data.ms

(70) **Pentachlorophenol (C)**

17.286min (+ 0.003) 23246.88 ng




response 77073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	64.75
264.00	64.20	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020223\
Data File : BG056516.D
Acq On : 2 Feb 2023 16:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 03 07:03:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

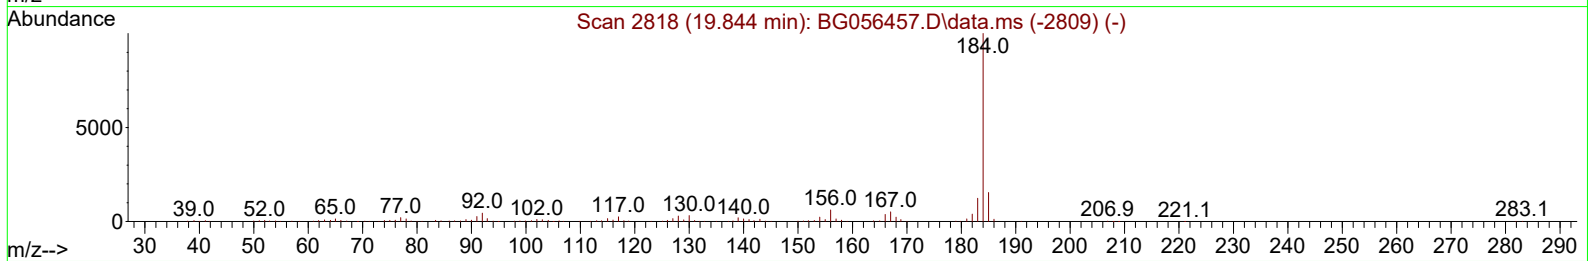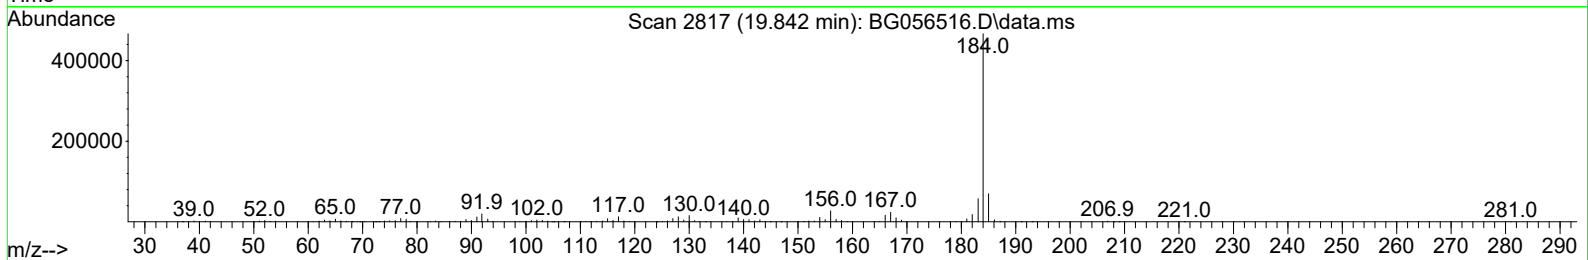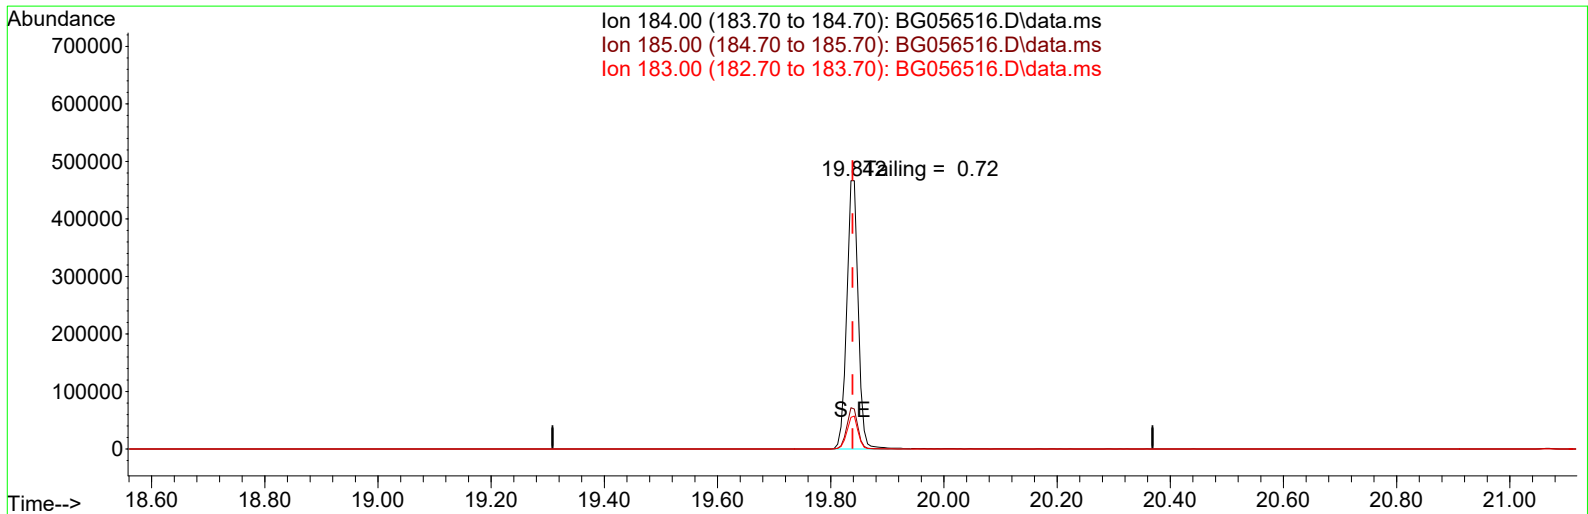

TIC: BG056516.D\data.ms

(77) Benzidine

19.842min (+ 0.003) 0.00 ng

response 655682

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.93
183.00	12.30	12.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/2/2023	BNA_G	<u>BG056516.D</u>
Compound Name	Response	Retention Time
DDT	334899	21.07
DDD	10415	20.617
DDE	417	20.106
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10832	345731	3.13

Instrument :
BNA_G
ClientSampleId :
DFTPP